

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
 Data File : BM006422.D
 Acq On : 14 Jul 2016 21:45
 Operator : UM/SJ
 Sample : H3990-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ64

Quant Time: Jul 15 05:02:09 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 04:34:07 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	111218	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	464079	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	283888	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	689382	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	874378	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	945317	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	5825	2.21	ng/uL	0.00
5) Phenol-d5	6.80	99	277977	30.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	172824	31.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	225121	30.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	228492	31.55	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	109733	31.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	128678	32.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	223352	29.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	299088	38.13	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	768396	33.07	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	910938	31.71	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	127156	31.50	ng/ul	0.00
57) Fluorene-d10	15.27	176	659958	31.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	105648	26.49	ng/ul	0.00
70) Anthracene-d10	17.12	188	1084554	33.28	ng/ul	0.00
76) Pyrene-d10	19.42	212	1292934	32.61	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1531055	35.42	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.73	163	272489	11.56	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
Data File : BM006422.D
Acq On : 14 Jul 2016 21:45
Operator : UM/SJ
Sample : H3990-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ64

Quant Time: Jul 15 05:02:09 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 04:34:07 2016
Response via : Initial Calibration

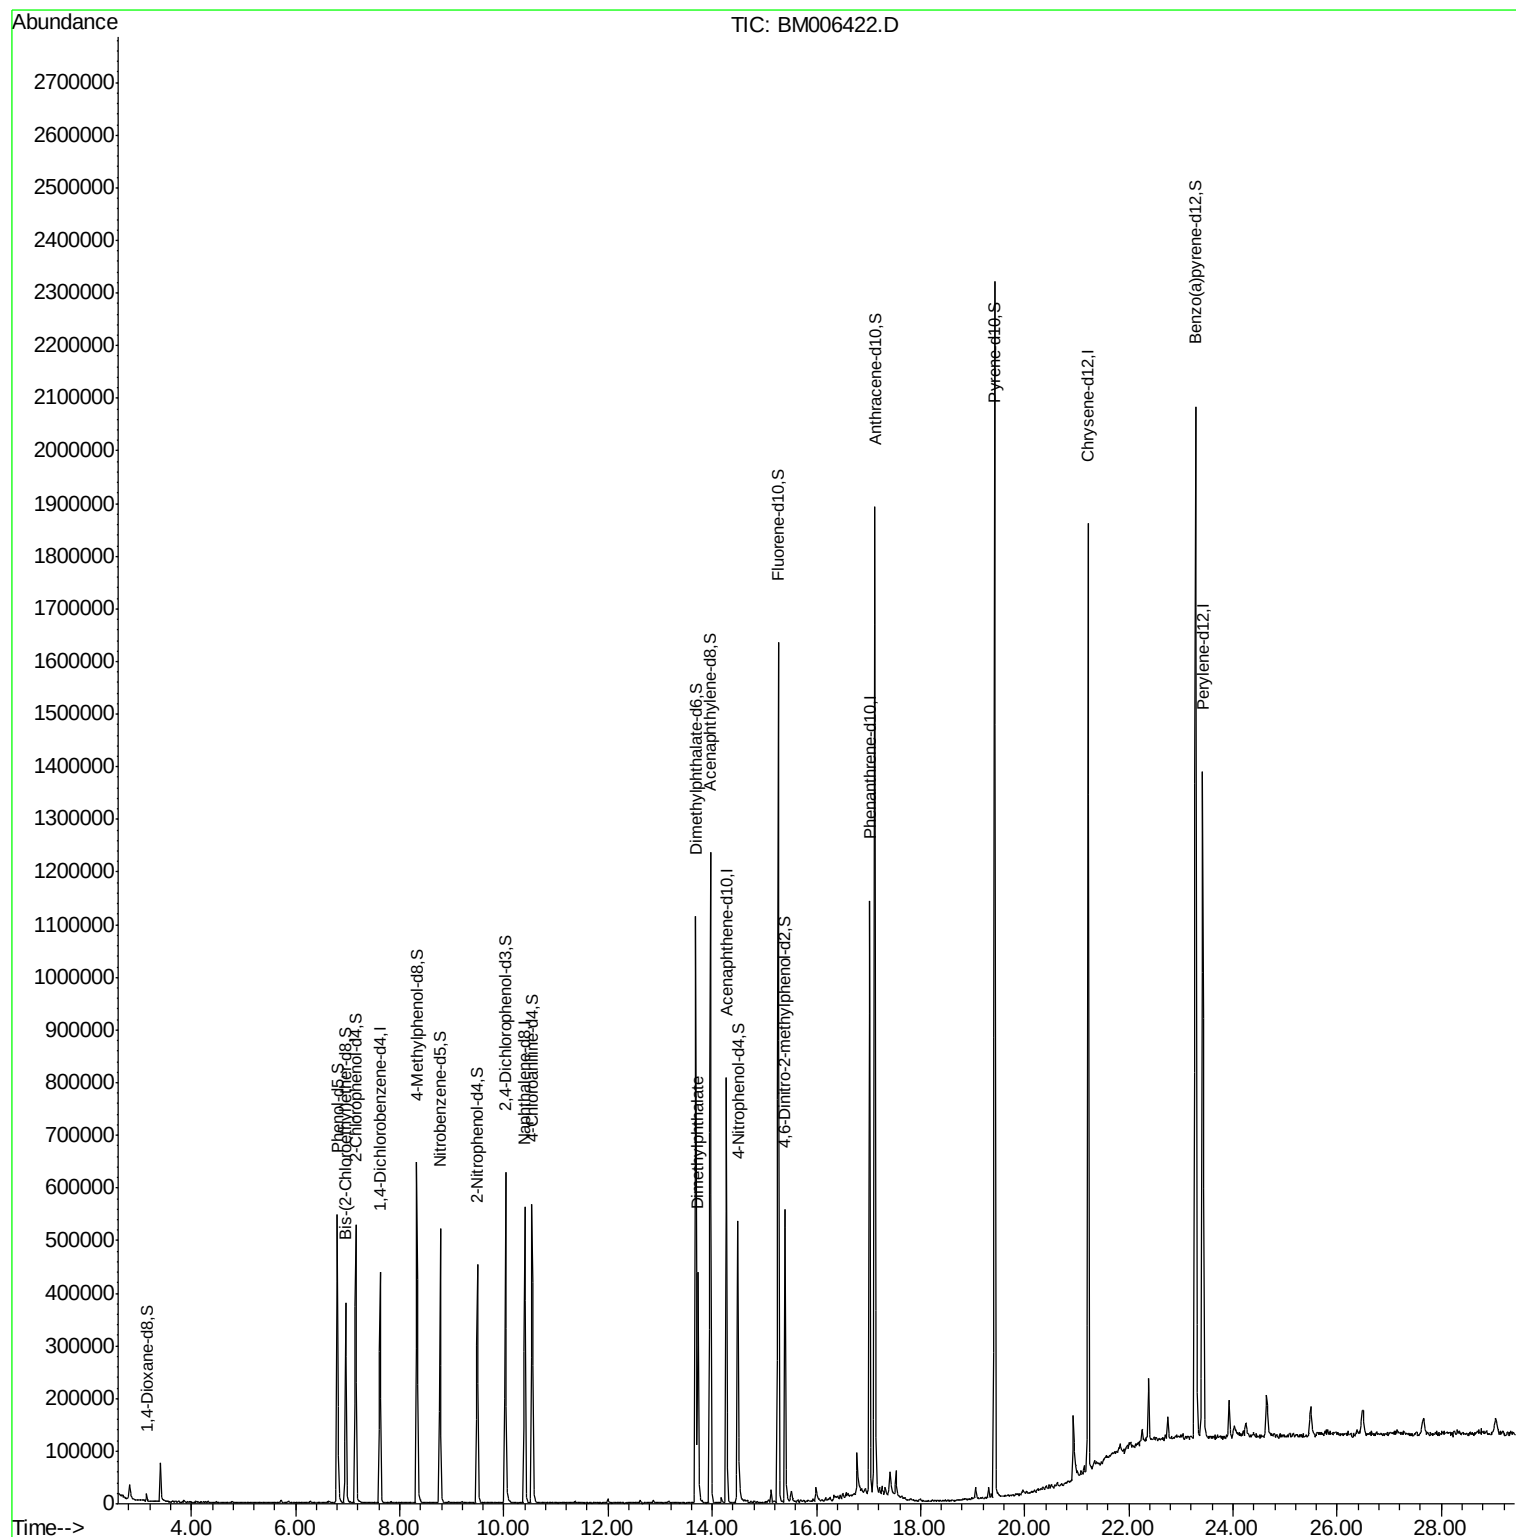

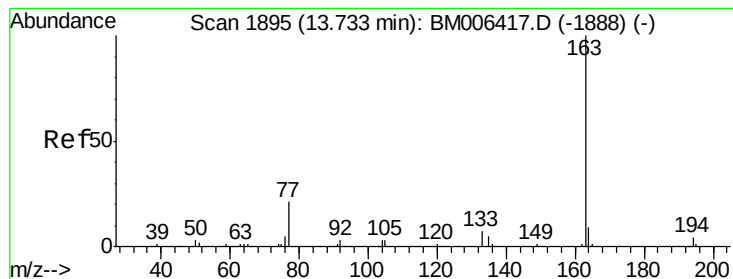

#44

Dimethylphthalate

Concen: 11.56 ng/ul

RT: 13.73 min Scan# 1895

Delta R.T. 0.00 min

Lab File: BM006422.D


Acq: 14 Jul 2016 21:45

Instrument :

BNA_M

ClientSampleId :

BDJ64

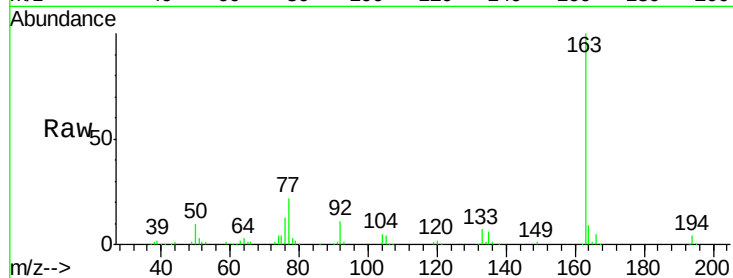

Tot Ion:163 Resp: 272489

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 9.4 7.8 11.8

