

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
 Data File : BM006425.D
 Acq On : 15 Jul 2016 03:51
 Operator : UM/SJ
 Sample : H3990-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ68

Quant Time: Jul 15 05:16:22 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 04:34:07 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	129333	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	553905	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	329113	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	798500	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	1000397	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1062792	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	8495	2.77	ng/uL	0.00
5) Phenol-d5	6.80	99	397848	37.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	242631	37.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	309194	36.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	320019	38.00	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	155196	36.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	178779	37.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	310090	34.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	412808	44.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	989255	36.73	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1207560	36.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	187809	40.14	ng/ul	0.00
57) Fluorene-d10	15.27	176	850291	35.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	156868	33.96	ng/ul	0.00
70) Anthracene-d10	17.12	188	1356861	35.95	ng/ul	0.00
76) Pyrene-d10	19.42	212	1595142	35.17	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1854772	38.16	ng/ul	0.00

Target Compounds


						Ovalue
6) Phenol	6.83	94	11250	1.01	ng/ul#	88
44) Dimethylphthalate	13.73	163	300781	11.01	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
Data File : BM006425.D
Acq On : 15 Jul 2016 03:51
Operator : UM/SJ
Sample : H3990-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ68

Quant Time: Jul 15 05:16:22 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 04:34:07 2016
Response via : Initial Calibration

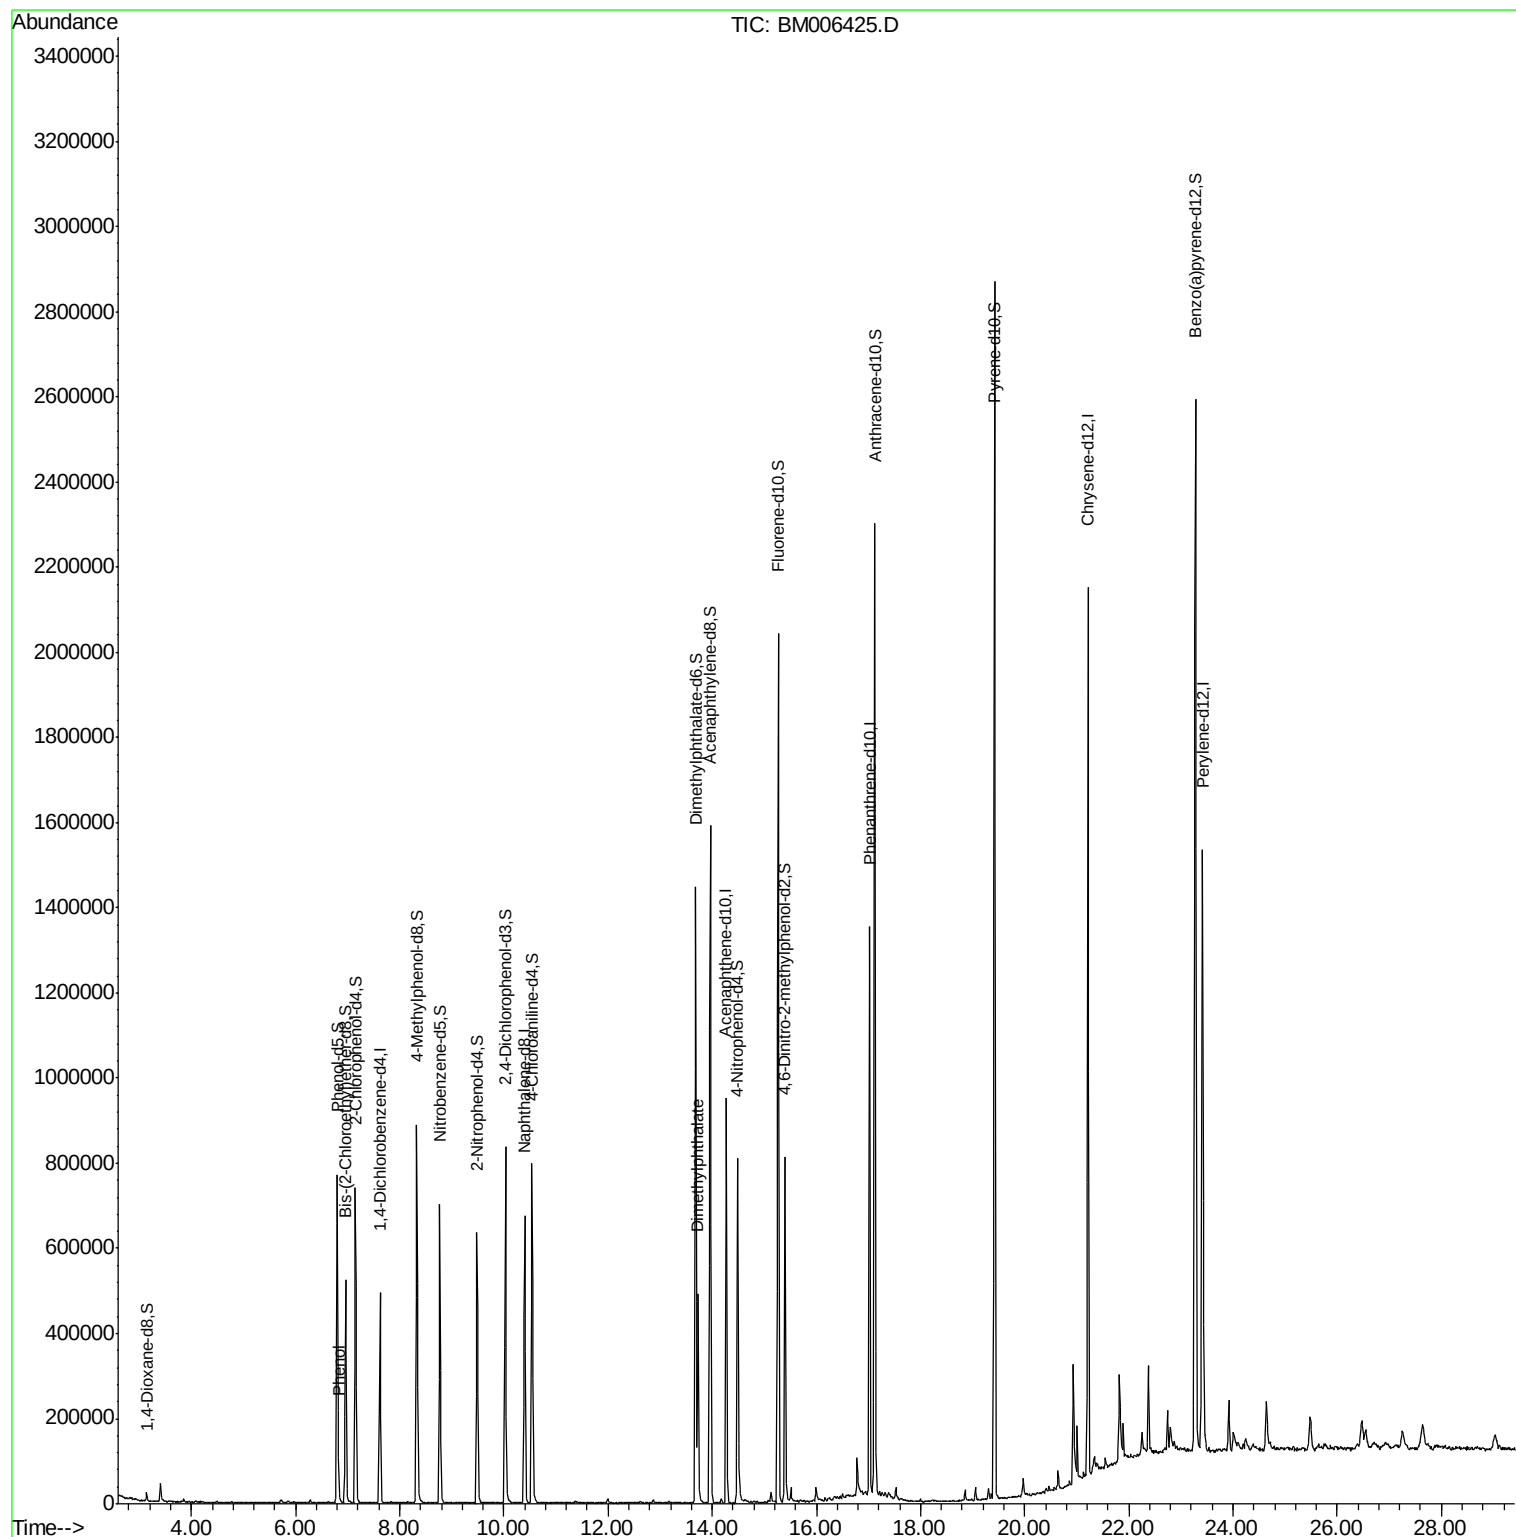

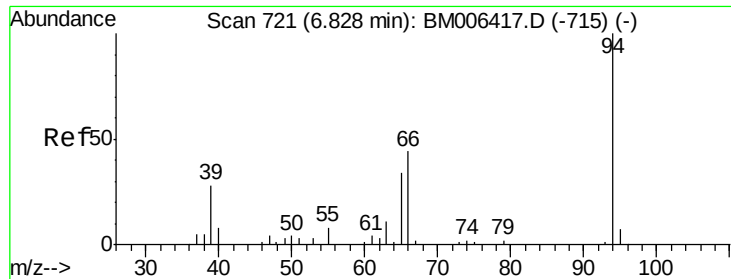

#6

Phenol

Concen: 1.01 ng/ul

RT: 6.83 min Scan# 721

Delta R.T. -0.00 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51

Instrument :

BNA_M

ClientSampled :

BDJ68


Tot Ion: 94 Resp: 11250

Ion Ratio Lower Upper

94 100

65 36.3 25.8 38.8




66 54.3 35.7 53.5#

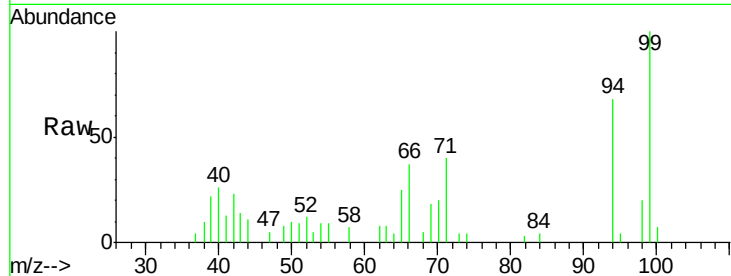

Abundance Ion 94.00 (93.70 to 94.70): BM006417.D (-715) (-)

Ion 65.00 (64.70 to 65.70): BM006417.D (-715) (-)

Ion 66.00 (65.70 to 66.70): BM006417.D (-715) (-)

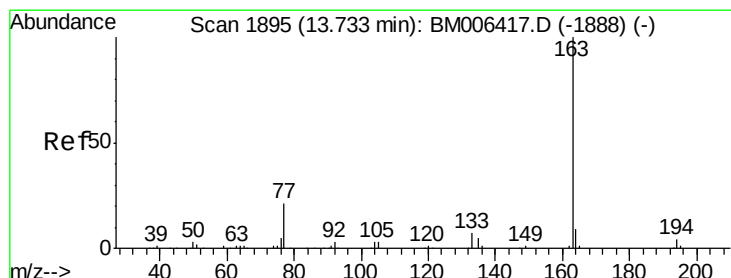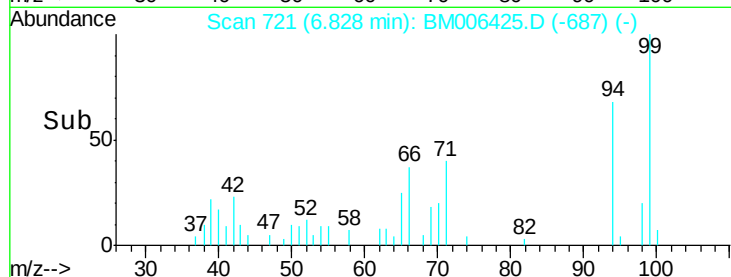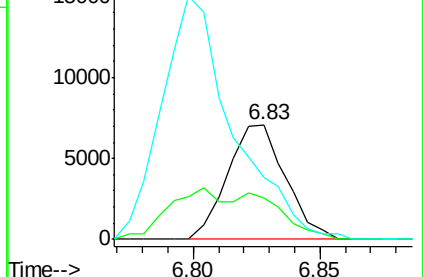

#44

Dimethylphthalate

Concen: 11.01 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BM006425.D

Acq: 15 Jul 2016 03:51


Tgt Ion:163 Resp: 300781

Ion Ratio Lower Upper

163 100

194 3.6 3.4 5.0

164 10.1 7.8 11.8

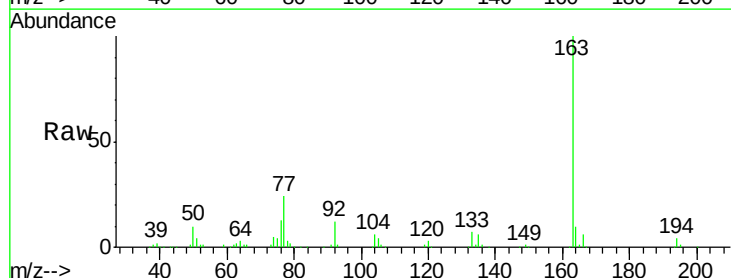

Abundance Ion 163.00 (162.70 to 163.70): BM006417.D (-1888) (-)

Ion 194.00 (193.70 to 194.70): BM006417.D (-1888) (-)

Ion 164.00 (163.70 to 164.70): BM006417.D (-1888) (-)

