

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
 Data File : BM006430.D
 Acq On : 15 Jul 2016 06:53
 Operator : UM/SJ
 Sample : H3990-21
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ74

Quant Time: Jul 15 08:09:19 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 04:34:07 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	125427	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	540042	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	320420	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	766080	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	955089	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	1014774	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	6564	2.20	ng/uL	0.00
5) Phenol-d5	6.80	99	268529	26.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	168539	27.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	215070	25.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	214950	26.32	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	104244	25.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	118439	25.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	206386	23.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	270580	29.65	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	689984	26.31	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	846423	26.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	113477	24.91	ng/ul	0.00
57) Fluorene-d10	15.27	176	609122	26.13	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	95349	21.52	ng/ul	0.00
70) Anthracene-d10	17.12	188	950052	26.24	ng/ul	0.00
76) Pyrene-d10	19.42	212	1146367	26.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1305244	28.13	ng/ul	0.00

Target Compounds


						Ovalue
44) Dimethylphthalate	13.73	163	201424	7.57	ng/ul	100
74) Fluoranthene	19.09	202	76730	1.57	ng/ul	98
77) Pyrene	19.45	202	72462	1.27	ng/ul	99
80) Benzo(a)anthracene	21.20	228	62652	1.07	ng/ul	95
85) Benzo(b)fluoranthene	22.76	252	77529	1.28	ng/ul	98
88) Benzo(a)pyrene	23.32	252	64551	1.11	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
Data File : BM006430.D
Acq On : 15 Jul 2016 06:53
Operator : UM/SJ
Sample : H3990-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ74

Quant Time: Jul 15 08:09:19 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 04:34:07 2016
Response via : Initial Calibration

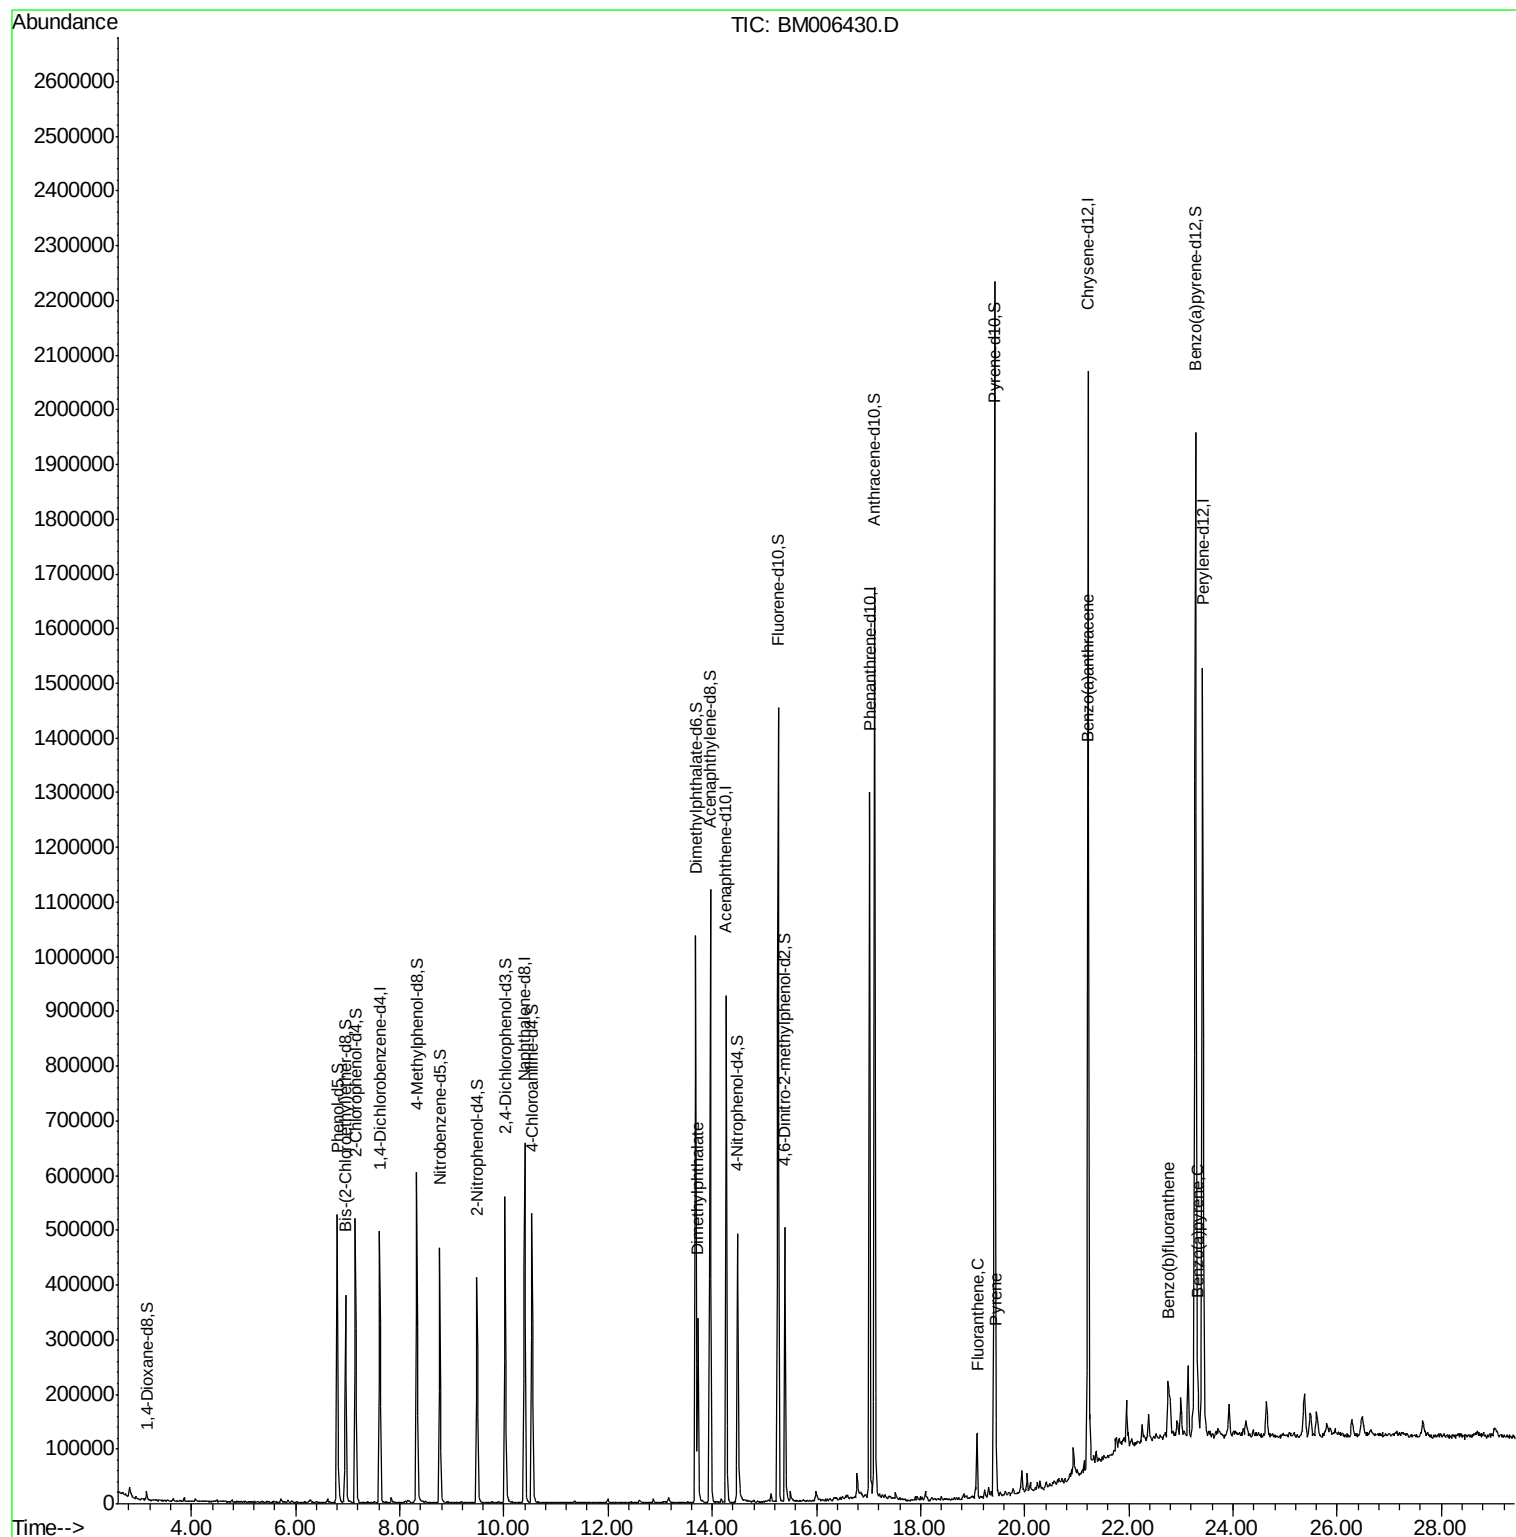


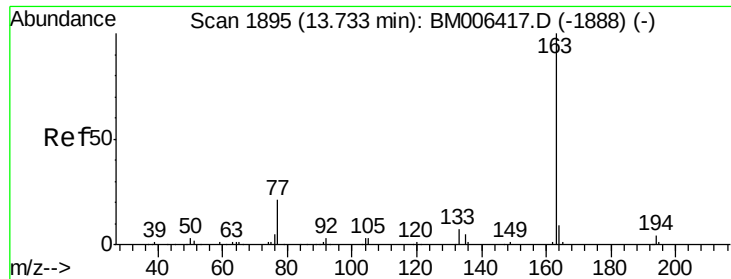




#44
Dimethylphthalate
Concen: 7.57 ng/ul
RT: 13.73 min Scan# 1894
Delta R.T. -0.01 min
Lab File: BM006430.D
Acq: 15 Jul 2016 06:53

Instrument :
BNA_M
ClientSampleId :
BDJ74

Tot Ion:163 Resp: 201424
Ion Ratio Lower Upper
163 100
194 3.8 3.4 5.0
164 9.7 7.8 11.8

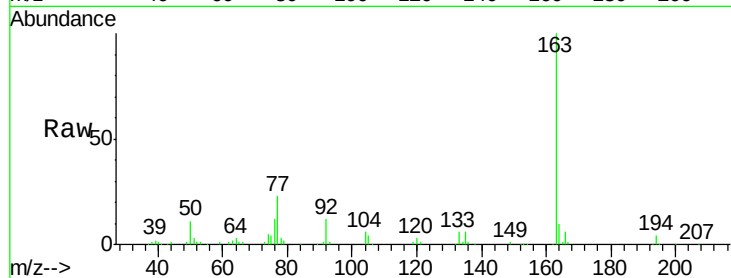


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

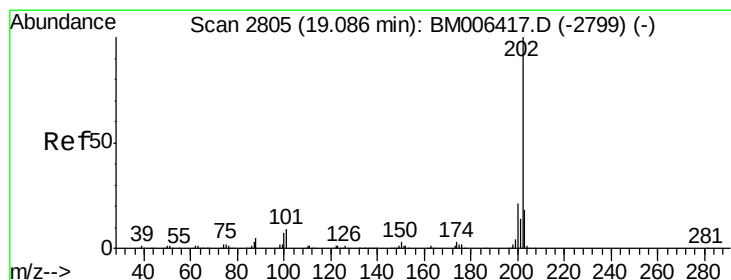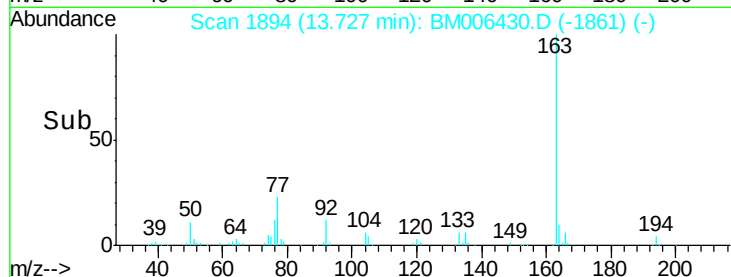
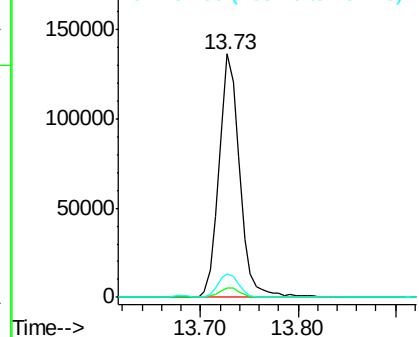



#74
Fluoranthene
Concen: 1.57 ng/ul
RT: 19.09 min Scan# 2805
Delta R.T. 0.00 min
Lab File: BM006430.D
Acq: 15 Jul 2016 06:53

Tgt Ion:202 Resp: 76730
Ion Ratio Lower Upper
202 100
101 9.7 8.6 12.8
100 8.5 6.4 9.6

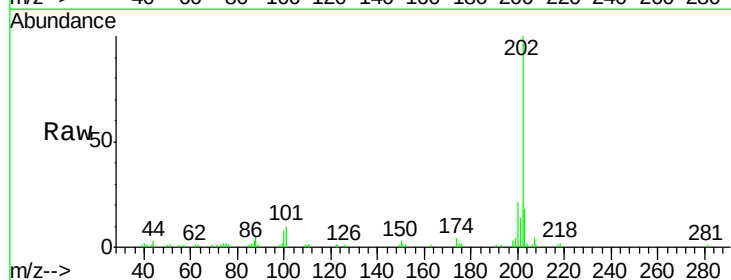

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B



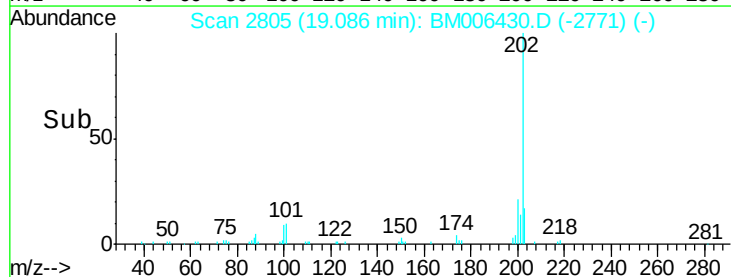
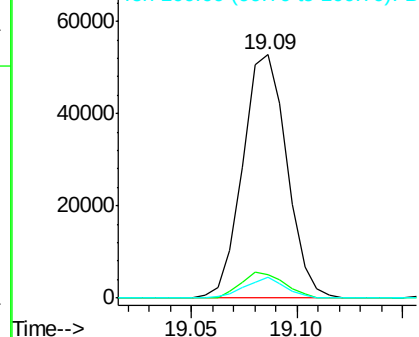


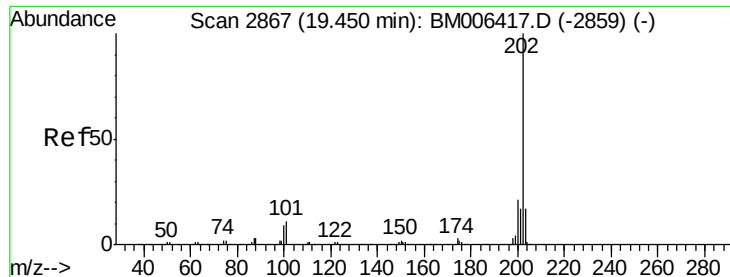

#77
Pvrene
Concen: 1.27 ng/ul
RT: 19.45 min Scan# 2867
Delta R.T. 0.00 min
Lab File: BM006430.D
Acq: 15 Jul 2016 06:53




Instrument :
BNA_M
ClientSampleId :
BDJ74


Tot Ion:202 Resp: 72462
Ion Ratio Lower Upper
202 100
101 12.6 10.0 15.0
100 8.8 7.9 11.9

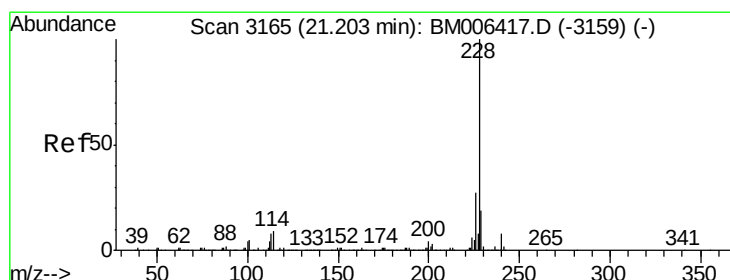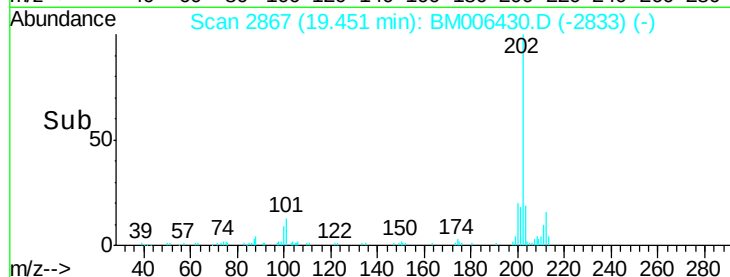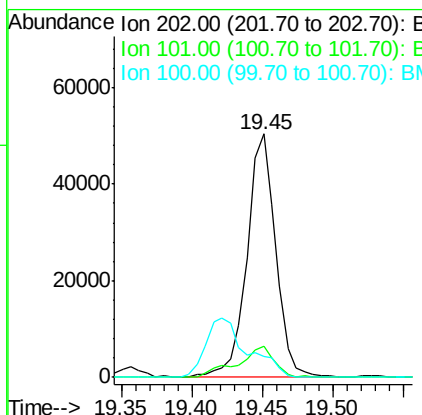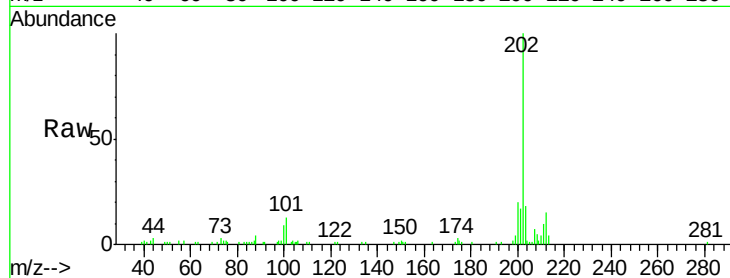

#80
Benzo(a)anthracene
Concen: 1.07 ng/ul
RT: 21.20 min Scan# 3165
Delta R.T. 0.00 min
Lab File: BM006430.D
Acq: 15 Jul 2016 06:53

Tgt Ion:228 Resp: 62652
Ion Ratio Lower Upper
228 100
229 20.4 15.6 23.4
226 30.2 21.4 32.2

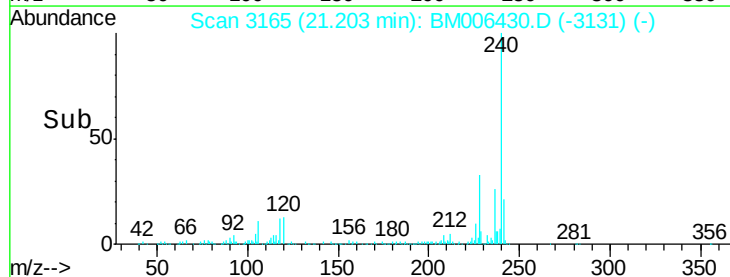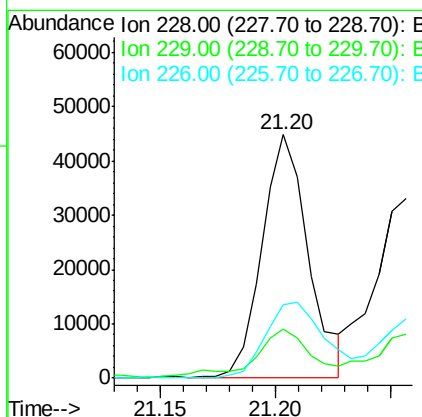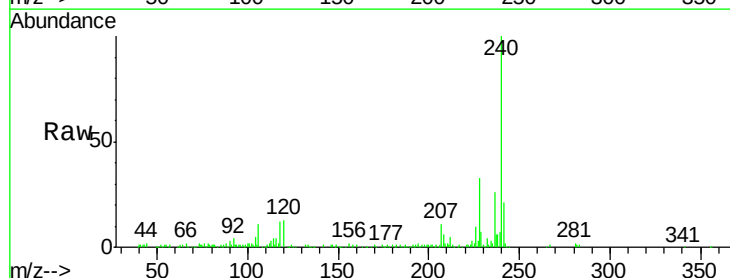

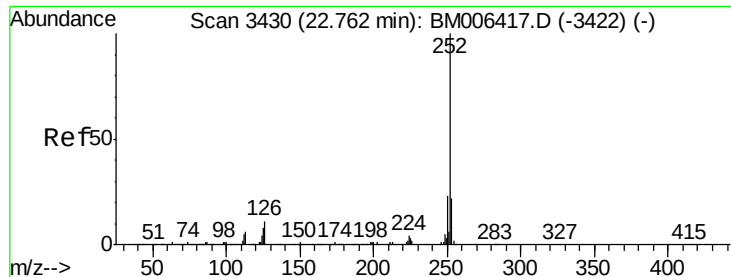

#85

Benzo(b)fluoranthene

Concen: 1.28 ng/ul

RT: 22.76 min Scan# 3430

Delta R.T. 0.00 min

Lab File: BM006430.D

Acq: 15 Jul 2016 06:53

Instrument :

BNA_M

ClientSampleId :

BDJ74


Tot Ion:252 Resp: 77529

Ion Ratio Lower Upper

252 100

253 23.0 17.4 26.2

125 8.5 6.7 10.1

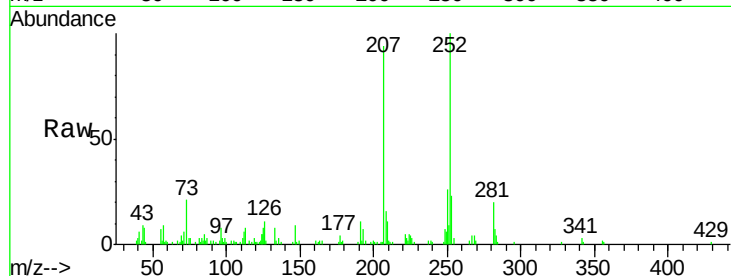


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->

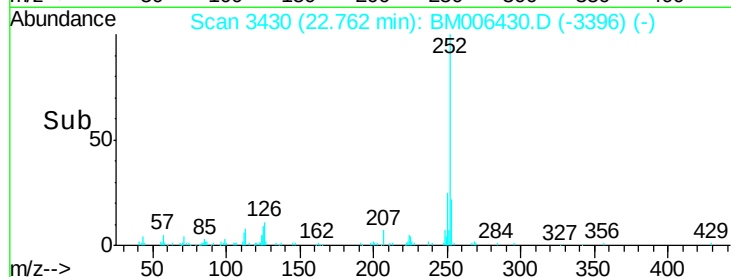


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->

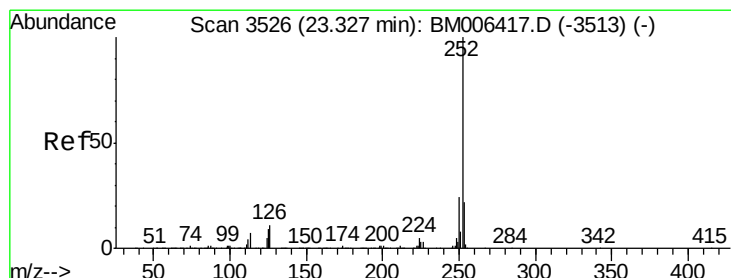

#88

Benzo(a)pyrene

Concen: 1.11 ng/ul

RT: 23.32 min Scan# 3525

Delta R.T. -0.01 min

Lab File: BM006430.D

Acq: 15 Jul 2016 06:53


Tgt Ion:252 Resp: 64551

Ion Ratio Lower Upper

252 100

253 23.0 17.4 26.2

125 10.0 7.6 11.4

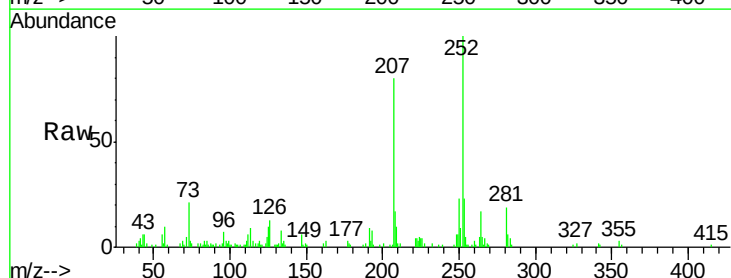


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->

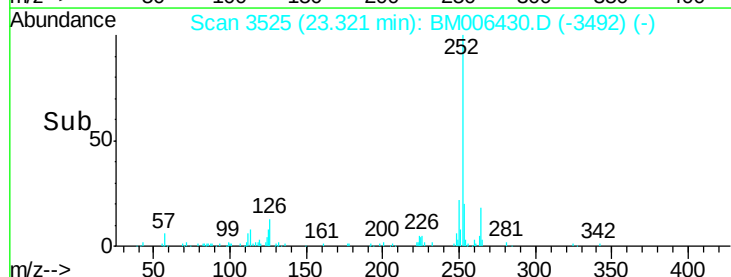

Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->