

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
 Data File : BM006418.D
 Acq On : 14 Jul 2016 19:17
 Operator : UM/SJ
 Sample : PB92088BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	90	94	101	rVB	35700	46847	1.37%	0.156%
2	6.798	708	716	731	rBV	477309	772808	22.55%	2.579%
3	6.963	736	744	756	rBV	327205	537671	15.69%	1.794%
4	7.157	770	777	789	rBV	468990	781142	22.79%	2.606%
5	7.622	849	856	870	rVB	340633	558304	16.29%	1.863%
6	8.328	969	976	992	rBV	543285	932660	27.21%	3.112%
7	8.775	1045	1052	1066	rBV	453480	767310	22.39%	2.560%
8	9.492	1167	1174	1186	rBV	397048	667748	19.48%	2.228%
9	10.028	1258	1265	1282	rBV	526190	928333	27.08%	3.097%
10	10.398	1321	1328	1344	rBV	445605	777992	22.70%	2.596%
11	10.539	1346	1352	1369	rBV	488788	913286	26.65%	3.047%
12	13.686	1880	1887	1906	rBV	1018350	1505943	43.94%	5.025%
13	13.963	1927	1934	1946	rBV	1074680	1652961	48.23%	5.515%
14	14.274	1979	1987	1998	rVB2	647293	1070483	31.23%	3.572%
15	14.492	2018	2024	2046	rBV	466467	811005	23.66%	2.706%
16	15.268	2150	2156	2168	rVB	1386885	2096812	61.17%	6.996%
17	15.404	2173	2179	2192	rVV	479532	727357	21.22%	2.427%
18	17.021	2448	2454	2464	rBV2	934005	1395262	40.71%	4.655%
19	17.121	2464	2471	2483	rVB2	1577368	2400857	70.05%	8.011%
20	19.427	2856	2863	2873	rBV	1974919	2949413	86.05%	9.841%
21	21.221	3162	3168	3177	rBV	1518943	2040157	59.52%	6.807%
22	23.280	3511	3518	3531	rVV2	1799173	3427568	100.00%	11.436%
23	23.421	3535	3542	3554	rVB	1103531	2094937	61.12%	6.990%
24	23.927	3624	3628	3635	rVB3	57013	113586	3.31%	0.379%


Sum of corrected areas: 29970442

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
Data File : BM006418.D
Acq On : 14 Jul 2016 19:17
Operator : UM/SJ
Sample : PB92088BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK88

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

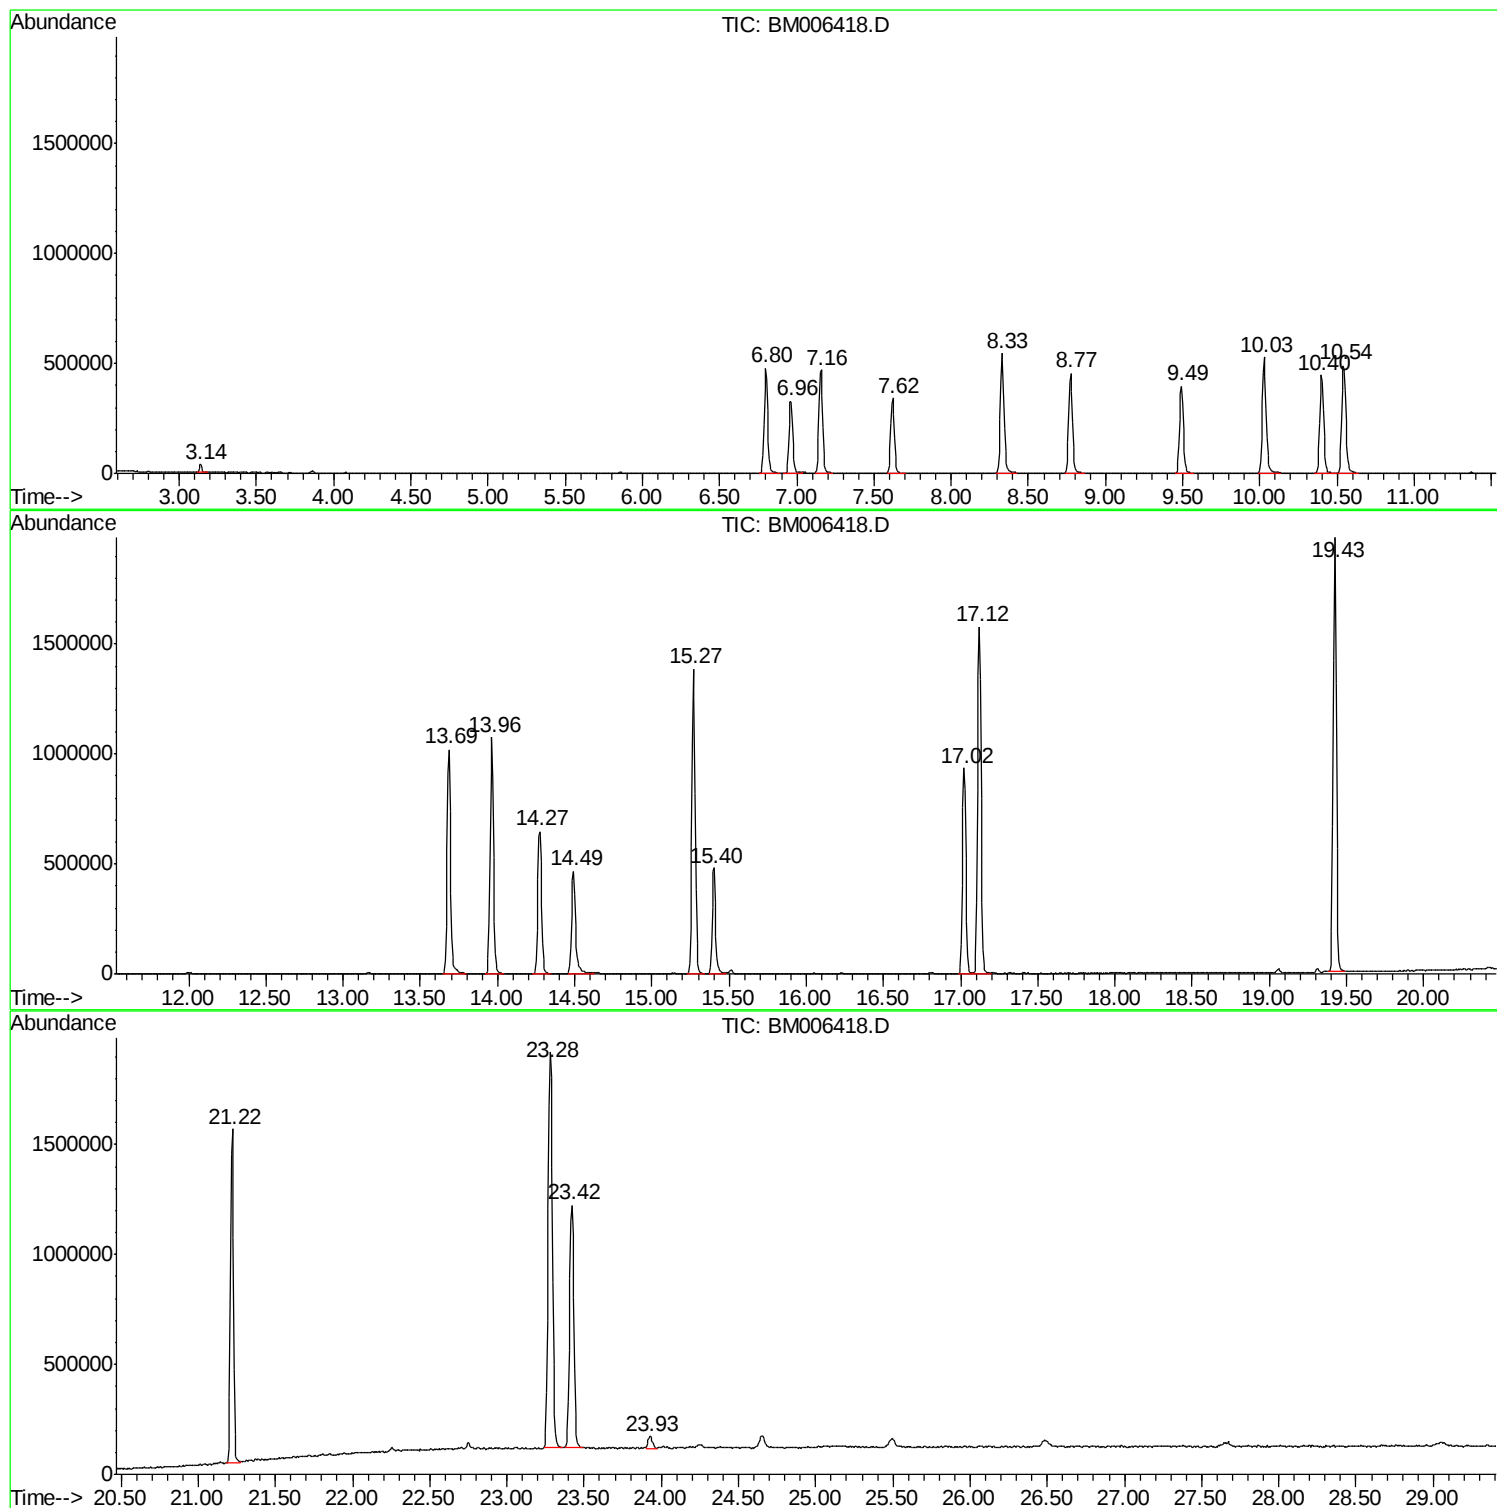

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
Data File : BM006418.D
Acq On : 14 Jul 2016 19:17
Operator : UM/SJ
Sample : PB92088BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK88

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
Data File : BM006418.D
Acq On : 14 Jul 2016 19:17
Operator : UM/SJ
Sample : PB92088BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK88

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc