

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
 Data File : BM006439.D
 Acq On : 15 Jul 2016 12:22
 Operator : UM/SJ
 Sample : H3990-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.798	709	716	727	rVB	91847	145208	4.31%	0.502%
2	6.957	737	743	752	rBV	268561	433125	12.86%	1.496%
3	7.151	770	776	793	rBV	314590	519363	15.43%	1.794%
4	7.616	849	855	868	rVB	451172	740467	21.99%	2.558%
5	8.328	970	976	988	rVB	232553	380700	11.31%	1.315%
6	8.769	1044	1051	1069	rBV	348542	606294	18.01%	2.094%
7	9.486	1166	1173	1186	rBV	295439	521260	15.48%	1.801%
8	10.022	1258	1264	1282	rBV	378322	703048	20.88%	2.429%
9	10.398	1321	1328	1342	rVB	568647	1006741	29.90%	3.478%
10	11.051	1430	1439	1446	rBV2	23846	45360	1.35%	0.157%
11	13.680	1880	1886	1903	rBV	820285	1248728	37.09%	4.314%
12	13.957	1927	1933	1948	rBV	853431	1355181	40.25%	4.682%
13	14.274	1980	1987	2008	rBV2	1547479	2622850	77.90%	9.061%
14	14.492	2018	2024	2038	rBV	66501	134478	3.99%	0.465%
15	15.268	2149	2156	2167	rBV	1208817	1866058	55.42%	6.446%
16	15.398	2173	2178	2193	rBV	453541	658520	19.56%	2.275%
17	17.021	2447	2454	2464	rVB	1185997	1761932	52.33%	6.087%
18	17.121	2464	2471	2482	rBV	1486788	2316832	68.81%	8.004%
19	19.421	2856	2862	2870	rBV2	2055259	2991752	88.86%	10.335%
20	20.356	3017	3021	3025	rBV3	29326	37838	1.12%	0.131%
21	21.221	3162	3168	3174	rBV	1943994	2526618	75.04%	8.728%
22	22.750	3425	3428	3440	rVB4	39860	64045	1.90%	0.221%
23	23.280	3511	3518	3529	rBV2	1738027	3366830	100.00%	11.631%
24	23.421	3534	3542	3553	rVB	1383321	2606829	77.43%	9.005%
25	23.927	3624	3628	3636	rVB3	67310	126916	3.77%	0.438%
26	24.650	3745	3751	3759	rVB3	71886	160201	4.76%	0.553%


Sum of corrected areas: 28947174

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
Data File : BM006439.D
Acq On : 15 Jul 2016 12:22
Operator : UM/SJ
Sample : H3990-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ60

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

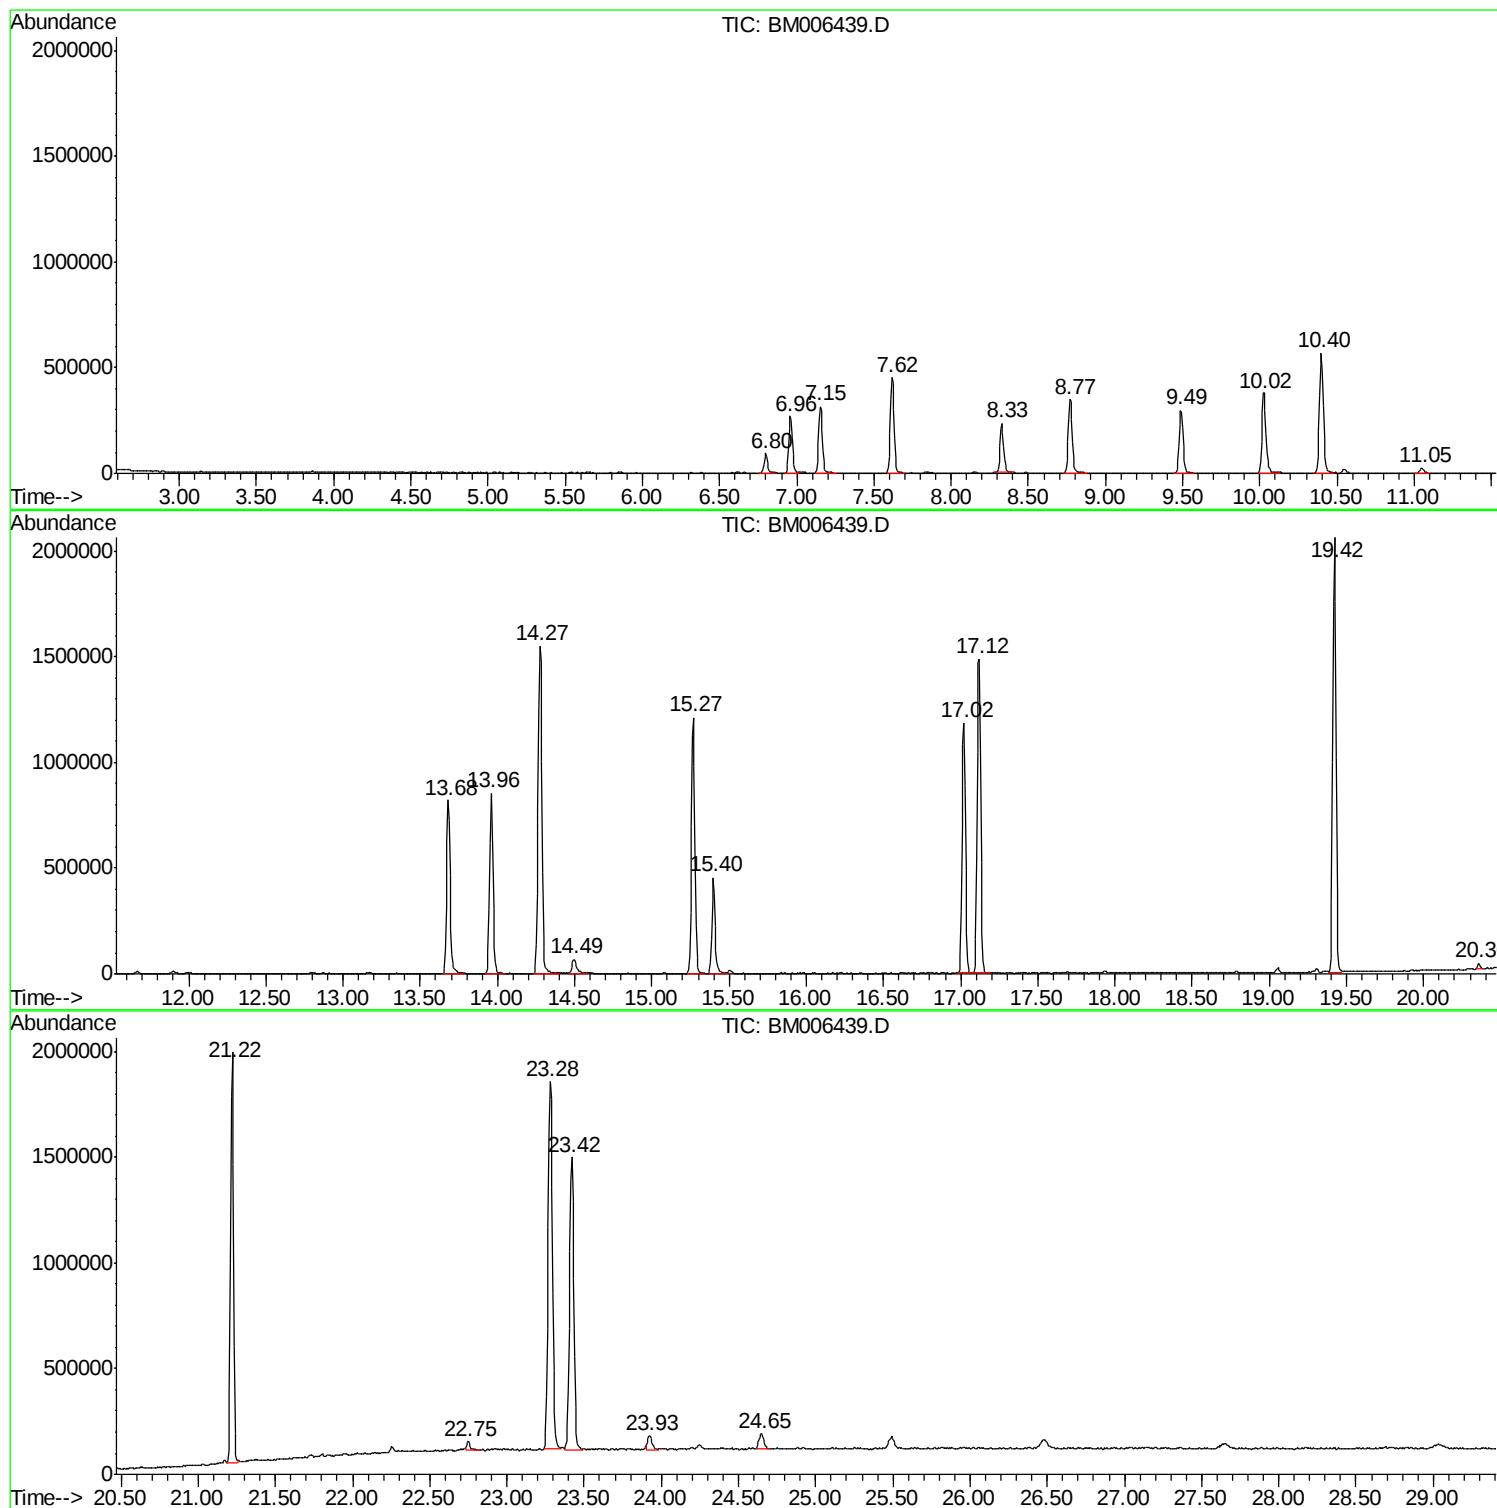

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
Data File : BM006439.D
Acq On : 15 Jul 2016 12:22
Operator : UM/SJ
Sample : H3990-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ60

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
Data File : BM006439.D
Acq On : 15 Jul 2016 12:22
Operator : UM/SJ
Sample : H3990-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ60

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc