

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
 Data File : BM006440.D
 Acq On : 15 Jul 2016 12:58
 Operator : UM/SJ
 Sample : PB92091BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.798	709	716	727	rBV	609272	969803	21.43%	2.491%
2	6.963	737	744	756	rBV	413263	675286	14.92%	1.735%
3	7.157	770	777	792	rVB	577597	968063	21.39%	2.487%
4	7.622	848	856	866	rBV	516541	859297	18.99%	2.207%
5	8.328	969	976	994	rBV	708679	1173471	25.93%	3.014%
6	8.775	1044	1052	1066	rBV	566515	959737	21.21%	2.465%
7	9.486	1166	1173	1194	rVB	481895	844106	18.65%	2.168%
8	10.022	1258	1264	1277	rBV	646319	1169040	25.84%	3.003%
9	10.398	1321	1328	1341	rBV	659169	1155795	25.54%	2.969%
10	10.539	1345	1352	1366	rVV	369221	655618	14.49%	1.684%
11	13.680	1880	1886	1904	rBV	1263410	1990670	43.99%	5.113%
12	13.963	1926	1934	1951	rBV	1307549	2138214	47.25%	5.492%
13	14.268	1980	1986	1998	rBV2	922091	1489903	32.93%	3.827%
14	14.486	2017	2023	2043	rBV	658329	1097744	24.26%	2.820%
15	15.268	2149	2156	2166	rBV	1809107	2735086	60.44%	7.025%
16	15.398	2173	2178	2192	rBV	691845	1017423	22.48%	2.613%
17	17.021	2446	2454	2464	rBV	1284869	1912186	42.26%	4.912%
18	17.121	2464	2471	2481	rBV2	2015340	3172206	70.11%	8.148%
19	19.421	2856	2862	2870	rBV2	2576049	3932238	86.90%	10.100%
20	21.221	3162	3168	3175	rBV	1955944	2623688	57.98%	6.739%
21	23.280	3510	3518	3528	rBV2	2367544	4524925	100.00%	11.623%
22	23.421	3534	3542	3553	rVB	1367650	2653089	58.63%	6.815%
23	23.921	3624	3627	3635	rVB	53442	92483	2.04%	0.238%
24	24.638	3746	3749	3760	rVB3	58076	122056	2.70%	0.314%


Sum of corrected areas: 38932127

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071416\
Data File : BM006440.D
Acq On : 15 Jul 2016 12:58
Operator : UM/SJ
Sample : PB92091BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

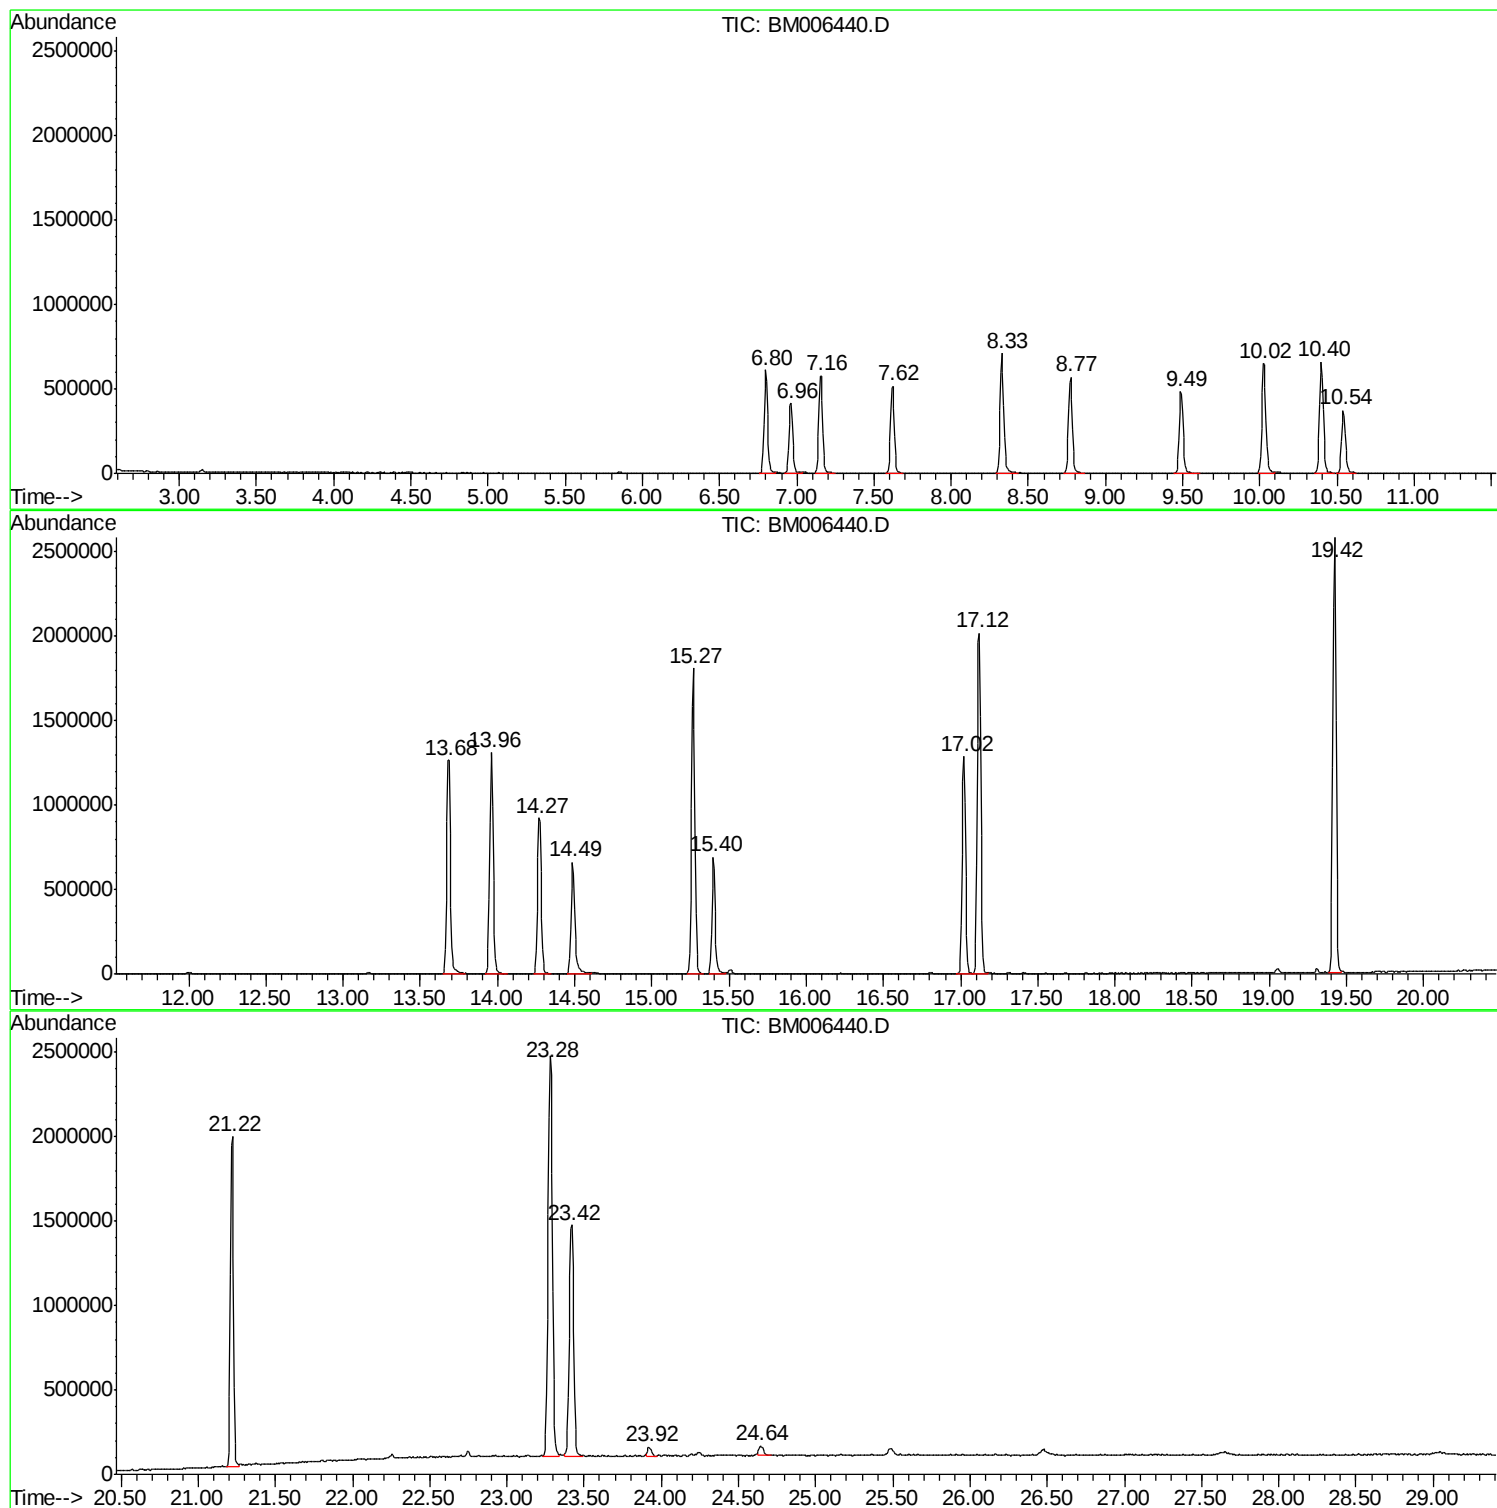

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
Data File : BM006440.D
Acq On : 15 Jul 2016 12:58
Operator : UM/SJ
Sample : PB92091BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071416\
Data File : BM006440.D
Acq On : 15 Jul 2016 12:58
Operator : UM/SJ
Sample : PB92091BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc