




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071420\
Data File : BM026748.D
Acq On : 14 Jul 2020 12:18
Operator : JU/CG
Sample : L1955-02
Misc : MDL-SOIL-02
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-SOIL-02

Manual Integrations
APPROVED

mohammad
7/20/2020 11:24:45 AM

Quant Time: Jul 14 12:50:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 10:31:32 2020
Response via : Initial Calibration

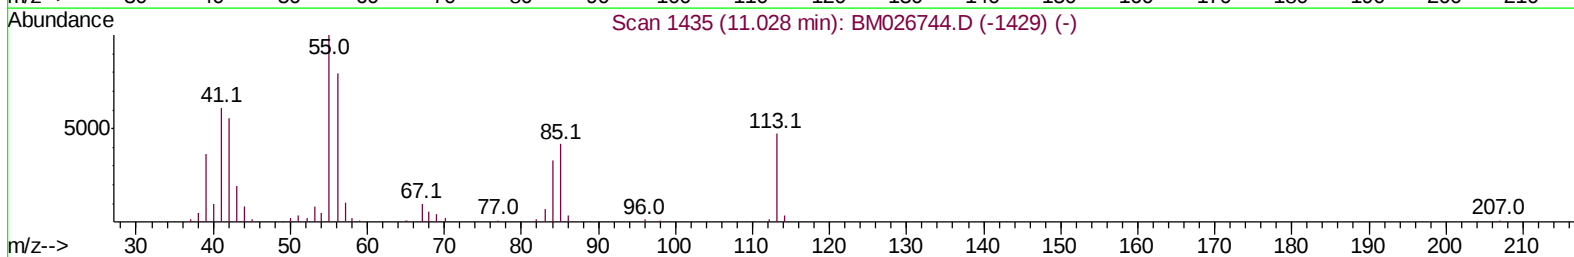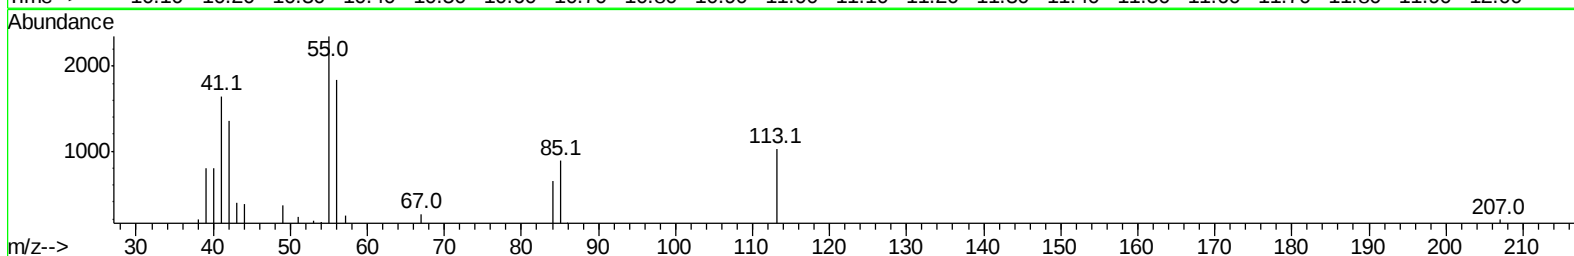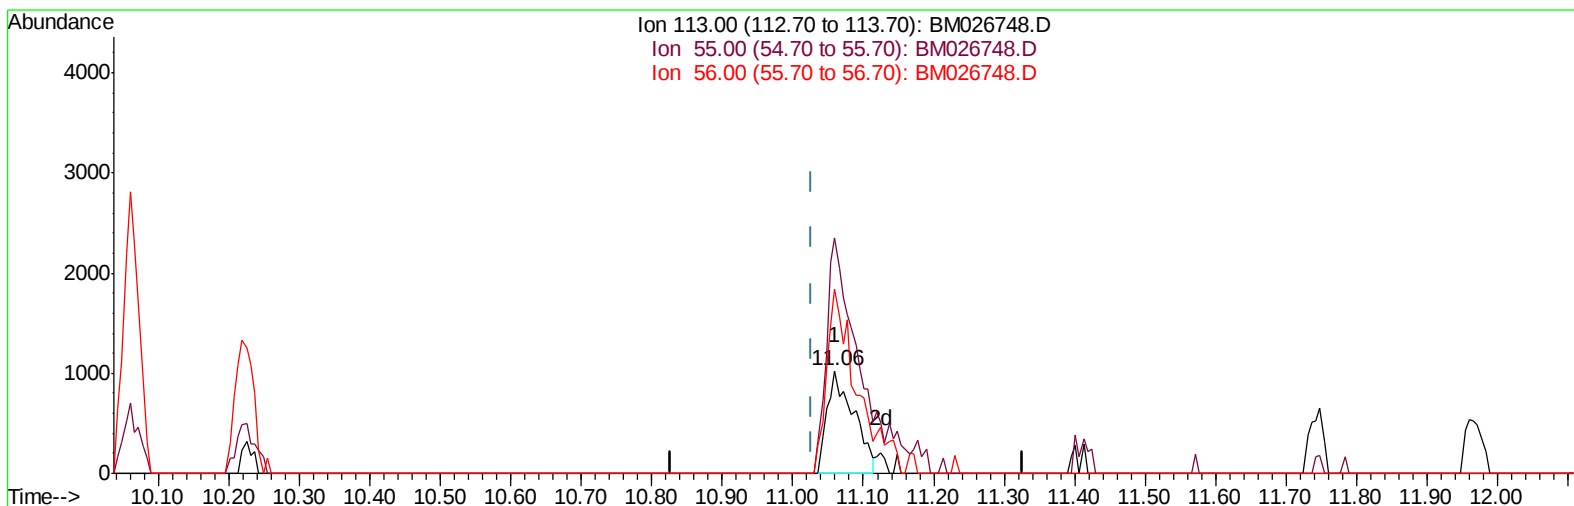

TIC: BM026748.D

(32) Caprolactam

11.060min (+0.032) 2.64ng/ul

response 2667

Ion	Exp%	Act%
113.00	100	100
55.00	224.90	228.60
56.00	168.60	179.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071420\
Data File : BM026748.D
Acq On : 14 Jul 2020 12:18
Operator : JU/CG
Sample : L1955-02
Misc : MDL-SOIL-02
ALS Vial : 6 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
MDL-SOIL-02

Manual Integrations
APPROVED

mohammad

7/20/2020 11:24:45 AM

Quant Time: Jul 14 12:50:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 10:31:32 2020
Response via : Initial Calibration

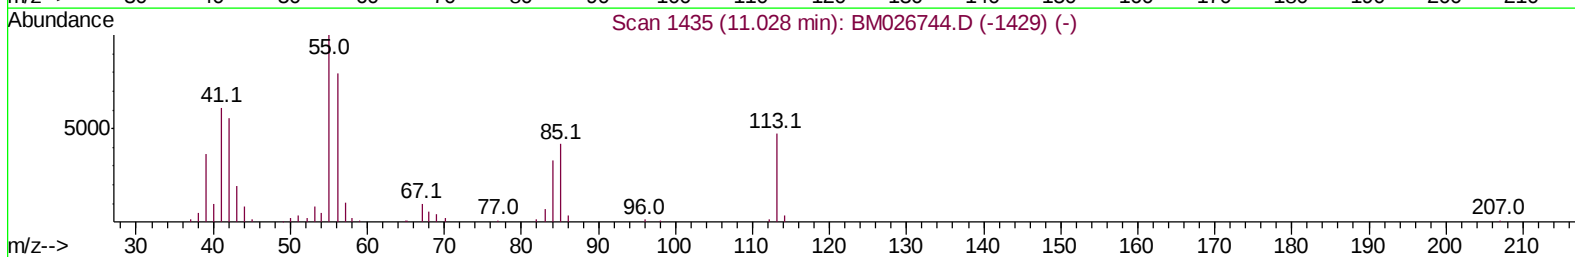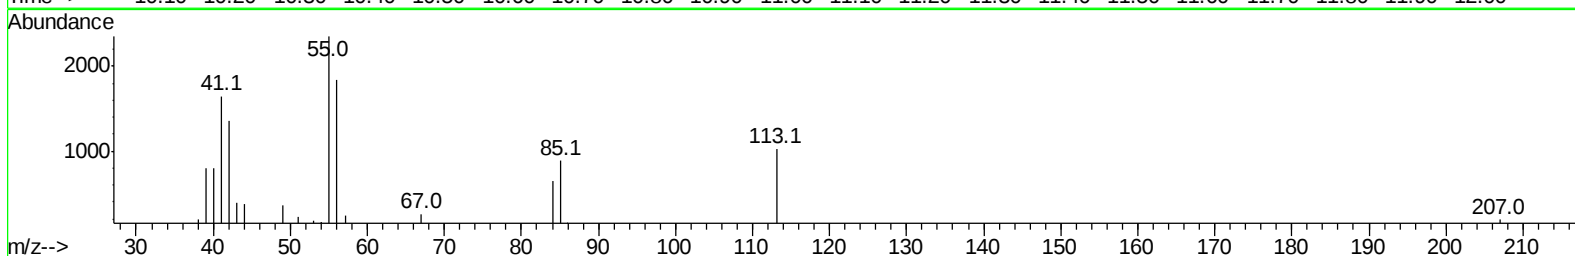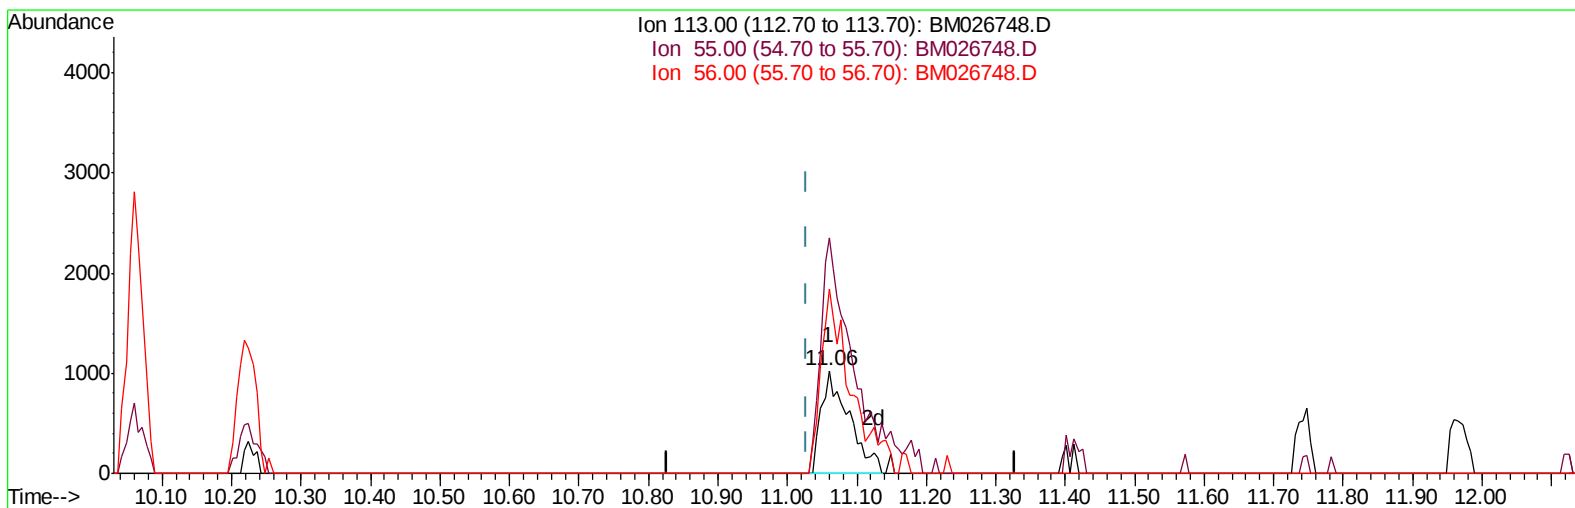

TIC: BM026748.D

(32) Caprolactam

11.060min (+0.032) 2.82ng/ul m

response 2852

Ion	Exp%	Act%
113.00	100	100
55.00	224.90	228.60
56.00	168.60	179.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071420\
Data File : BM026748.D
Acq On : 14 Jul 2020 12:18
Operator : JU/CG
Sample : L1955-02
Misc : MDL-SOIL-02
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
MDL-SOIL-02

Manual Integrations
APPROVED

mohammad

7/20/2020 11:24:45 AM

Quant Time: Jul 14 12:50:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 10:31:32 2020
Response via : Initial Calibration

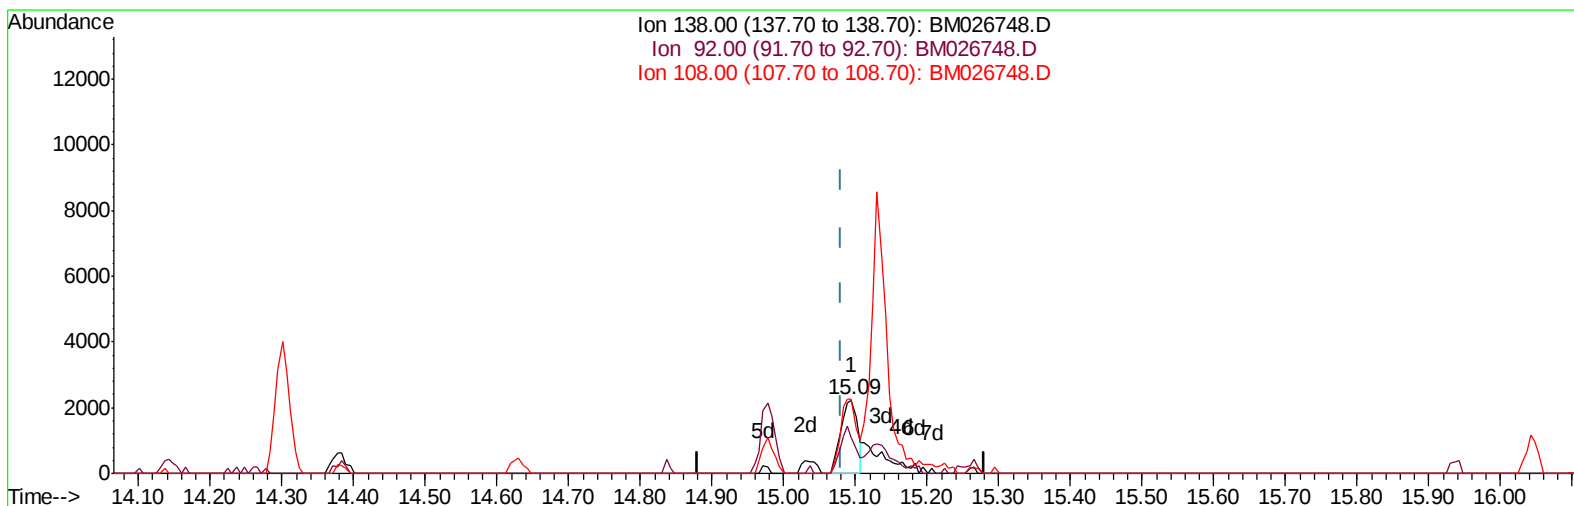

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071420\
Data File : BM026748.D
Acq On : 14 Jul 2020 12:18
Operator : JU/CG
Sample : L1955-02
Misc : MDL-SOIL-02
ALS Vial : 6 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
MDL-SOIL-02

Manual Integrations
APPROVED

mohammad

7/20/2020 11:24:45 AM

Quant Time: Jul 14 12:50:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 10:31:32 2020
Response via : Initial Calibration

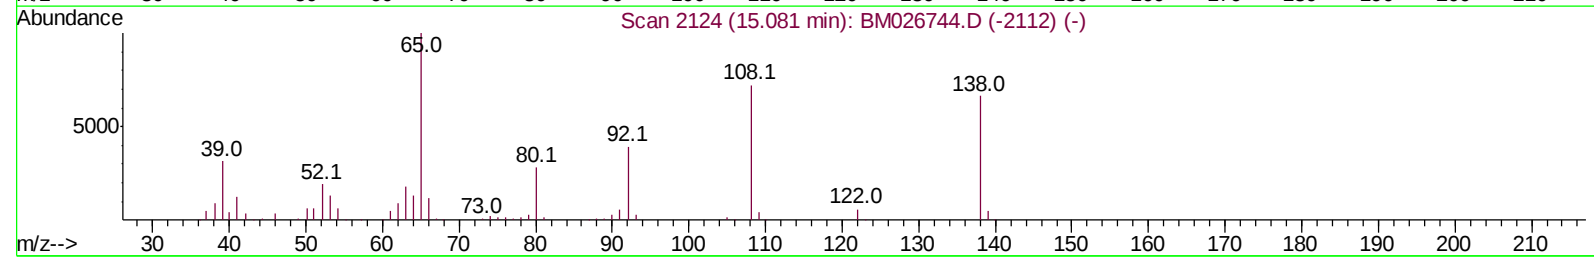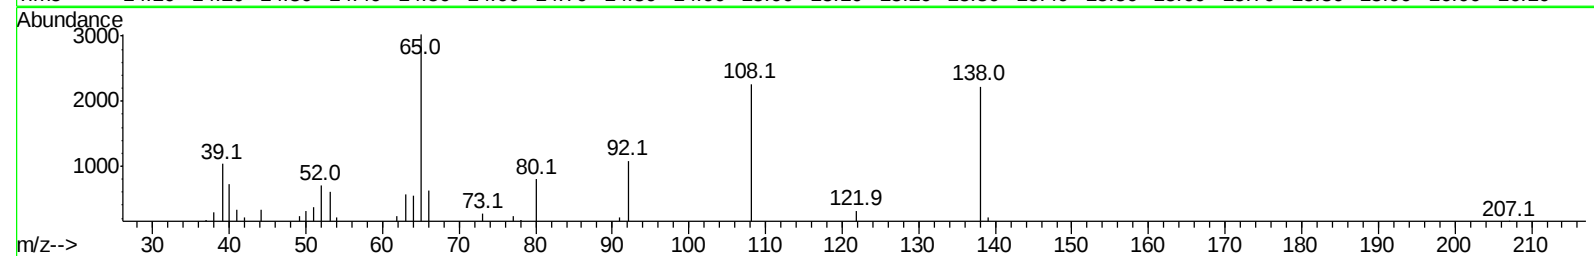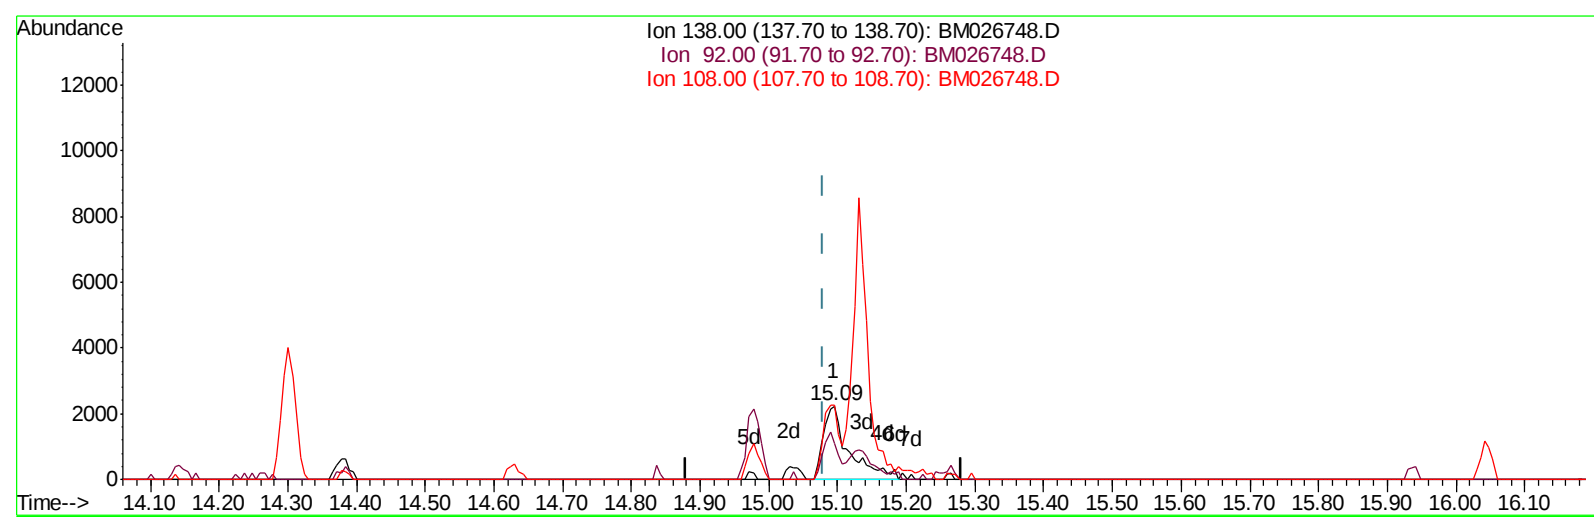

TIC: BM026748.D

(61) 4-Nitroaniline

15.095min (+0.014) 2.95ng/ul m

response 5725

Ion	Exp%	Act%
138.00	100	100
92.00	59.60	48.88
108.00	103.20	101.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071420\
Data File : BM026748.D
Acq On : 14 Jul 2020 12:18
Operator : JU/CG
Sample : L1955-02
Misc : MDL-SOIL-02
ALS Vial : 6 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
MDL-SOIL-02

Manual Integrations
APPROVED

mohammad

7/20/2020 11:24:45 AM

Quant Time: Jul 14 12:50:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 10:31:32 2020
Response via : Initial Calibration

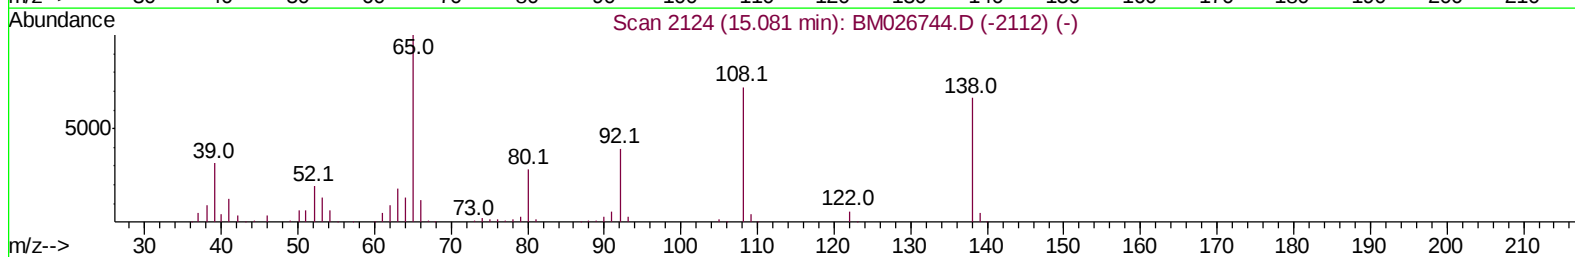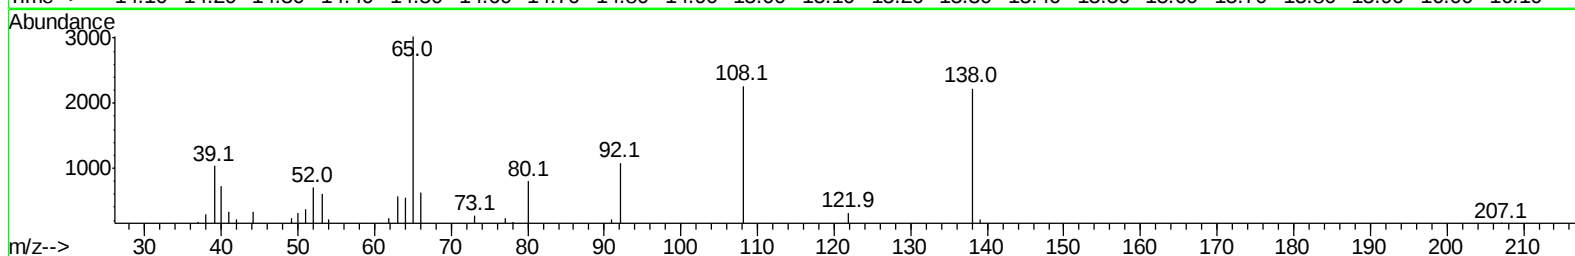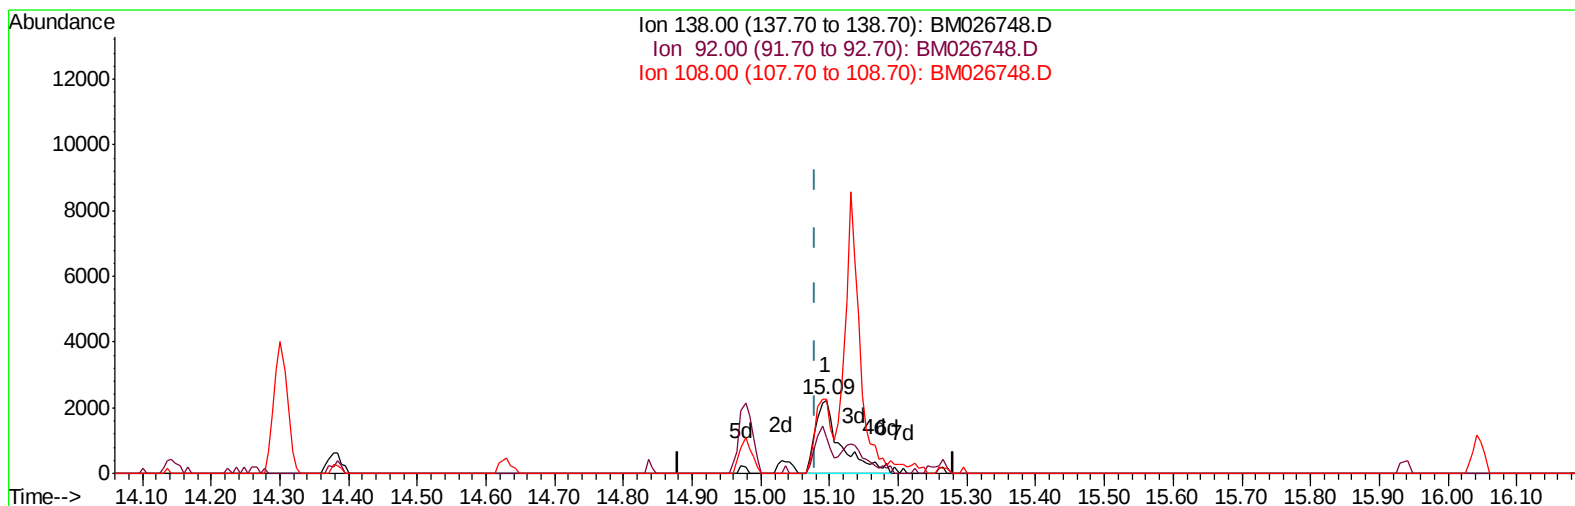

TIC: BM026748.D

(61) 4-Nitroaniline

15.095min (+0.014) 2.95ng/ul m

response 5725

Ion	Exp%	Act%
138.00	100	100
92.00	59.60	48.88
108.00	103.20	101.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071420\
 Data File : BM026748.D
 Acq On : 14 Jul 2020 12:18
 Operator : JU/CG
 Sample : L1955-02
 Misc : MDL-SOIL-02
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-SOIL-02

Manual Integrations
 APPROVED

mohammad

7/20/2020 11:24:45 AM

Quant Time: Jul 14 12:52:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 14 10:31:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.31	152	57147	20.00	ng/ul	0.00
18) Naphthalene-d8	10.07	136	214679	20.00	ng/ul	0.00
36) Acenaphthene-d10	13.97	164	127966	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.74	188	264287	20.00	ng/ul	0.00
78) Chrysene-d12	20.95	240	281487	20.00	ng/ul	0.00
86) Perylene-d12	23.02	264	330114	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.91	96	2988	1.57	ng/uL	0.00
5) Phenol-d5	6.52	99	139843	26.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.67	67	98840	27.92	ng/ul	0.00
9) 2-Chlorophenol-d4	6.85	132	112437	27.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.04	113	108830	26.00	ng/ul	0.00
19) Nitrobenzene-d5	8.46	128	50936	30.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.17	143	55737	30.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.71	165	101933	28.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.22	131	136276	36.51	ng/ul	0.00
44) Dimethylphthalate-d6	13.40	166	302037	29.59	ng/ul	0.00
47) Acenaphthylene-d8	13.66	160	364866	29.58	ng/ul	0.00
52) 4-Nitrophenol-d4	14.24	143	34085	23.14	ng/ul	0.00
58) Fluorene-d10	14.98	176	256548	28.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.13	200	43856	26.56	ng/ul	0.00
71) Anthracene-d10	16.83	188	393753	30.25	ng/ul	0.00
79) Pyrene-d10	19.14	212	450953	30.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.89	264	514579	28.88	ng/ul	0.00

Target Compounds

				Ovalue	
2) 1,4-Dioxane	2.94	88	2789	1.355	ng/uL# 90
4) Benzaldehyde	6.48	77	8673	3.120	ng/ul 95
6) Phenol	6.55	94	19404	3.372	ng/ul 98
8) Bis(2-Chloroethyl)ether	6.76	93	15450	3.526	ng/ul 91
10) 2-Chlorophenol	6.88	128	14956	3.374	ng/ul 93
11) 2-Methylphenol	7.78	108	13007	3.164	ng/ul 96
12) 2,2'-oxybis(1-Chloropropan	7.85	45	31161	3.666	ng/ul 98
14) Acetophenone	8.14	105	23541	3.319	ng/ul 98
15) N-Nitroso-di-n-propylamine	8.12	70	12783	3.051	ng/ul# 97
16) 4-Methylphenol	8.11	108	15083	3.301	ng/ul 99
17) Hexachloroethane	8.36	117	7010	3.568	ng/ul 91
20) Nitrobenzene	8.50	77	20849	3.894	ng/ul 98
21) Isophorone	9.02	82	31823	3.536	ng/ul 98
23) 2-Nitrophenol	9.20	139	8005	3.822	ng/ul 92
24) 2,4-Dimethylphenol	9.29	107	17454	3.619	ng/ul 91
25) Bis(2-Chloroethoxy)methane	9.51	93	19788	3.698	ng/ul# 94
27) 2,4-Dichlorophenol	9.74	162	13648	3.726	ng/ul 90
28) Naphthalene	10.11	128	45872	3.610	ng/ul 96
30) 4-Chloroaniline	10.25	127	17381	4.382	ng/ul 96
31) Hexachlorobutadiene	10.40	225	10181	3.835	ng/ul 96
32) Caprolactam	11.06	113	2852m	2.819	ng/ul
33) 4-Chloro-3-methylphenol	11.41	107	13800	3.311	ng/ul 95
34) 2-Methylnaphthalene	11.74	142	30961	3.478	ng/ul 91

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071420\
 Data File : BM026748.D
 Acq On : 14 Jul 2020 12:18
 Operator : JU/CG
 Sample : L1955-02
 Misc : MDL-SOIL-02
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 MDL-SOIL-02

Manual Integrations
 APPROVED

Quant Time: Jul 14 12:52:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 14 10:31:32 2020
 Response via : Initial Calibration

mohammad

7/20/2020 11:24:45 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	11.97	142	29247	3.525	ng/ul#	90
37) 1,2,4,5-Tetrachlorobenzene	12.13	216	17609	3.786	ng/ul	95
38) Hexachlorocyclopentadiene	12.10	237	2726	1.148	ng/ul#	89
39) 2,4,6-Trichlorophenol	12.40	196	9683	3.527	ng/ul	97
40) 2,4,5-Trichlorophenol	12.48	196	10033	3.341	ng/ul	100
41) 1,1'-Biphenyl	12.79	154	38893	3.511	ng/ul	98
42) 2-Chloronaphthalene	12.83	162	31873	3.656	ng/ul	95
43) 2-Nitroaniline	13.06	65	8988	3.066	ng/ul	89
45) Dimethylphthalate	13.45	163	39592	3.706	ng/ul	98
46) 2,6-Dinitrotoluene	13.58	165	6774	3.280	ng/ul#	91
48) Acenaphthylene	13.68	152	47749	3.615	ng/ul	99
49) 3-Nitroaniline	13.91	138	5442	3.170	ng/ul	91
50) Acenaphthene	14.04	153	32499	3.481	ng/ul	98
51) 2,4-Dinitrophenol	14.15	184	2094	1.952	ng/ul#	83
53) 4-Nitrophenol	14.25	109	4675	3.083	ng/ul	84
54) Dibenzofuran	14.38	168	48111	3.632	ng/ul	97
55) 2,4-Dinitrotoluene	14.38	165	10057	3.275	ng/ul	93
56) 2,3,4,6-Tetrachlorophenol	14.63	232	8589	3.323	ng/ul#	88
57) Diethylphthalate	14.84	149	38098	3.548	ng/ul	98
59) Fluorene	15.04	166	37956	3.507	ng/ul	97
60) 4-Chlorophenyl-phenylether	15.04	204	19991	3.554	ng/ul	97
61) 4-Nitroaniline	15.09	138	5725m	2.949	ng/ul	
64) 4,6-Dinitro-2-methylphenol	15.15	198	5951	3.403	ng/ul#	88
65) N-Nitrosodiphenylamine	15.26	169	31979	3.619	ng/ul	98
66) 4-Bromophenyl-phenylether	15.94	248	12127	3.806	ng/ul	95
67) Hexachlorobenzene	16.04	284	13509	3.721	ng/ul#	89
68) Atrazine	16.24	200	11107	3.858	ng/ul	97
69) Pentachlorophenol	16.42	266	4740	2.648	ng/ul	90
70) Phenanthrene	16.77	178	62343	3.788	ng/ul	96
72) Anthracene	16.87	178	61471	3.702	ng/ul	98
73) 1,2,3,4-Tetrachlorobenzene	12.75	216	17105	3.754	ng/uL	98
74) Pentachlorobenzene	14.30	250	17071	3.912	ng/uL	94
75) Carbazole	17.15	167	47667	3.585	ng/ul	96
76) Di-n-butylphthalate	17.74	149	58483	3.636	ng/ul	99
77) Fluoranthene	18.81	202	70059	4.115	ng/ul#	95
80) Pvrene	19.17	202	77744	3.897	ng/ul	99
81) Butylbenzylphthalate	20.11	149	25580	3.615	ng/ul	99
82) 3,3'-Dichlorobenzidine	20.89	252	16247	2.863	ng/ul#	95
83) Benzo(a)anthracene	20.94	228	76436	3.945	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	20.91	149	39545	3.752	ng/ul#	96
85) Chrysene	20.99	228	73188	3.807	ng/ul	98
87) Di-n-octyl phthalate	21.75	149	70737	3.478	ng/ul	100
88) Benzo(b)fluoranthene	22.42	252	80192	3.576	ng/ul	99
89) Benzo(k)fluoranthene	22.46	252	77929	3.507	ng/ul	99
91) Benzo(a)pyrene	22.93	252	80298	4.037	ng/ul	96
92) Indeno(1,2,3-cd)pyrene	25.02	276	92213	3.552	ng/ul	98
93) Dibenzo(a,h)anthracene	25.03	278	77454	3.541	ng/ul	97
94) Benzo(a,h,i)perylene	25.63	276	78691	3.634	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071420\
Data File : BM026748.D
Acq On : 14 Jul 2020 12:18
Operator : JU/CG
Sample : L1955-02
Misc : MDL-SOIL-02
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-SOIL-02

Manual Integrations
APPROVED

mohammad

7/20/2020 11:24:45 AM

Quant Time: Jul 14 12:52:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 14 10:31:32 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

