

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071420\
 Data File : BM026754.D
 Acq On : 14 Jul 2020 15:57
 Operator : JU/CG
 Sample : PB130124BL
 Misc : PBBL-WATER-02
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.907	25	29	34	rBV	31662	40859	2.36%	0.212%
2	3.596	143	146	150	rBV3	4452	4461	0.26%	0.023%
3	3.825	181	185	192	rBV	46977	57925	3.34%	0.301%
4	4.225	248	253	260	rBV	29411	39402	2.27%	0.205%
5	4.631	320	322	325	rVB3	1474	1786	0.10%	0.009%
6	5.813	518	523	524	rBV4	1266	1893	0.11%	0.010%
7	5.831	524	526	530	rBV3	1047	1775	0.10%	0.009%
8	6.525	638	644	659	rBV	374643	604769	34.92%	3.144%
9	6.666	663	668	681	rVB	276942	427034	24.65%	2.220%
10	6.854	694	700	708	rBV	386533	609192	35.17%	3.167%
11	7.307	771	777	787	rBV	286802	432246	24.95%	2.247%
12	8.042	896	902	915	rBV	418172	675513	39.00%	3.511%
13	8.160	921	922	929	rVB4	1538	2623	0.15%	0.014%
14	8.454	966	972	985	rBV	358900	580461	33.51%	3.017%
15	9.172	1087	1094	1109	rBV	301053	494250	28.53%	2.569%
16	9.713	1178	1186	1205	rBV	364555	682883	39.42%	3.550%
17	9.842	1207	1208	1214	rVB4	1370	2097	0.12%	0.011%
18	10.060	1239	1245	1255	rBV	351331	566084	32.68%	2.942%
19	10.219	1266	1272	1294	rBV	348663	675484	39.00%	3.511%
20	11.683	1516	1521	1530	rBV4	3325	7563	0.44%	0.039%
21	13.401	1807	1813	1824	rBV	695740	967861	55.88%	5.031%
22	13.654	1850	1856	1868	rBV	745113	1078906	62.29%	5.608%
23	13.860	1886	1891	1893	rBV3	4160	5977	0.35%	0.031%
24	13.971	1904	1910	1920	rVB	513000	701242	40.48%	3.645%
25	14.236	1950	1955	1982	rBV	164098	431337	24.90%	2.242%
26	14.483	1995	1997	2002	rVB4	1706	2191	0.13%	0.011%
27	14.818	2050	2054	2057	rBV4	1422	2381	0.14%	0.012%
28	14.977	2075	2081	2095	rBV	970392	1347461	77.79%	7.004%
29	15.130	2101	2107	2119	rBV	280778	449352	25.94%	2.336%
30	15.224	2119	2123	2127	rVB4	11892	17715	1.02%	0.092%
31	15.771	2212	2216	2220	rBV3	2810	3506	0.20%	0.018%
32	16.377	2316	2319	2322	rVB2	1935	2091	0.12%	0.011%
33	16.524	2340	2344	2348	rBV4	2207	3157	0.18%	0.016%
34	16.624	2357	2361	2369	rBV3	11074	16629	0.96%	0.086%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071420\
 Data File : BM026754.D
 Acq On : 14 Jul 2020 15:57
 Operator : JU/CG
 Sample : PB130124BL
 Misc : PBBL-WATER-02
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
 Title : SVOA CALIBRATION

35	16.730	2373	2379	2387	rVB	589971	805244	46.49%	4.186%
36	16.830	2390	2396	2410	rBV	839430	1186181	68.48%	6.166%
37	17.489	2503	2508	2509	rBV4	1225	2064	0.12%	0.011%
38	17.683	2537	2541	2547	rBV6	3117	5733	0.33%	0.030%
39	17.877	2570	2574	2576	rBV4	1439	2270	0.13%	0.012%
40	17.983	2586	2592	2596	rBV5	6642	14848	0.86%	0.077%
41	18.571	2688	2692	2695	rVB5	3088	4266	0.25%	0.022%
42	18.777	2723	2727	2732	rBV2	8963	12539	0.72%	0.065%
43	19.030	2767	2770	2775	rVB	8676	10966	0.63%	0.057%
44	19.142	2783	2789	2801	rBV	1254396	1639813	94.67%	8.524%
45	19.271	2809	2811	2815	rVB2	3203	2191	0.13%	0.011%
46	19.442	2838	2840	2841	rBV2	2020	1810	0.10%	0.009%
47	19.565	2859	2861	2864	rBV3	2194	2565	0.15%	0.013%
48	20.177	2963	2965	2971	rBV7	6896	8979	0.52%	0.047%
49	20.953	3092	3097	3108	rBV	696046	949408	54.81%	4.935%
50	21.989	3270	3273	3277	rBV2	59936	78680	4.54%	0.409%
51	22.447	3348	3351	3355	rVB	98218	119660	6.91%	0.622%
52	22.894	3421	3427	3434	rBV	1103871	1732115	100.00%	9.003%
53	22.953	3434	3437	3442	rVV	157201	219838	12.69%	1.143%
54	23.024	3443	3449	3460	rVB	563022	1016822	58.70%	5.285%
55	23.530	3530	3535	3541	rVB	149971	238965	13.80%	1.242%
56	24.183	3642	3646	3653	rVB	128917	245316	14.16%	1.275%


Sum of corrected areas: 19238379

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071420\
Data File : BM026754.D
Acq On : 14 Jul 2020 15:57
Operator : JU/CG
Sample : PB130124BL
Misc : PBBL-WATER-02
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK24

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

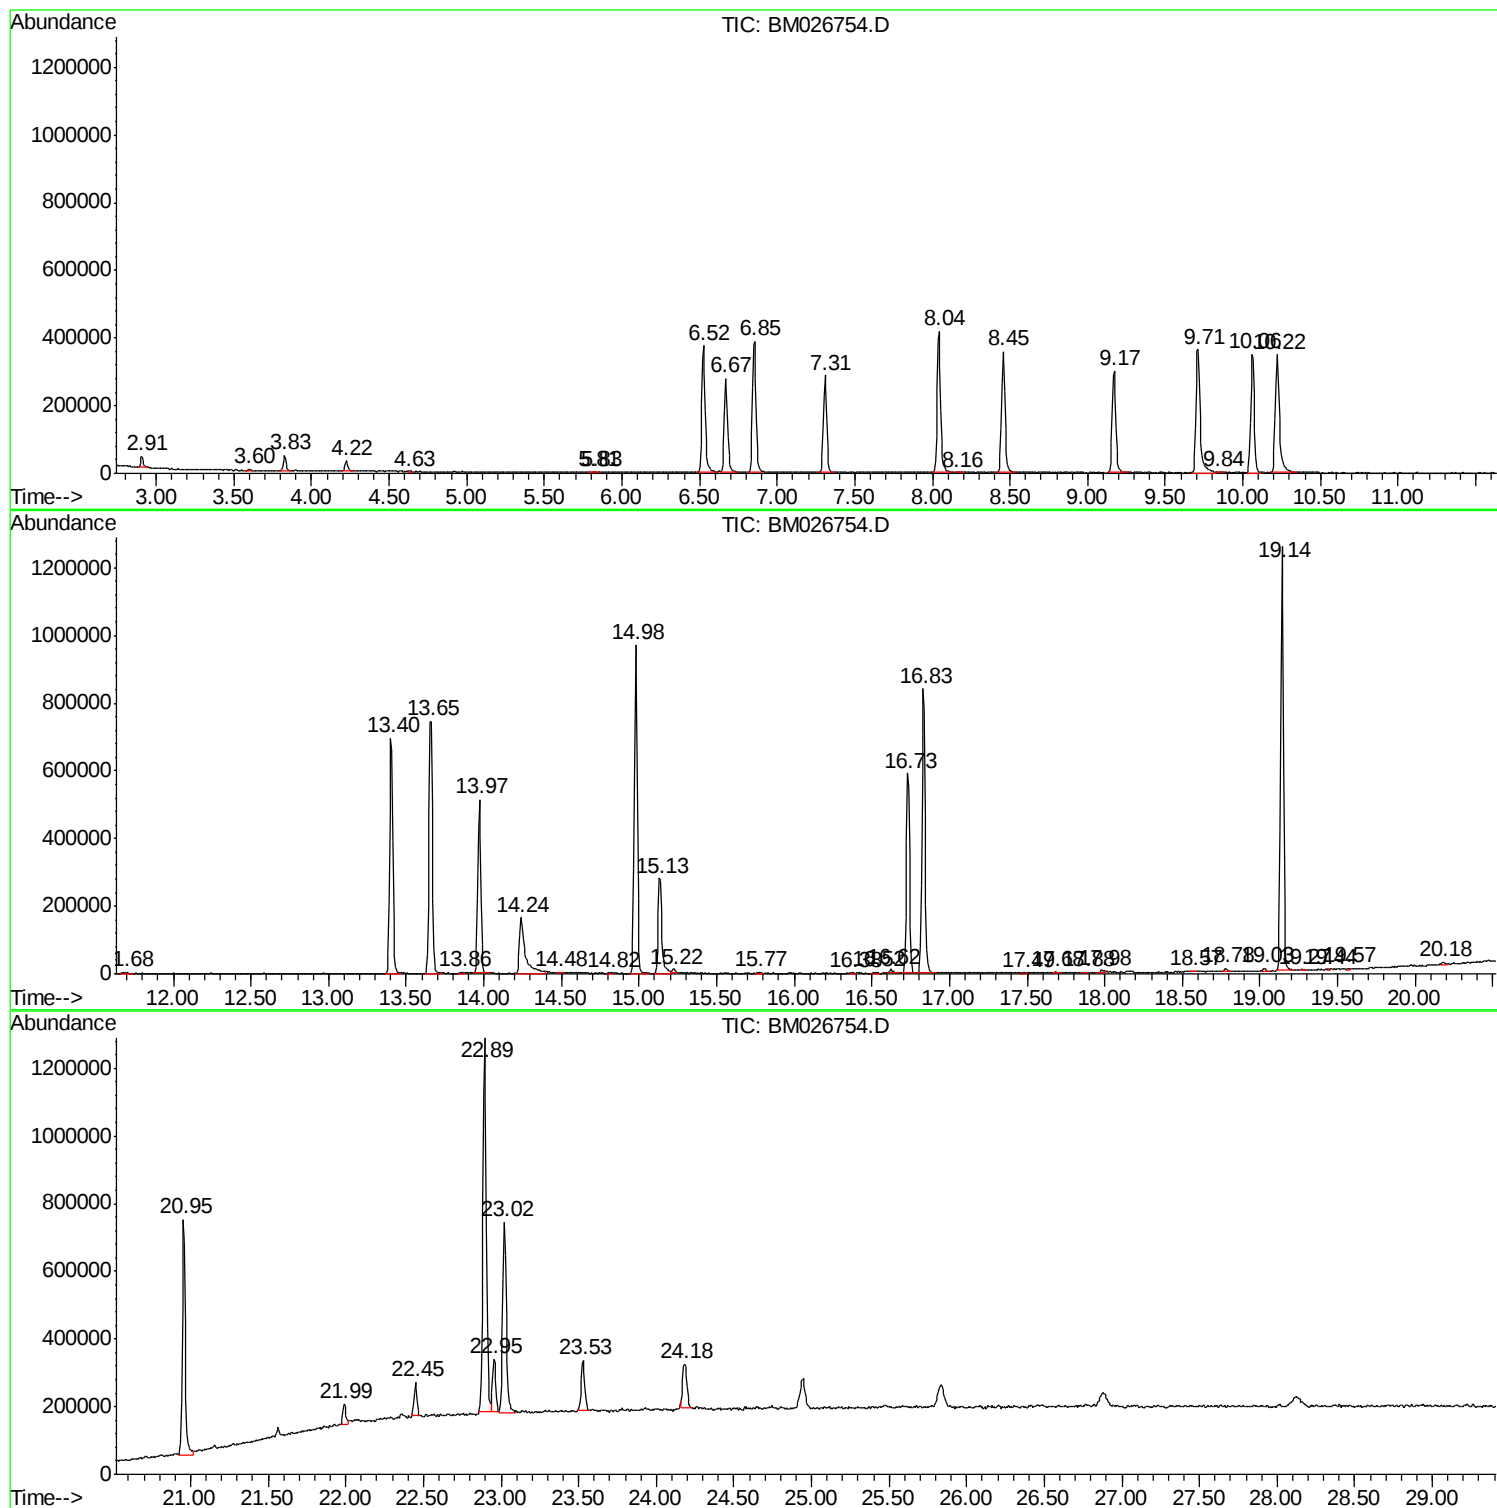

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071420\
Data File : BM026754.D
Acq On : 14 Jul 2020 15:57
Operator : JU/CG
Sample : PB130124BL
Misc : PBBL-WATER-02
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK24

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071420\
Data File : BM026754.D
Acq On : 14 Jul 2020 15:57
Operator : JU/CG
Sample : PB130124BL
Misc : PBBL-WATER-02
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK24

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM063020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc