

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071515\
 Data File : BM001924.D
 Acq On : 14 Jul 2015 23:19
 Operator : TP/UM
 Sample : G2938-20
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01Z7

Quant Time: Jul 15 05:14:24 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 15 05:12:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	84690	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	372164	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	257354	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	597701	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	579809	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	459837	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	1883	1.09	ng/uL	0.00
5) Phenol-d5	6.82	99	38619	5.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	98271	26.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	112864	20.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	72475	12.76	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	70090	25.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	80965	26.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	140565	22.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.45	131	574	0.09	ng/ul	-0.14
43) Dimethylphthalate-d6	13.72	166	528359	25.45	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	615615	24.66	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	15305	4.35	ng/ul	0.00
57) Fluorene-d10	15.30	176	473564	26.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	89600	23.15	ng/ul	0.00
70) Anthracene-d10	17.16	188	724459	25.82	ng/ul	0.00
78) Pyrene-d10	19.46	212	796771	30.08	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	564413	24.27	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	2.88	88	5207	2.85	ng/uL#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071515\
Data File : BM001924.D
Acq On : 14 Jul 2015 23:19
Operator : TP/UM
Sample : G2938-20
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01Z7

Quant Time: Jul 15 05:14:24 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 15 05:12:40 2015
Response via : Initial Calibration

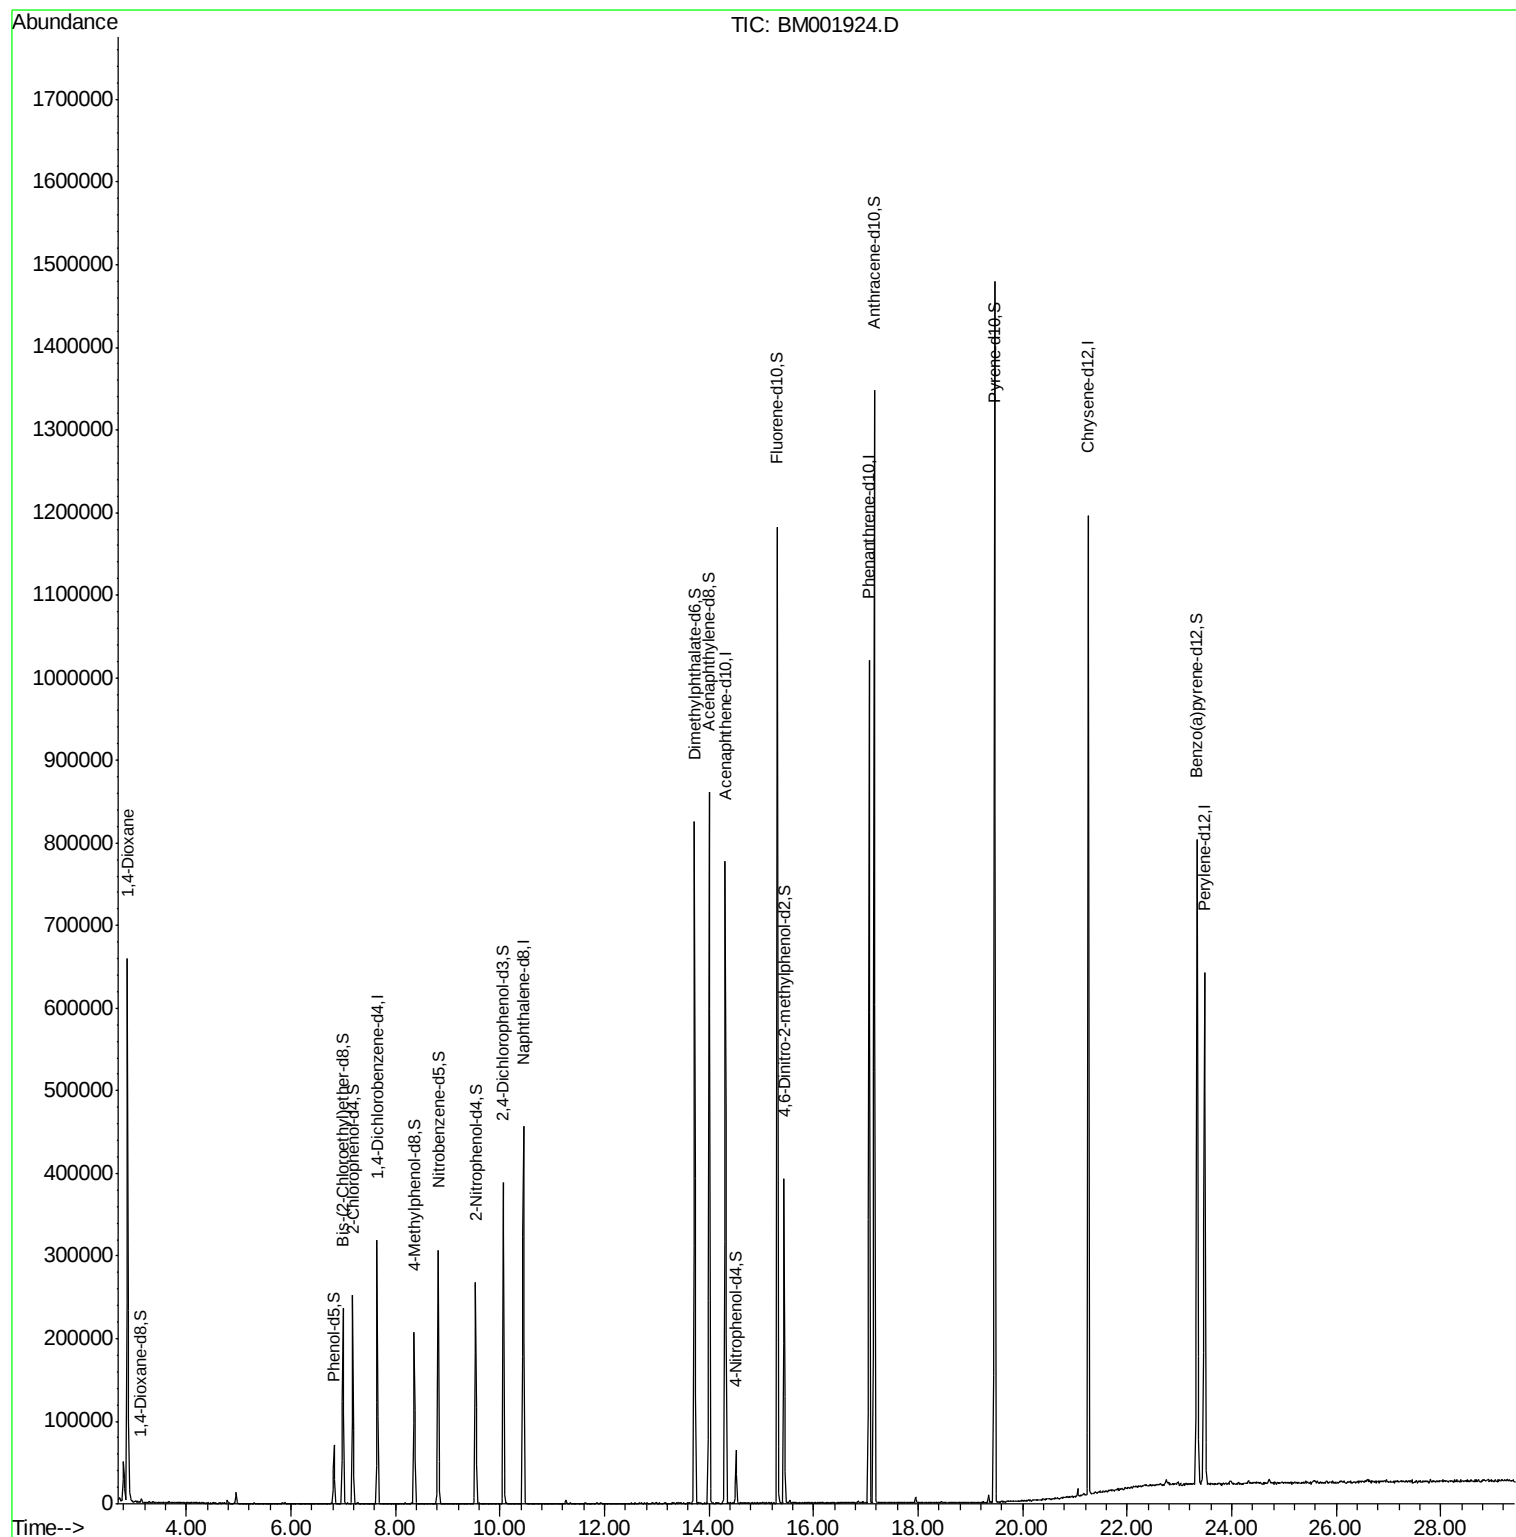

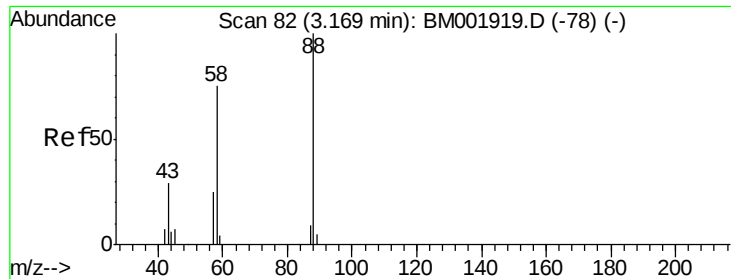

#2
 1,4-Dioxane
 Concen: 2.85 ng/uL
 RT: 2.88 min Scan# 32
 Delta R.T. -0.29 min
 Lab File: BM001924.D
 Acq: 14 Jul 2015 23:19

Instrument :
 BNA_M
 ClientSampleId :
 C01Z7

Tgt Ion: 88 Resp: 5207
 Ion Ratio Lower Upper
 88 100
 43 2268.9 22.1 33.1#
 58 29.6 54.9 82.3#

