

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071515\
 Data File : BM001921.D
 Acq On : 14 Jul 2015 21:29
 Operator : TP/UM
 Sample : G2938-17
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01Y3

Quant Time: Jul 15 05:51:22 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 15 05:12:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	84833	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	358065	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	235383	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	526112	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	493010	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	425062	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	1800	1.04	ng/uL	0.00
5) Phenol-d5	6.82	99	35289	5.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	92784	24.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	105988	19.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	66579	11.70	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	64686	24.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	75282	25.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	130452	21.78	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	449742	23.69	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	557198	24.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	11854	3.69	ng/ul	0.00
57) Fluorene-d10	15.30	176	404737	24.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	70719	20.76	ng/ul	0.00
70) Anthracene-d10	17.16	188	616106	24.95	ng/ul	0.00
78) Pyrene-d10	19.46	212	645497	28.66	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	503790	23.44	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.17	88	19909	10.88	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071515\
Data File : BM001921.D
Acq On : 14 Jul 2015 21:29
Operator : TP/UM
Sample : G2938-17
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01Y3

Quant Time: Jul 15 05:51:22 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 15 05:12:40 2015
Response via : Initial Calibration

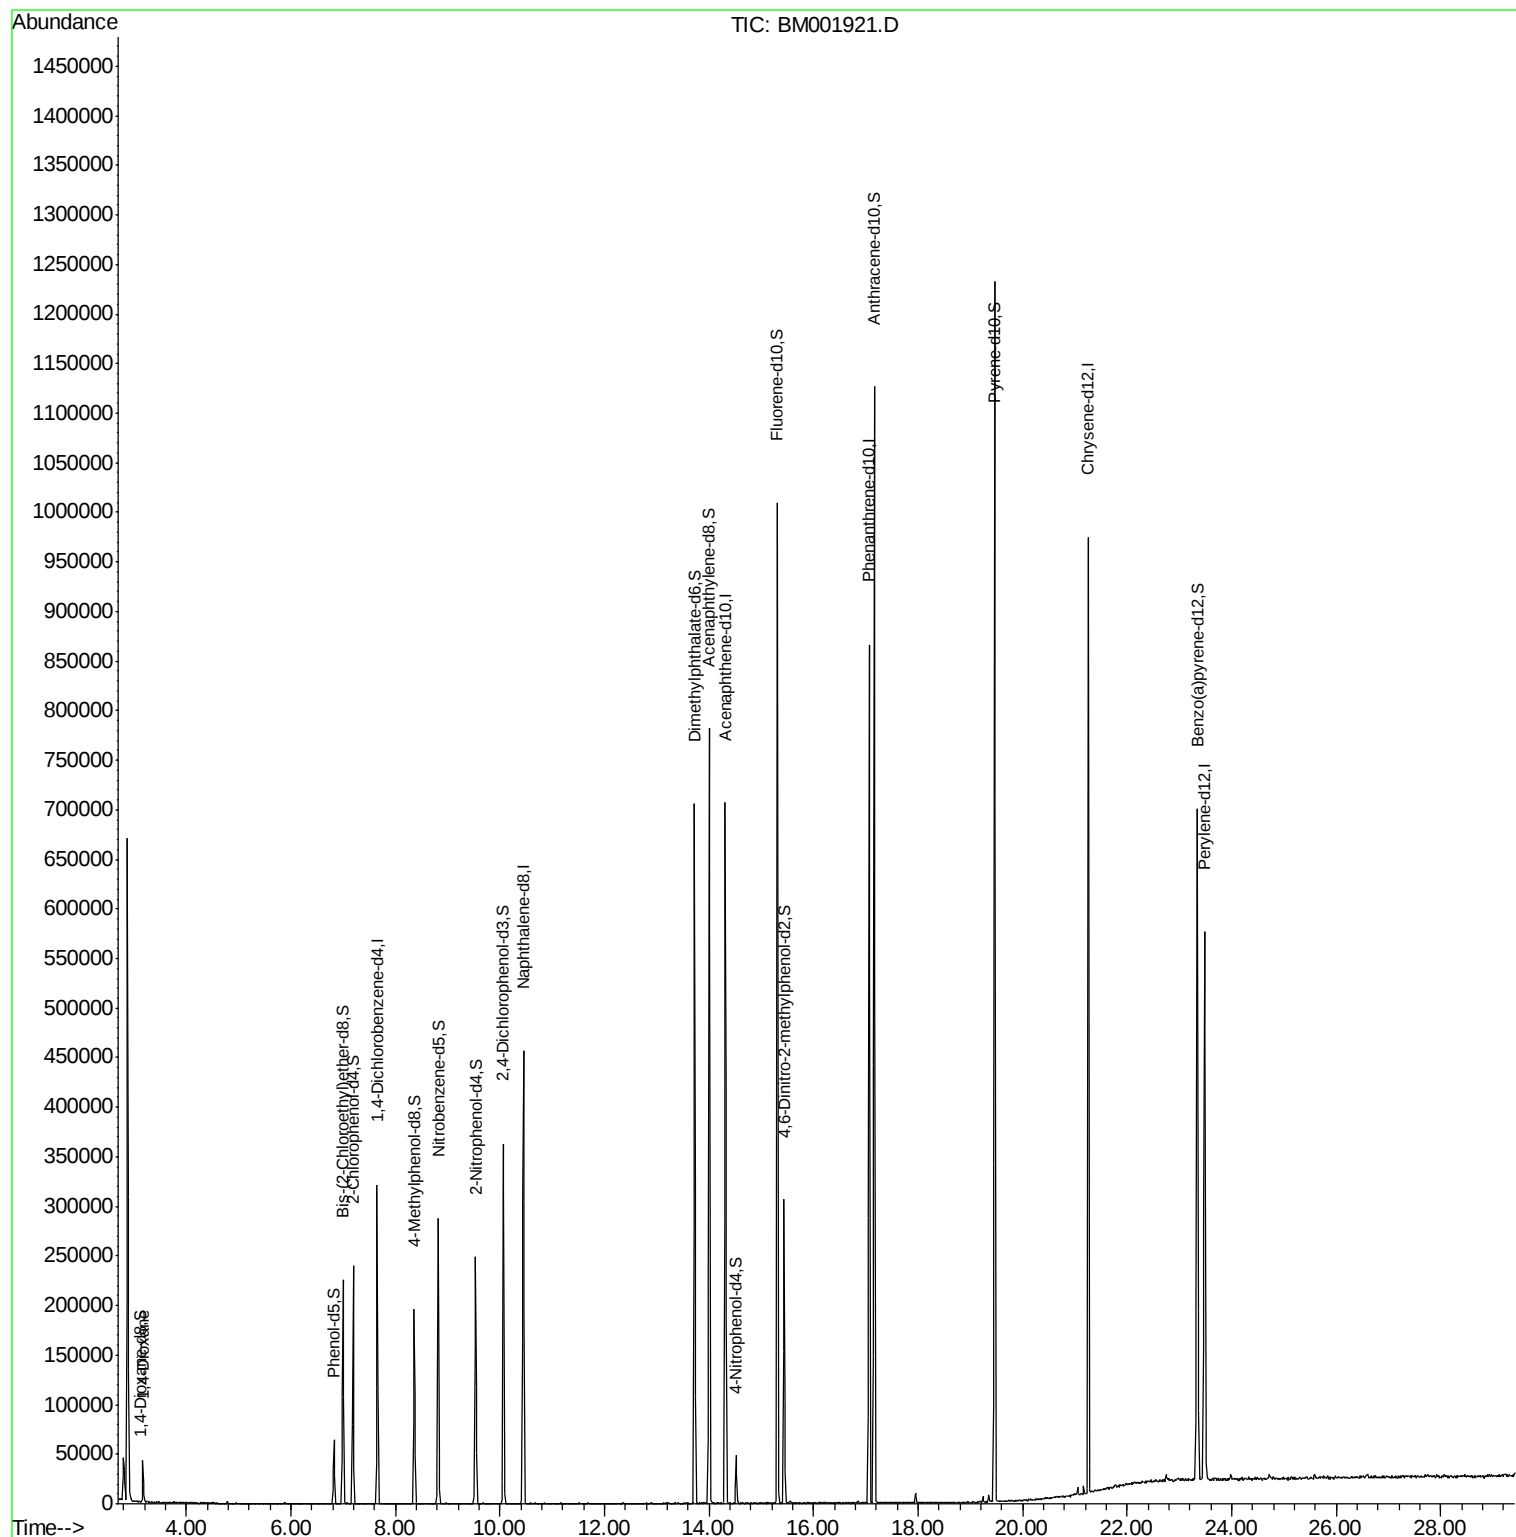

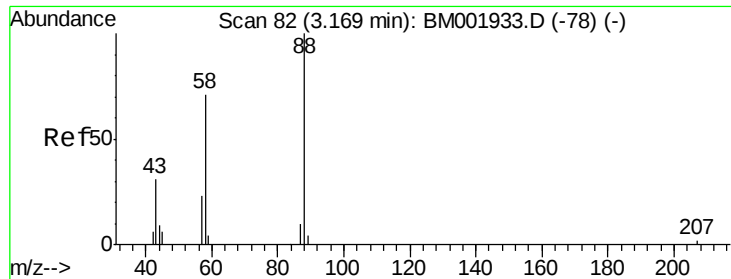

#2
 1,4-Dioxane
 Concen: 10.88 ng/uL
 RT: 3.17 min Scan# 82
 Delta R.T. -0.00 min
 Lab File: BM001921.D
 Acq: 14 Jul 2015 21:29

Instrument :
 BNA_M
 ClientSampleId :
 C01Y3

Tgt Ion: 88 Resp: 19909
 Ion Ratio Lower Upper
 88 100
 43 28.4 22.1 33.1
 58 70.7 54.9 82.3

