

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071515\
 Data File : BM001930.D
 Acq On : 15 Jul 2015 02:57
 Operator : TP/UM
 Sample : G2940-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0211

Quant Time: Jul 15 05:15:08 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 15 05:12:40 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	80338	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	313984	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	186405	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	402245	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	402637	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	389239	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	1937	1.18	ng/uL	0.00
5) Phenol-d5	6.82	99	36716	5.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	86012	24.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	103049	19.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	67314	12.50	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	60295	25.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	68754	26.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	119241	22.70	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.72	166	372989	24.81	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	471452	26.07	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	10691	4.20	ng/ul	0.00
57) Fluorene-d10	15.30	176	332833	25.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	56516	21.70	ng/ul	0.00
70) Anthracene-d10	17.16	188	495644	26.25	ng/ul	0.00
78) Pyrene-d10	19.46	212	526432	28.62	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	473138	24.04	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.17	88	2290	1.32	ng/uL	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071515\
Data File : BM001930.D
Acq On : 15 Jul 2015 02:57
Operator : TP/UM
Sample : G2940-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0211

Quant Time: Jul 15 05:15:08 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 15 05:12:40 2015
Response via : Initial Calibration

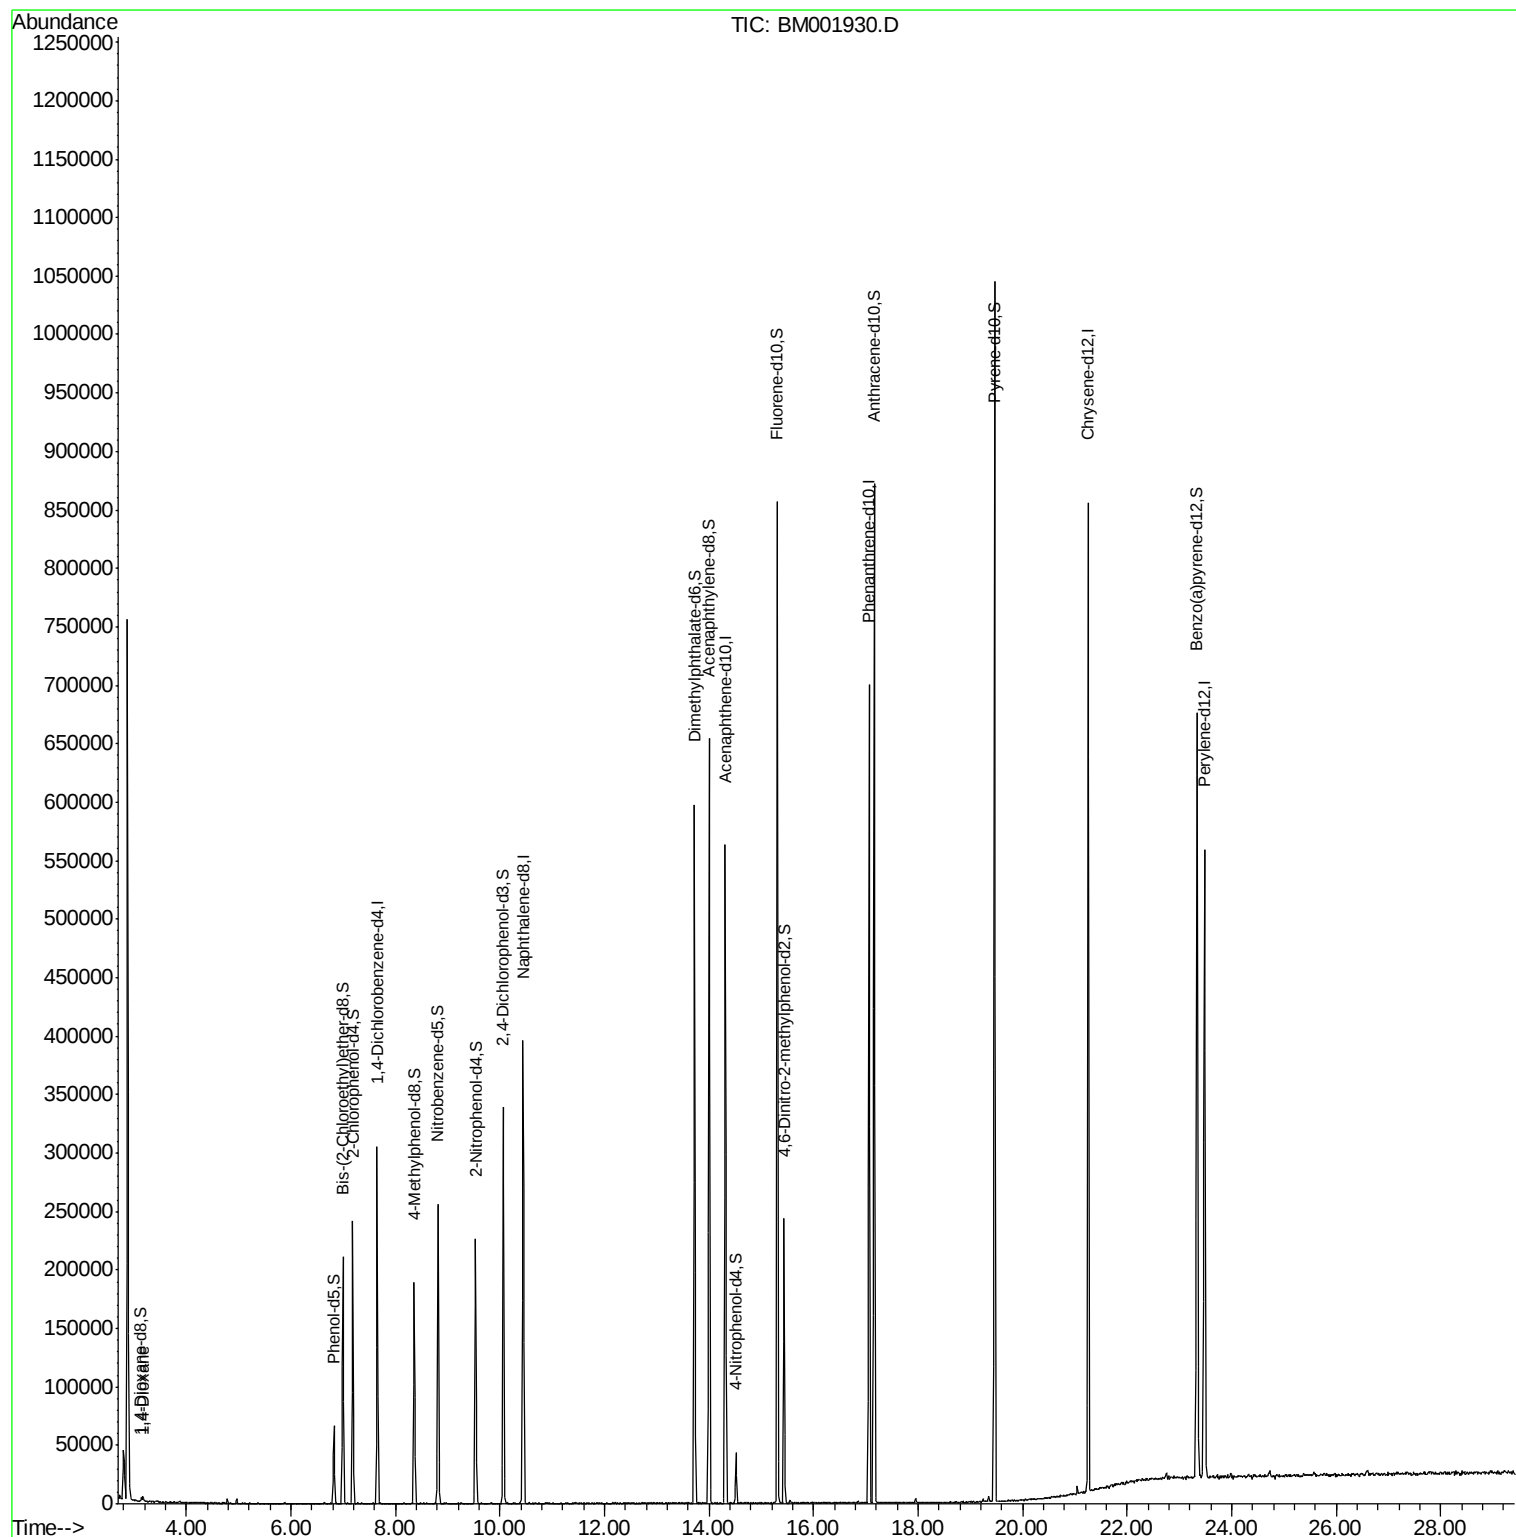

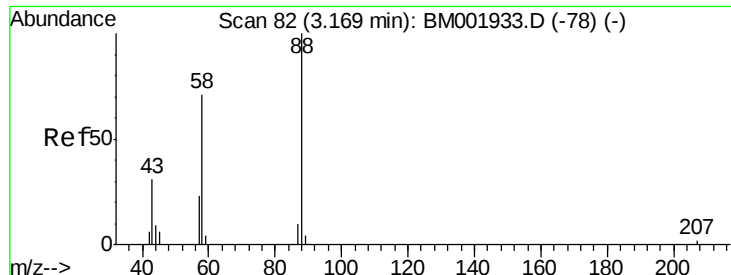

#2
 1,4-Dioxane
 Concen: 1.32 ng/uL
 RT: 3.17 min Scan# 82
 Delta R.T. 0.00 min
 Lab File: BM001930.D
 Acq: 15 Jul 2015 02:57

Instrument :
 BNA_M
 ClientSampleId :
 C0211

Tgt Ion: 88 Resp: 2290
 Ion Ratio Lower Upper
 88 100
 43 25.2 22.1 33.1
 58 56.8 54.9 82.3

