

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071515\
 Data File : BM001934.D
 Acq On : 15 Jul 2015 05:59
 Operator : TP/UM
 Sample : G2940-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0214

Quant Time: Jul 15 07:11:49 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 15 07:11:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	79839	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	342345	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	225655	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	529668	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	565745	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	476651	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	2140	1.31	ng/uL	0.00
5) Phenol-d5	6.82	99	42645	6.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	96632	27.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	116828	22.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	79018	14.76	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	70187	27.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	80636	28.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	141105	24.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	2078	0.35	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	496946	27.30	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	601923	27.50	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	16649	5.40	ng/ul	0.00
57) Fluorene-d10	15.30	176	443070	28.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	85465	24.92	ng/ul	0.00
70) Anthracene-d10	17.16	188	703523	28.29	ng/ul	0.00
78) Pyrene-d10	19.46	212	783443	30.32	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	639979	26.55	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.17	88	9792	5.69	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071515\
Data File : BM001934.D
Acq On : 15 Jul 2015 05:59
Operator : TP/UM
Sample : G2940-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0214

Quant Time: Jul 15 07:11:49 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 15 07:11:15 2015
Response via : Initial Calibration

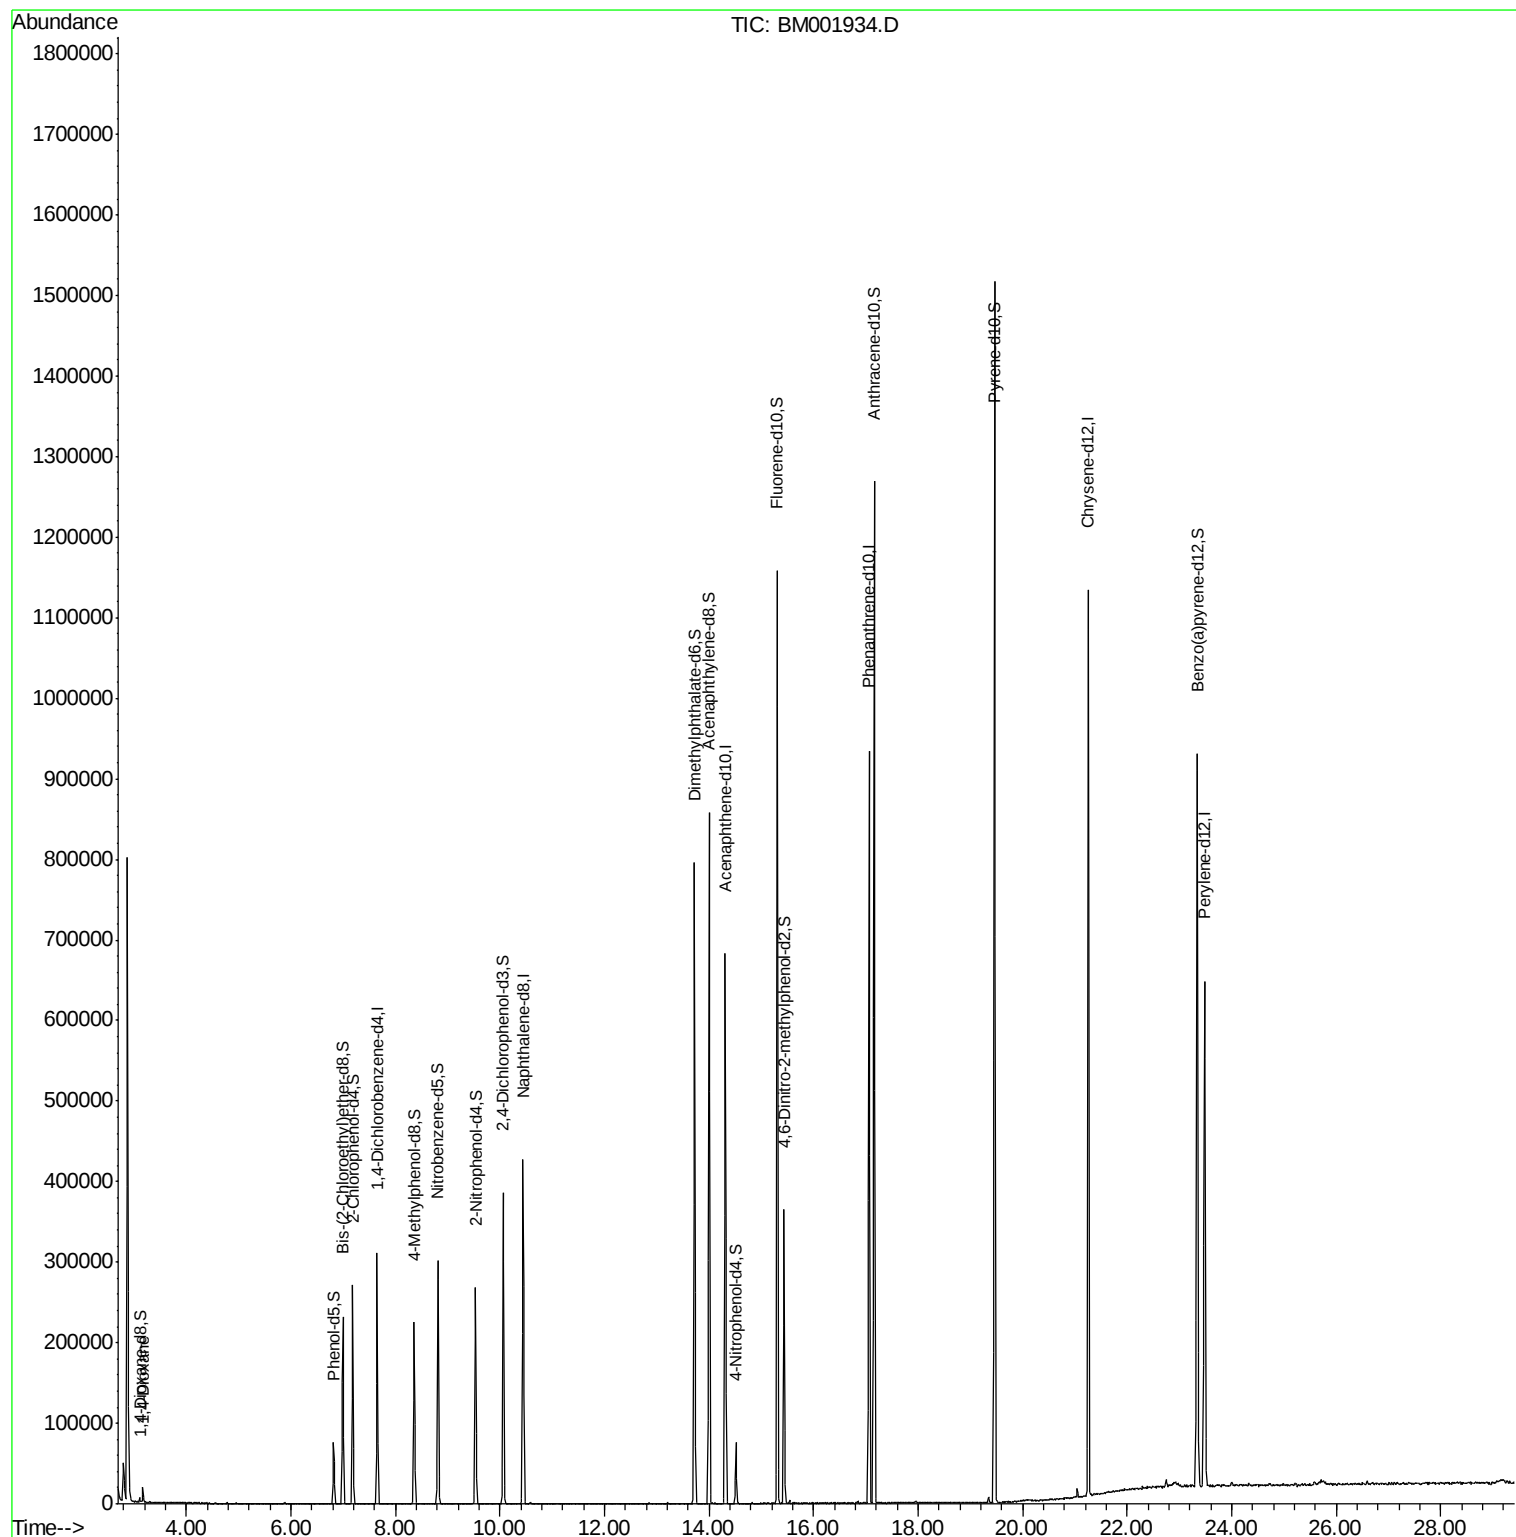

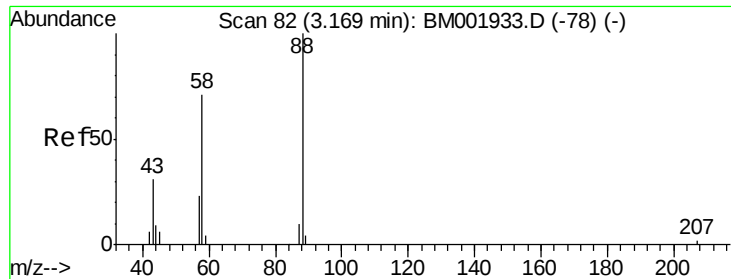

#2
 1,4-Dioxane
 Concen: 5.69 ng/uL
 RT: 3.17 min Scan# 82
 Delta R.T. 0.00 min
 Lab File: BM001934.D
 Acq: 15 Jul 2015 05:59

Instrument :
 BNA_M
 ClientSampleId :
 C0214

Tgt Ion: 88 Resp: 9792
 Ion Ratio Lower Upper
 88 100
 43 28.9 22.1 33.1
 58 65.9 54.9 82.3

