


Data Path : Z:\HPCHEM1\BNA_M\Data\BM071515\
Data File : BM001918.D
Acq On : 14 Jul 2015 18:26
Operator : TP/UM
Sample : DFTPP75
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP75

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042815.M
Title : SVOA CALIBRATION
Last Update : Tue Apr 28 06:36:34 2015

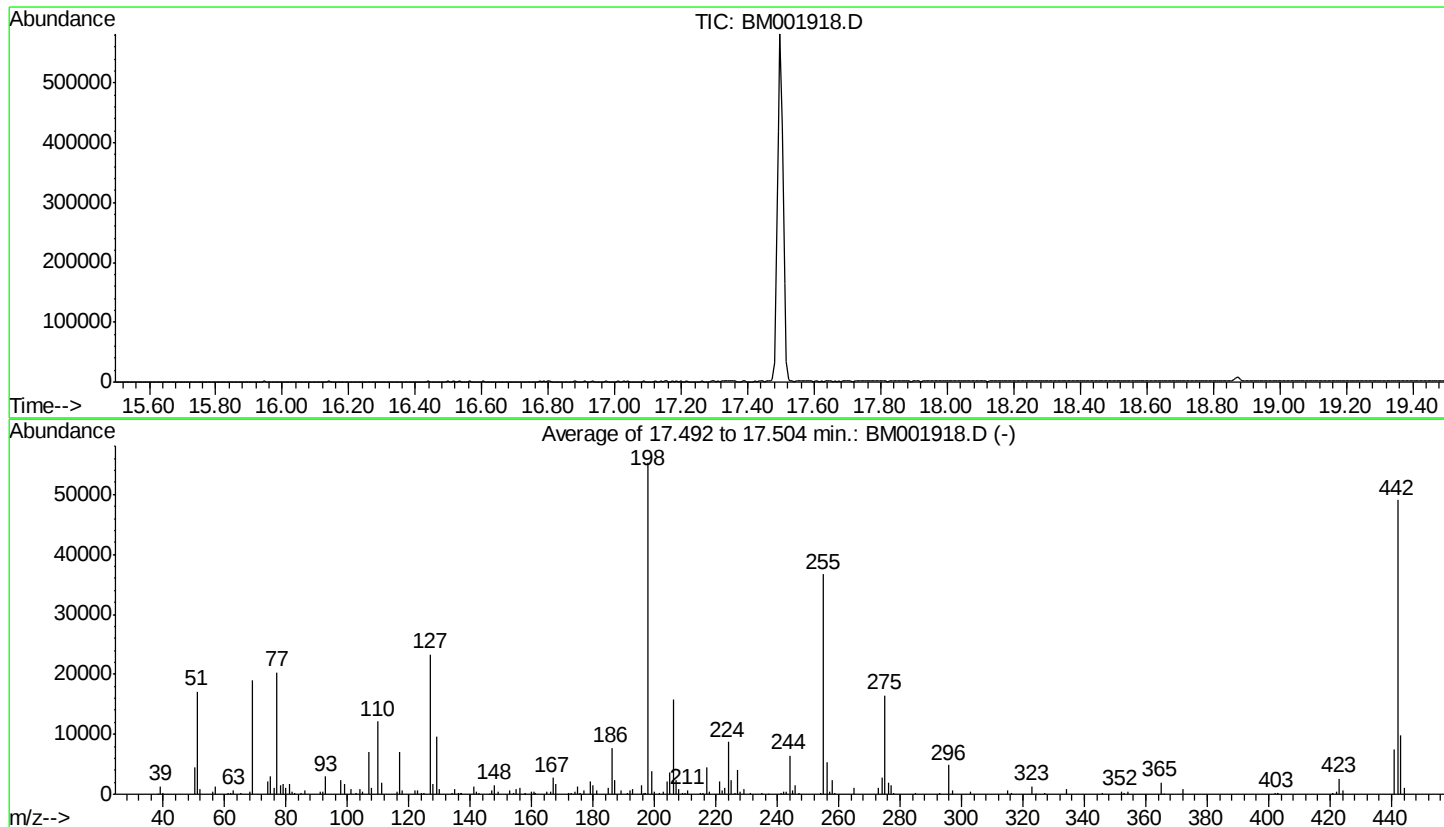

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	17173	PASS
68	69	0.00	2	1.8	335	PASS
69	198	0.00	100	34.5	19091	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	23381	PASS
197	198	0.00	2	0.5	291	PASS
198	198	100	100	100.0	55304	PASS
199	198	5	9	6.9	3805	PASS
275	198	10	60	29.8	16495	PASS
365	198	1	100	3.6	1999	PASS
441	443	0.01	100	77.2	7524	PASS
442	198	50	100	88.7	49066	PASS
443	442	15	24	19.9	9742	PASS

m/z	Abundance
39.00	1334.0
44.00	805.0
50.10	4552.0
51.10	17288.0
52.10	1052.0
56.00	577.0
56.90	1511.0
62.90	674.0
68.00	406.0
69.00	19712.0
74.00	2390.0
75.00	3135.0
76.10	983.0
77.00	20432.0
78.00	1574.0
79.00	1905.0
80.00	1108.0
81.00	1686.0
81.90	432.0
82.90	475.0
86.00	641.0
91.00	438.0
92.00	459.0
93.00	2838.0
98.00	2248.0
99.00	1581.0
101.00	1022.0
104.00	828.0
104.80	659.0
107.00	7003.0
108.00	1097.0
110.00	12127.0
111.00	1985.0
116.00	427.0
117.00	6835.0
117.90	530.0
121.90	537.0
122.90	799.0
123.90	333.0
127.00	22424.0
127.90	1586.0
129.00	9702.0
129.90	937.0
134.00	383.0
135.10	721.0
136.00	341.0
136.80	473.0
141.00	1328.0
141.90	476.0
143.00	366.0
146.90	615.0
147.90	1586.0
149.00	333.0
152.90	551.0
155.10	786.0
156.00	869.0
157.80	330.0
160.00	494.0
161.00	694.0
165.00	450.0
166.00	433.0
167.00	2733.0
168.00	1717.0
171.90	360.0
174.00	577.0
175.00	1110.0
175.90	518.0
177.00	487.0
178.90	2052.0
179.90	1473.0
181.00	687.0
185.00	1076.0
186.00	7188.0
187.00	2159.0
188.90	518.0
191.10	318.0
191.90	615.0
193.00	774.0
195.90	1442.0
196.70	360.0
197.00	324.0
198.00	49744.0
198.90	3310.0
200.00	359.0
203.00	372.0
204.10	1785.0
205.00	2832.0
206.00	13977.0
207.00	2495.0
208.00	665.0
210.90	656.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

217.00	4144.0
217.90	435.0
221.00	1550.0
222.00	473.0
222.90	930.0
224.00	7383.0
225.00	1979.0
226.90	3392.0
227.90	559.0
228.90	976.0
235.00	359.0
242.10	381.0
243.00	329.0
244.00	5719.0
244.90	855.0
245.90	1331.0
255.00	30848.0
256.00	4618.0
257.00	435.0
258.00	1981.0
265.00	857.0
273.00	804.0
274.00	2266.0
275.00	13580.0
276.00	1699.0
277.00	1160.0
296.00	3791.0
297.00	543.0
303.00	354.0
315.00	450.0
323.10	1073.0
334.00	841.0
352.10	453.0
354.00	391.0
364.90	1351.0
366.00	315.0
372.10	528.0
402.90	342.0
423.00	1750.0
424.00	405.0
441.00	4800.0
442.10	31784.0
443.00	6464.0
444.00	645.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

m/z	Abundance
38.00	330.0
39.00	1519.0
44.00	679.0
50.10	5628.0
51.10	21176.0
52.00	1260.0
56.00	645.0
57.00	1555.0
61.00	347.0
62.00	421.0
63.00	933.0
65.10	573.0
68.00	601.0
69.00	23120.0
74.00	2281.0
75.00	3585.0
76.00	1425.0
77.00	24896.0
78.00	1577.0
79.00	2171.0
80.00	1497.0
81.00	1895.0
82.00	428.0
83.00	437.0
85.00	412.0
86.00	615.0
91.00	497.0
92.00	440.0
93.00	3660.0
98.00	2741.0
99.00	1913.0
101.00	1099.0
102.90	355.0
104.00	903.0
105.00	737.0
107.00	8293.0
108.00	1211.0
110.00	14298.0
111.00	2240.0
115.90	444.0
117.00	8515.0
117.90	637.0
122.00	785.0
123.00	873.0
123.90	494.0
125.00	583.0
127.00	29016.0
128.00	2159.0
129.00	11304.0
130.00	1145.0
133.90	436.0
135.00	904.0
135.90	351.0
137.00	525.0
140.90	1501.0
141.90	523.0
143.00	392.0
146.00	326.0
147.00	814.0
148.00	2010.0
148.90	379.0
153.00	630.0
153.90	386.0
155.00	986.0
156.00	1195.0
158.00	398.0
159.90	535.0
160.80	891.0
164.90	719.0
166.00	458.0
167.00	3560.0
168.00	1963.0
173.00	434.0
173.90	575.0
175.00	1515.0
175.90	326.0
176.80	606.0
179.00	2576.0
180.00	2005.0
181.00	629.0
185.00	1357.0
186.00	9215.0
187.00	2950.0
189.00	655.0
191.00	447.0
192.00	940.0
193.00	1049.0
196.00	1892.0
196.80	514.0
197.90	68144.0
199.00	4670.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

199.90	513.0
201.50	385.0
202.90	665.0
204.00	2881.0
205.00	4475.0
206.00	19224.0
207.00	3302.0
208.00	995.0
209.00	390.0
210.10	414.0
211.00	921.0
214.90	388.0
215.90	507.0
217.00	5346.0
218.00	599.0
221.10	2609.0
221.90	829.0
223.00	1052.0
224.00	11200.0
225.00	2837.0
226.10	430.0
227.00	5027.0
227.90	650.0
228.90	1063.0
231.00	418.0
234.90	389.0
237.10	304.0
241.00	368.0
242.10	469.0
242.90	447.0
244.00	7335.0
245.10	1097.0
246.00	1920.0
246.90	342.0
254.10	459.0
255.00	44440.0
256.00	6744.0
257.00	541.0
258.00	2830.0
258.90	342.0
264.90	1265.0
272.90	1137.0
274.00	3386.0
275.00	19816.0
276.10	2561.0
277.00	1666.0
277.90	421.0
284.90	356.0
292.90	325.0
296.00	5734.0
297.00	931.0
303.00	552.0
315.00	671.0
316.10	329.0
323.00	1594.0
327.00	310.0
334.00	890.0
346.00	384.0
351.90	424.0
353.00	438.0
354.00	553.0
365.00	2278.0
372.00	825.0
402.90	376.0
422.00	509.0
423.00	3070.0
424.10	693.0
441.00	9091.0
442.10	58464.0
443.10	11548.0
444.00	1164.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

m/z	Abundance
39.10	1055.0
40.00	350.0
44.00	743.0
50.00	3215.0
51.00	13055.0
52.00	586.0
56.10	378.0
56.90	902.0
63.00	625.0
69.00	14443.0
74.00	1703.0
75.00	2485.0
76.00	642.0
77.00	15570.0
78.10	1054.0
79.00	1194.0
80.00	656.0
81.00	1400.0
82.00	337.0
84.90	317.0
85.90	373.0
90.90	317.0
91.90	368.0
93.00	2188.0
98.00	2012.0
99.00	1525.0
100.90	541.0
103.90	642.0
105.00	385.0
107.00	5702.0
108.00	874.0
110.00	9912.0
110.90	1519.0
116.00	341.0
117.00	5567.0
118.00	505.0
122.00	374.0
122.90	492.0
127.00	18704.0
128.00	1406.0
129.00	7557.0
129.90	681.0
134.90	657.0
136.90	330.0
140.90	974.0
141.90	337.0
146.90	583.0
147.90	1223.0
148.90	387.0
152.90	491.0
154.90	691.0
156.10	909.0
160.00	323.0
161.10	533.0
164.90	433.0
166.10	476.0
167.00	2028.0
167.90	1245.0
173.90	365.0
175.00	1015.0
176.90	536.0
179.00	1601.0
179.90	1200.0
181.00	622.0
185.00	678.0
186.00	6974.0
186.90	2039.0
189.00	493.0
192.10	646.0
192.90	764.0
195.90	1444.0
197.10	439.0
197.90	48024.0
198.90	3435.0
199.90	355.0
204.00	1993.0
205.00	3415.0
206.00	14216.0
207.00	2622.0
208.00	833.0
211.00	436.0
216.00	335.0
216.90	3861.0
217.90	437.0
220.90	2207.0
221.80	537.0
222.90	1115.0
224.00	7591.0
225.00	2067.0
226.00	347.0
226.90	3995.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

227.90	326.0
228.90	802.0
241.90	437.0
242.80	329.0
244.00	6357.0
245.00	1006.0
245.90	1358.0
246.90	409.0
255.00	34776.0
256.00	4722.0
257.00	361.0
258.00	2268.0
258.90	486.0
264.90	940.0
273.00	970.0
274.00	2748.0
275.00	16091.0
276.10	1797.0
276.90	1516.0
293.00	362.0
296.00	5125.0
297.00	684.0
302.90	520.0
314.90	521.0
316.00	383.0
323.00	1184.0
324.10	322.0
326.90	329.0
334.00	930.0
345.90	415.0
352.00	460.0
354.10	451.0
365.00	2370.0
372.00	968.0
402.00	378.0
403.10	497.0
421.00	631.0
422.00	608.0
423.00	2870.0
424.00	1074.0
441.10	8681.0
442.10	56952.0
443.10	11214.0
444.10	1310.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

m/z	Abundance
44.00	756.0
207.00	479.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75