

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
 Data File : BM006454.D
 Acq On : 15 Jul 2016 22:21
 Operator : UM/SJ
 Sample : H3992-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ86

Quant Time: Jul 15 23:21:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 23:20:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	117031	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	510440	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	311182	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	980842	20.00	ng/ul	0.09
75) Chrysene-d12	21.21	240	982256	20.00	ng/ul	-0.01
83) Perylene-d12	23.41	264	1033417	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	6940	2.50	ng/uL	0.00
5) Phenol-d5	6.80	99	267919	27.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	172255	29.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	215775	27.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	217083	28.49	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	103267	26.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	116914	26.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	205992	24.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	295945	34.31	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	696321	27.34	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	841897	26.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	106155	23.99	ng/ul	0.00
57) Fluorene-d10	15.27	176	611993	27.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	91725	16.17	ng/ul	0.00
70) Anthracene-d10	17.12	188	980023	21.14	ng/ul	0.00
76) Pyrene-d10	19.42	212	1203159	27.02	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1406517	29.76	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.73	163	303379	11.74	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006454.D
Acq On : 15 Jul 2016 22:21
Operator : UM/SJ
Sample : H3992-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ86

Quant Time: Jul 15 23:21:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 23:20:22 2016
Response via : Initial Calibration

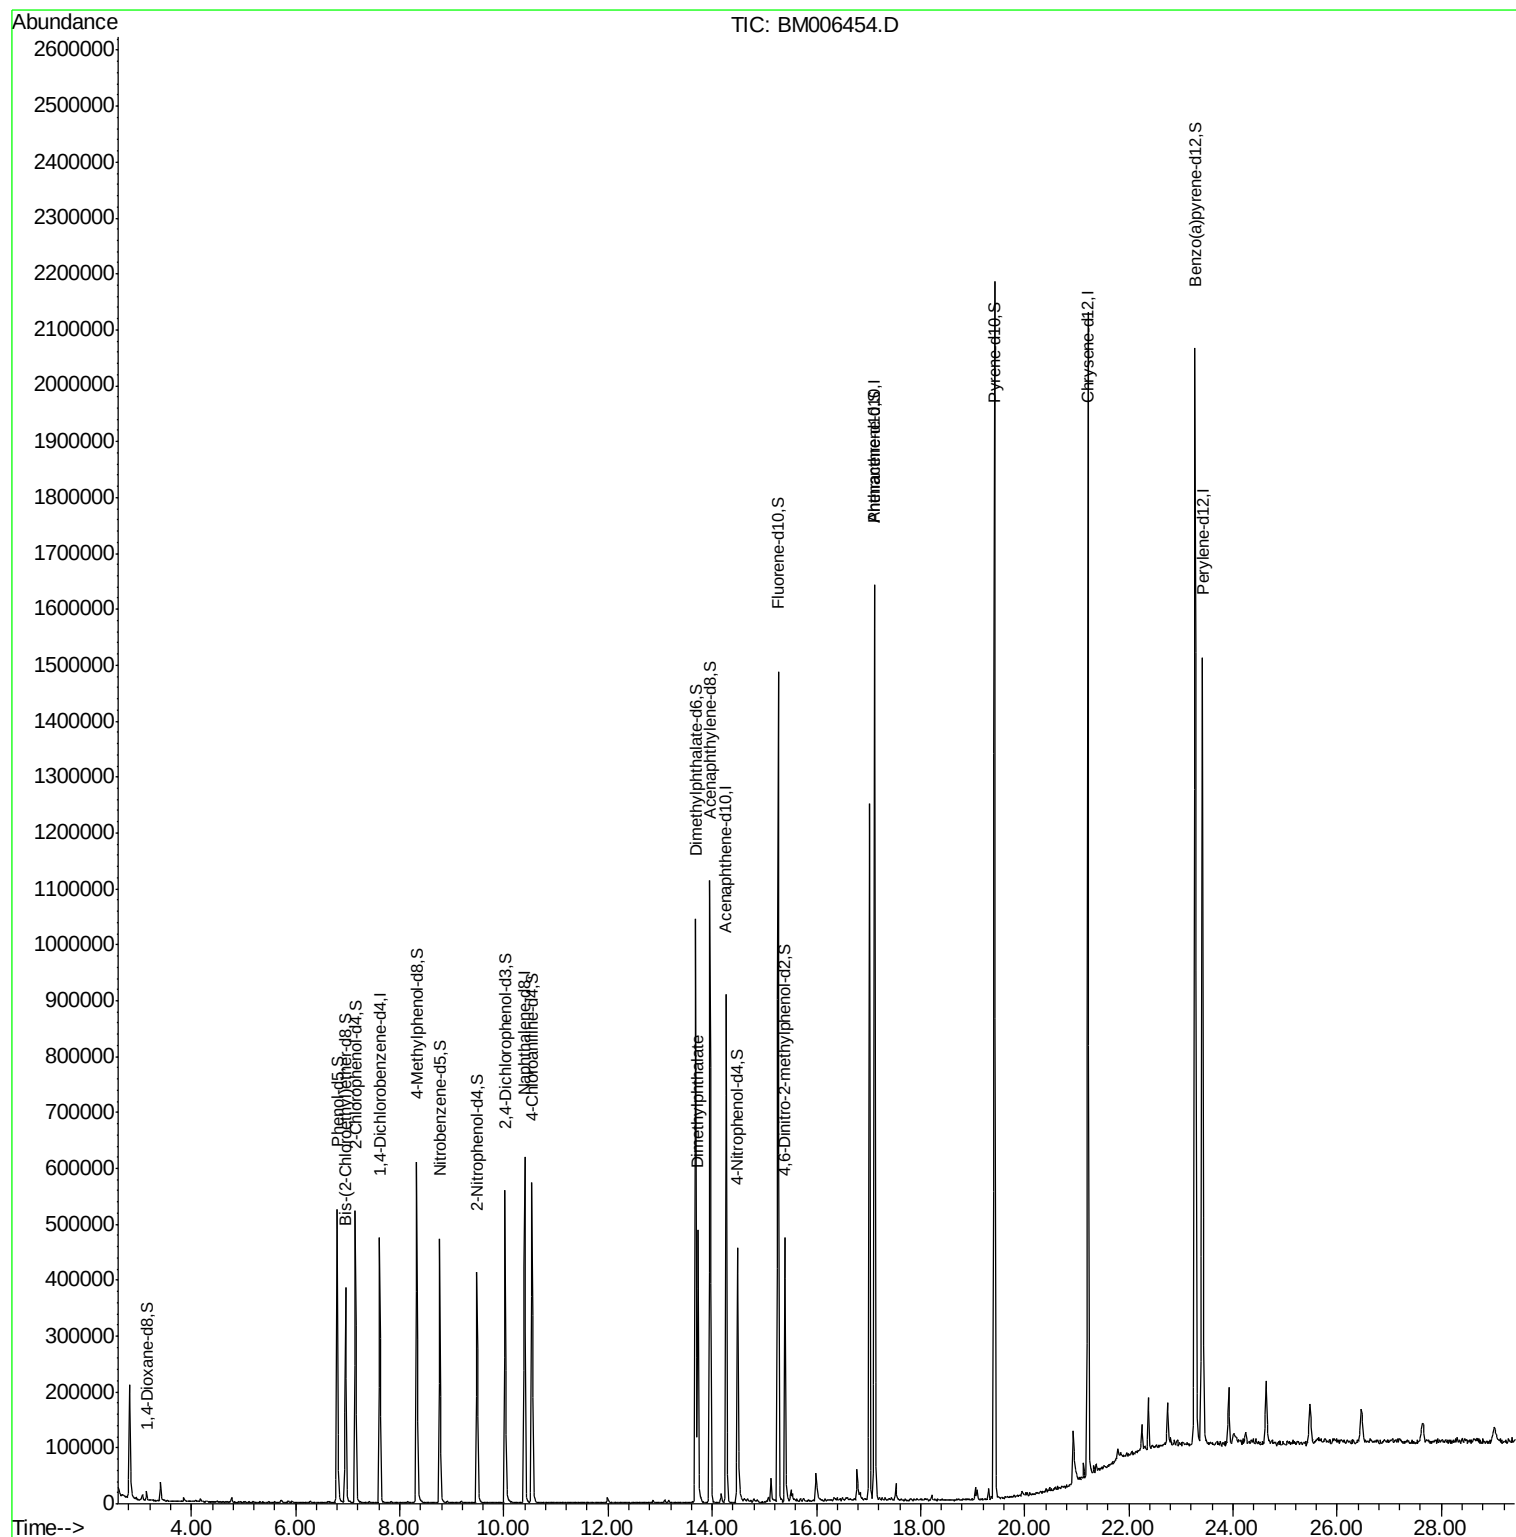

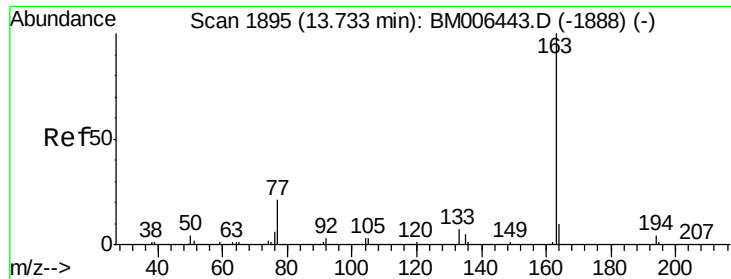

#44

Dimethylphthalate

Concen: 11.74 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BM006454.D

Acq: 15 Jul 2016 22:21

Instrument :

BNA_M

ClientSampleId :

BDJ86


Tgt Ion:163 Resp: 303379

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 9.9 7.8 11.8

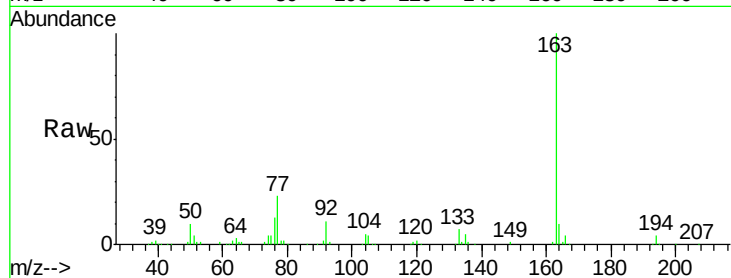

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

