

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
 Data File : BM006458.D
 Acq On : 16 Jul 2016 00:48
 Operator : UM/SJ
 Sample : H3992-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ89

Quant Time: Jul 16 02:25:33 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 23:20:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	134129	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	576959	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	340252	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	836795	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1072734	20.00	ng/ul	-0.01
83) Perylene-d12	23.41	264	1170023	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	5770	1.81	ng/uL	0.00
5) Phenol-d5	6.80	99	241641	21.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	149210	22.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	190177	21.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	194260	22.24	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	93103	21.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	102944	20.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	187849	20.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	269092	27.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	652097	23.42	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	786499	22.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	107230	22.17	ng/ul	0.00
57) Fluorene-d10	15.27	176	579129	23.39	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	90526	18.70	ng/ul	0.00
70) Anthracene-d10	17.12	188	956861	24.19	ng/ul	0.00
76) Pyrene-d10	19.42	212	1208258	24.84	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1426082	26.65	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.73	163	299076	10.59	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
Data File : BM006458.D
Acq On : 16 Jul 2016 00:48
Operator : UM/SJ
Sample : H3992-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ89

Quant Time: Jul 16 02:25:33 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 23:20:22 2016
Response via : Initial Calibration

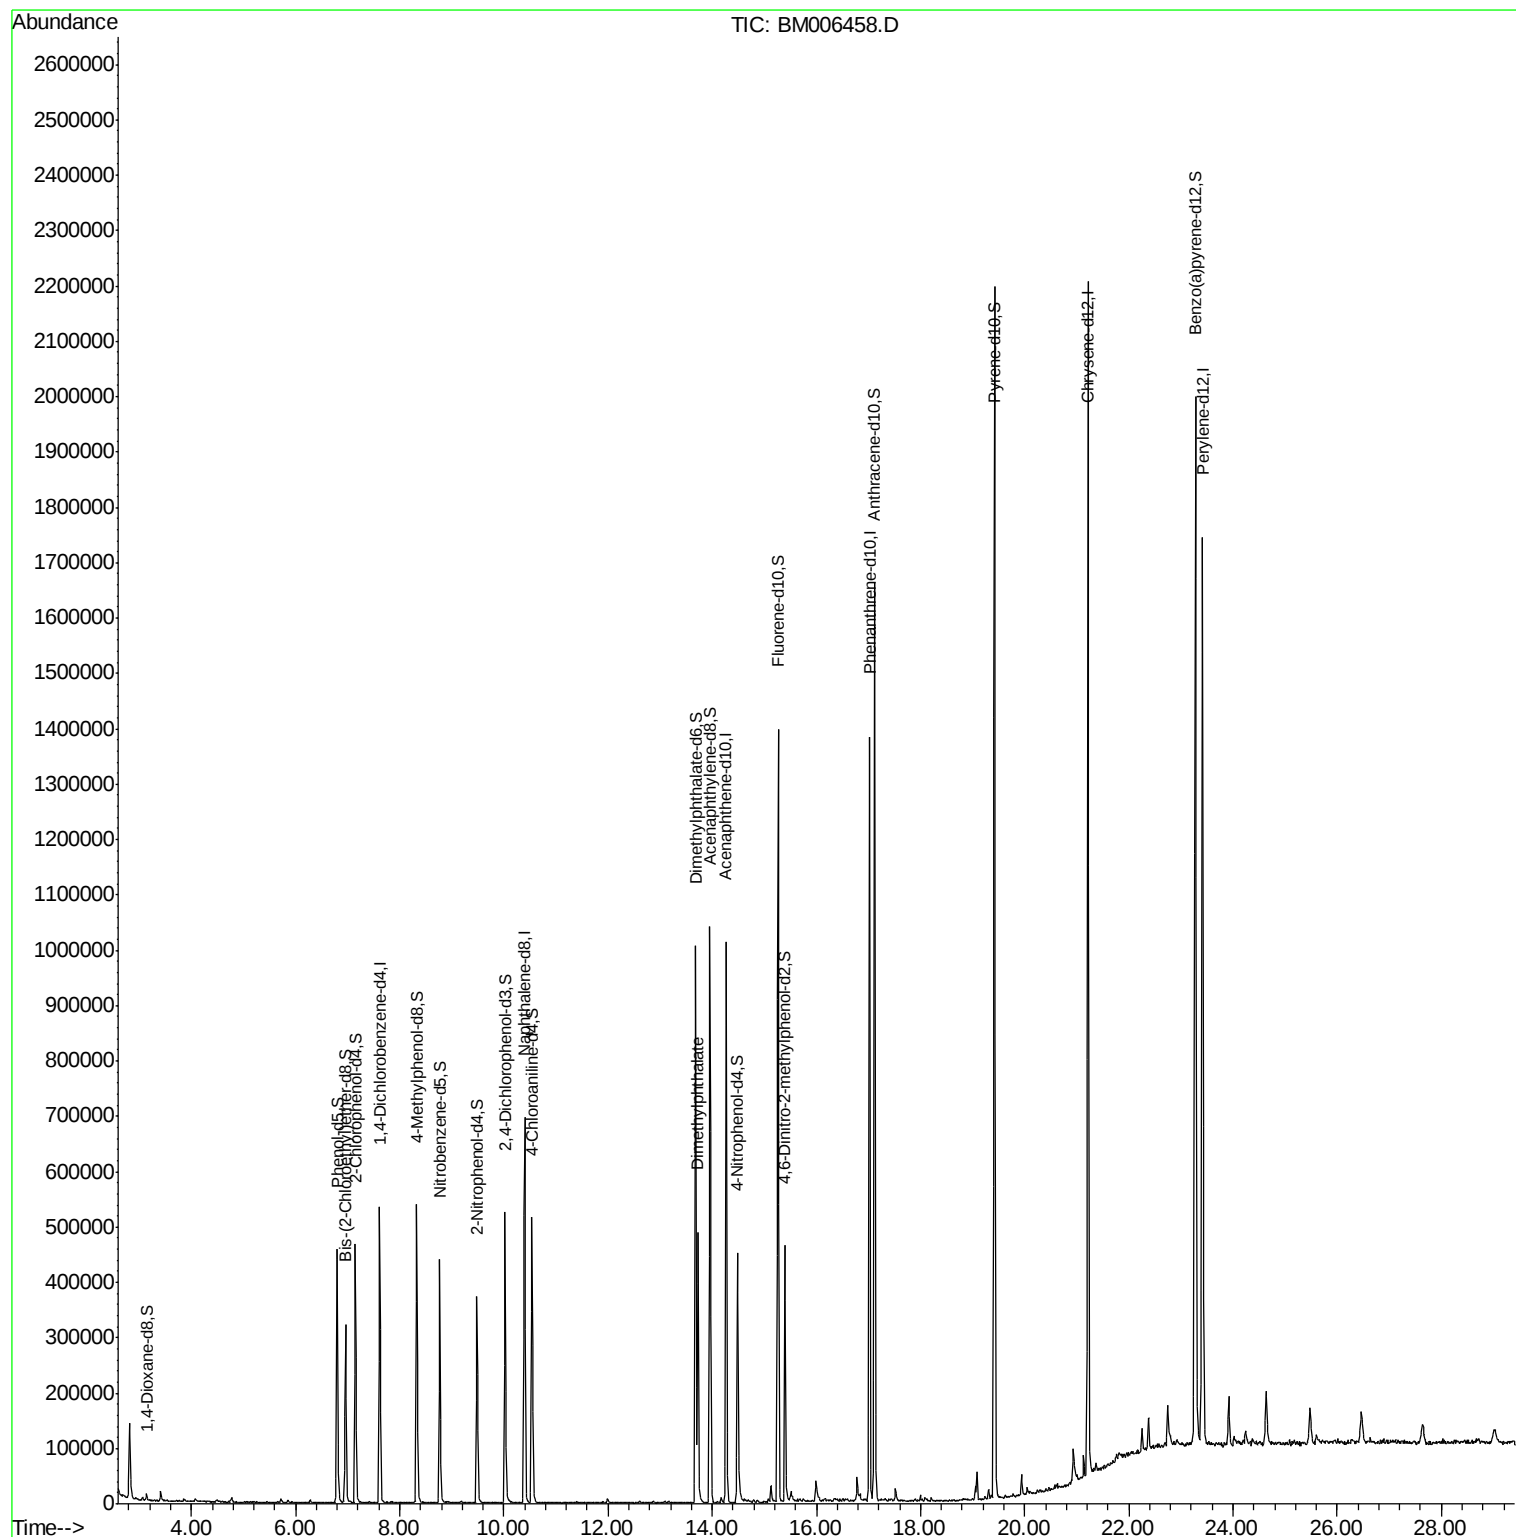

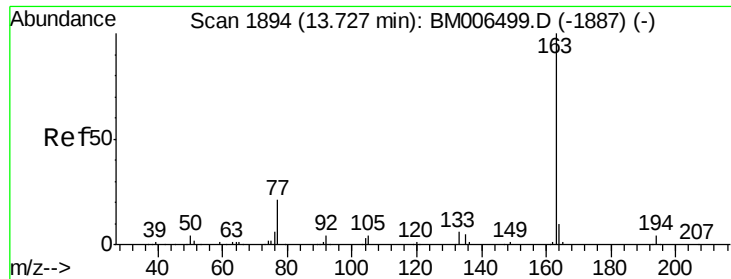

#44

Dimethylphthalate

Concen: 10.59 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BM006458.D

Acq: 16 Jul 2016 00:48

Instrument :

BNA_M

ClientSampleId :

BDJ89


Tot Ion:163 Resp: 299076

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.0

164 9.8 7.8 11.8

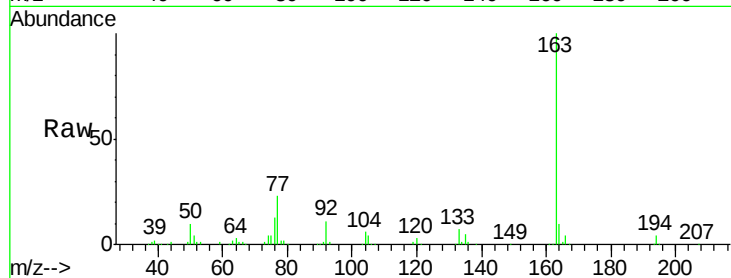

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

