

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
 Data File : BM006444.D
 Acq On : 15 Jul 2016 16:13
 Operator : UM/SJ
 Sample : PB92091BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.798	706	716	732	rBV	551772	904318	21.46%	2.536%
2	6.957	736	743	755	rBV	397705	637382	15.13%	1.787%
3	7.151	770	776	793	rVB	560413	897074	21.29%	2.516%
4	7.616	849	855	867	rVB	405678	644703	15.30%	1.808%
5	8.328	968	976	990	rBV	662263	1106761	26.27%	3.104%
6	8.769	1044	1051	1069	rBV	518260	903741	21.45%	2.534%
7	9.487	1166	1173	1185	rBV	458338	785692	18.65%	2.203%
8	10.022	1257	1264	1279	rBV	600289	1100861	26.13%	3.087%
9	10.398	1321	1328	1339	rBV	520348	893359	21.20%	2.505%
10	10.539	1345	1352	1366	rBV	398546	731152	17.35%	2.050%
11	13.680	1880	1886	1903	rBV	1259575	1934939	45.92%	5.426%
12	13.957	1927	1933	1951	rBV	1290662	2083245	49.44%	5.842%
13	14.269	1980	1986	1996	rBV2	736604	1208824	28.69%	3.390%
14	14.486	2017	2023	2040	rBV	627614	1051643	24.96%	2.949%
15	15.268	2149	2156	2167	rVB	1758782	2678868	63.58%	7.512%
16	15.398	2173	2178	2193	rBV	683130	983200	23.33%	2.757%
17	17.021	2445	2454	2463	rBV2	1031371	1572942	37.33%	4.411%
18	17.121	2464	2471	2482	rVV2	1938901	3071408	72.89%	8.613%
19	19.421	2856	2862	2874	rVB2	2564814	3794862	90.06%	10.642%
20	21.221	3162	3168	3177	rBV	1691281	2121572	50.35%	5.949%
21	23.280	3511	3518	3529	rBV2	2193075	4213528	100.00%	11.816%
22	23.421	3535	3542	3553	rVB	1134309	2136332	50.70%	5.991%
23	23.927	3624	3628	3636	rVB2	52476	102162	2.42%	0.286%
24	24.644	3747	3750	3758	rVB2	53272	101481	2.41%	0.285%


Sum of corrected areas: 35660049

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
Data File : BM006444.D
Acq On : 15 Jul 2016 16:13
Operator : UM/SJ
Sample : PB92091BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

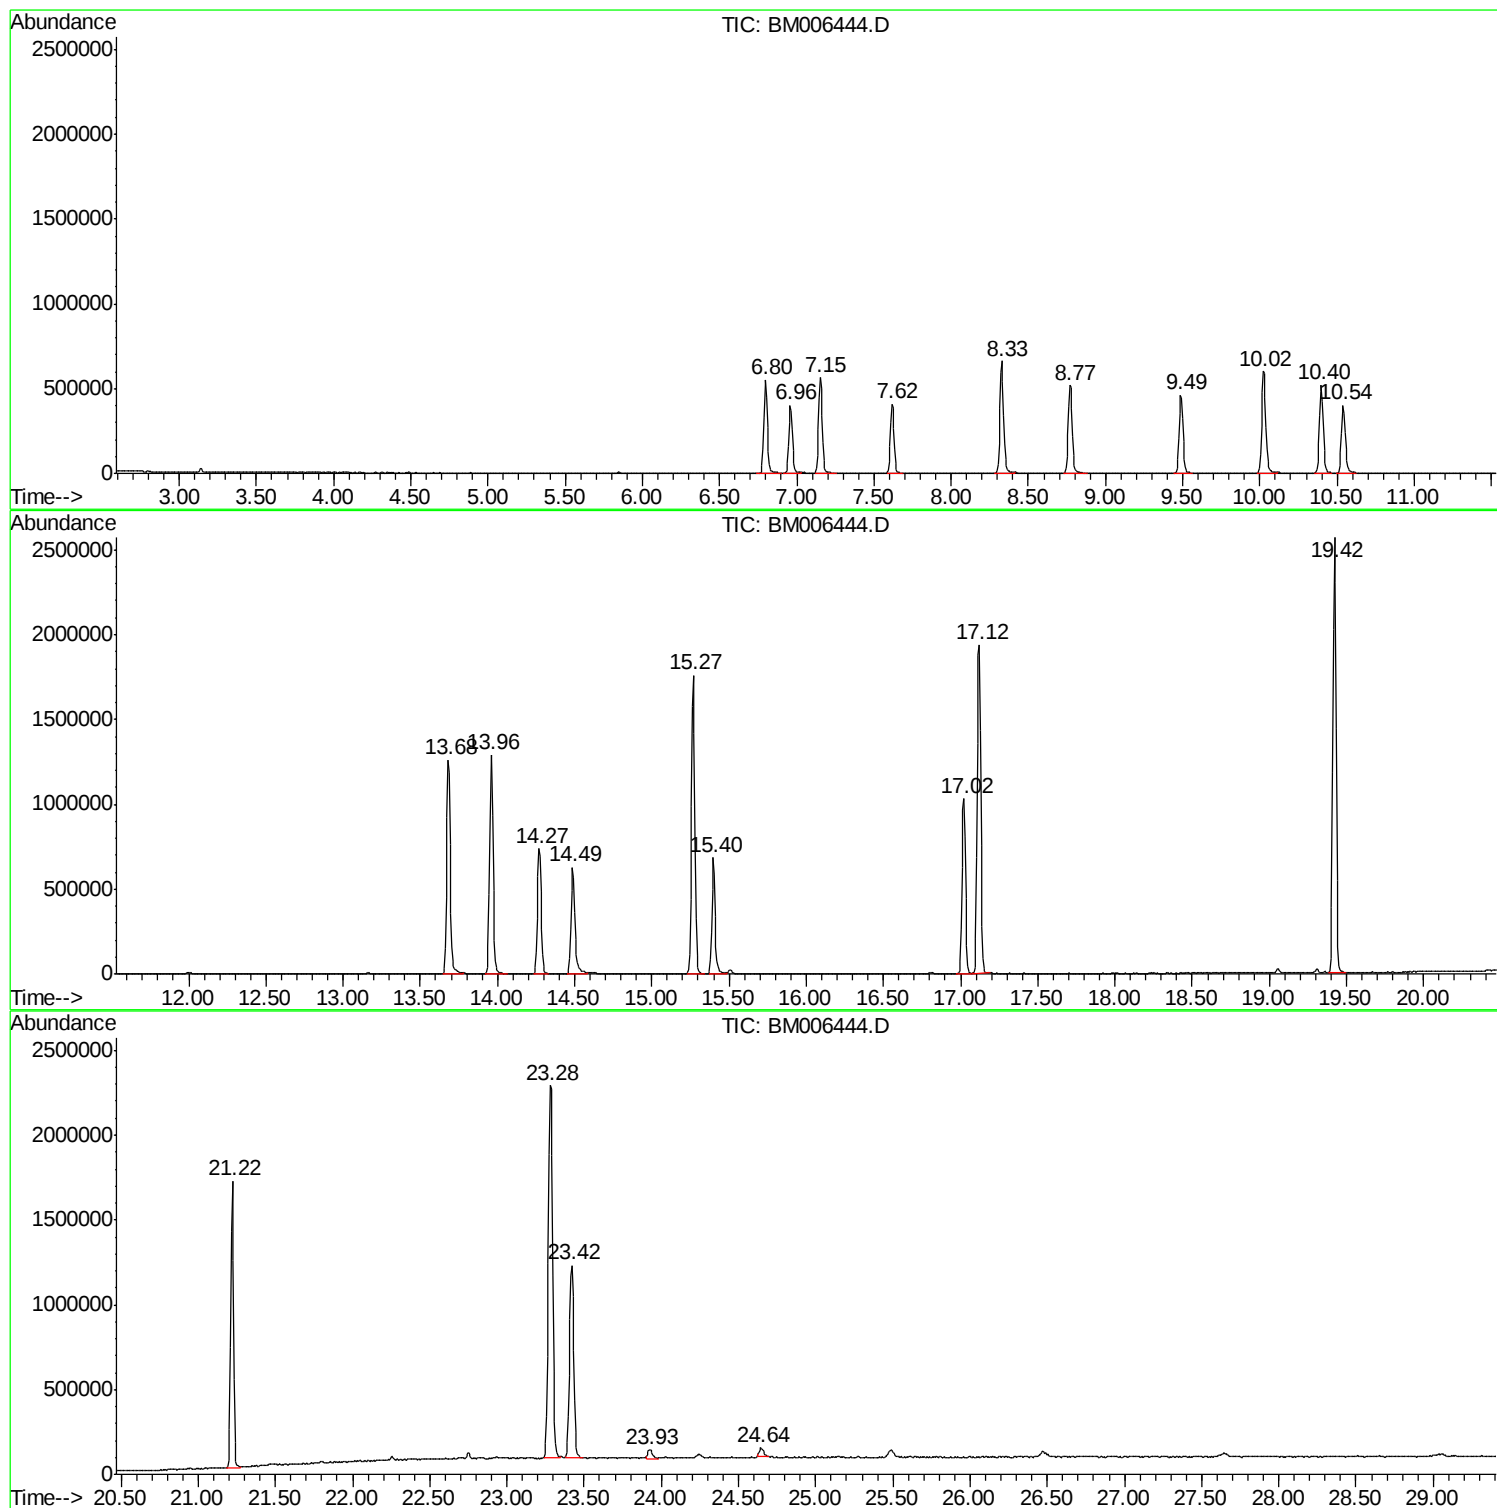

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006444.D
Acq On : 15 Jul 2016 16:13
Operator : UM/SJ
Sample : PB92091BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006444.D
Acq On : 15 Jul 2016 16:13
Operator : UM/SJ
Sample : PB92091BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK91

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc