

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
 Data File : BM006445.D
 Acq On : 15 Jul 2016 16:50
 Operator : UM/SJ
 Sample : PB92126BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.798	709	716	729	rBV	537277	842974	19.69%	2.465%
2	6.957	737	743	756	rBV	372638	594098	13.87%	1.737%
3	7.151	770	776	789	rBV	520549	841140	19.64%	2.459%
4	7.616	849	855	866	rBV	370436	604556	14.12%	1.768%
5	8.328	969	976	996	rBV	616978	1033491	24.13%	3.022%
6	8.775	1045	1052	1066	rBV	480923	847370	19.79%	2.478%
7	9.486	1166	1173	1185	rBV	425357	728739	17.02%	2.131%
8	10.022	1258	1264	1285	rBV	571350	1025717	23.95%	2.999%
9	10.398	1321	1328	1339	rBV	491181	841193	19.64%	2.460%
10	10.539	1345	1352	1363	rBV	371916	667491	15.59%	1.952%
11	13.680	1880	1886	1903	rBV	1154740	1799415	42.02%	5.261%
12	13.962	1927	1934	1944	rBV	1175395	1925308	44.96%	5.629%
13	14.268	1980	1986	2000	rVB3	679176	1124207	26.25%	3.287%
14	14.486	2017	2023	2042	rBV	597522	988664	23.09%	2.891%
15	15.268	2149	2156	2165	rBV	1622825	2506664	58.54%	7.329%
16	15.398	2172	2178	2193	rBV	593077	910664	21.27%	2.663%
17	17.021	2447	2454	2464	rBV	1002344	1494460	34.90%	4.370%
18	17.115	2464	2470	2479	rBV2	1823077	2903443	67.80%	8.489%
19	19.421	2856	2862	2871	rBV2	2453612	3676721	85.86%	10.751%
20	21.221	3162	3168	3177	rBV	1585326	2079337	48.56%	6.080%
21	22.750	3424	3428	3435	rVB4	42305	64853	1.51%	0.190%
22	23.280	3511	3518	3529	rBV2	2172795	4282164	100.00%	12.521%
23	23.421	3535	3542	3555	rVB	1116011	2131520	49.78%	6.232%
24	23.927	3623	3628	3636	rVB	70953	134762	3.15%	0.394%
25	24.650	3746	3751	3757	rVB2	76093	151501	3.54%	0.443%


Sum of corrected areas: 34200452

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
Data File : BM006445.D
Acq On : 15 Jul 2016 16:50
Operator : UM/SJ
Sample : PB92126BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK26

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

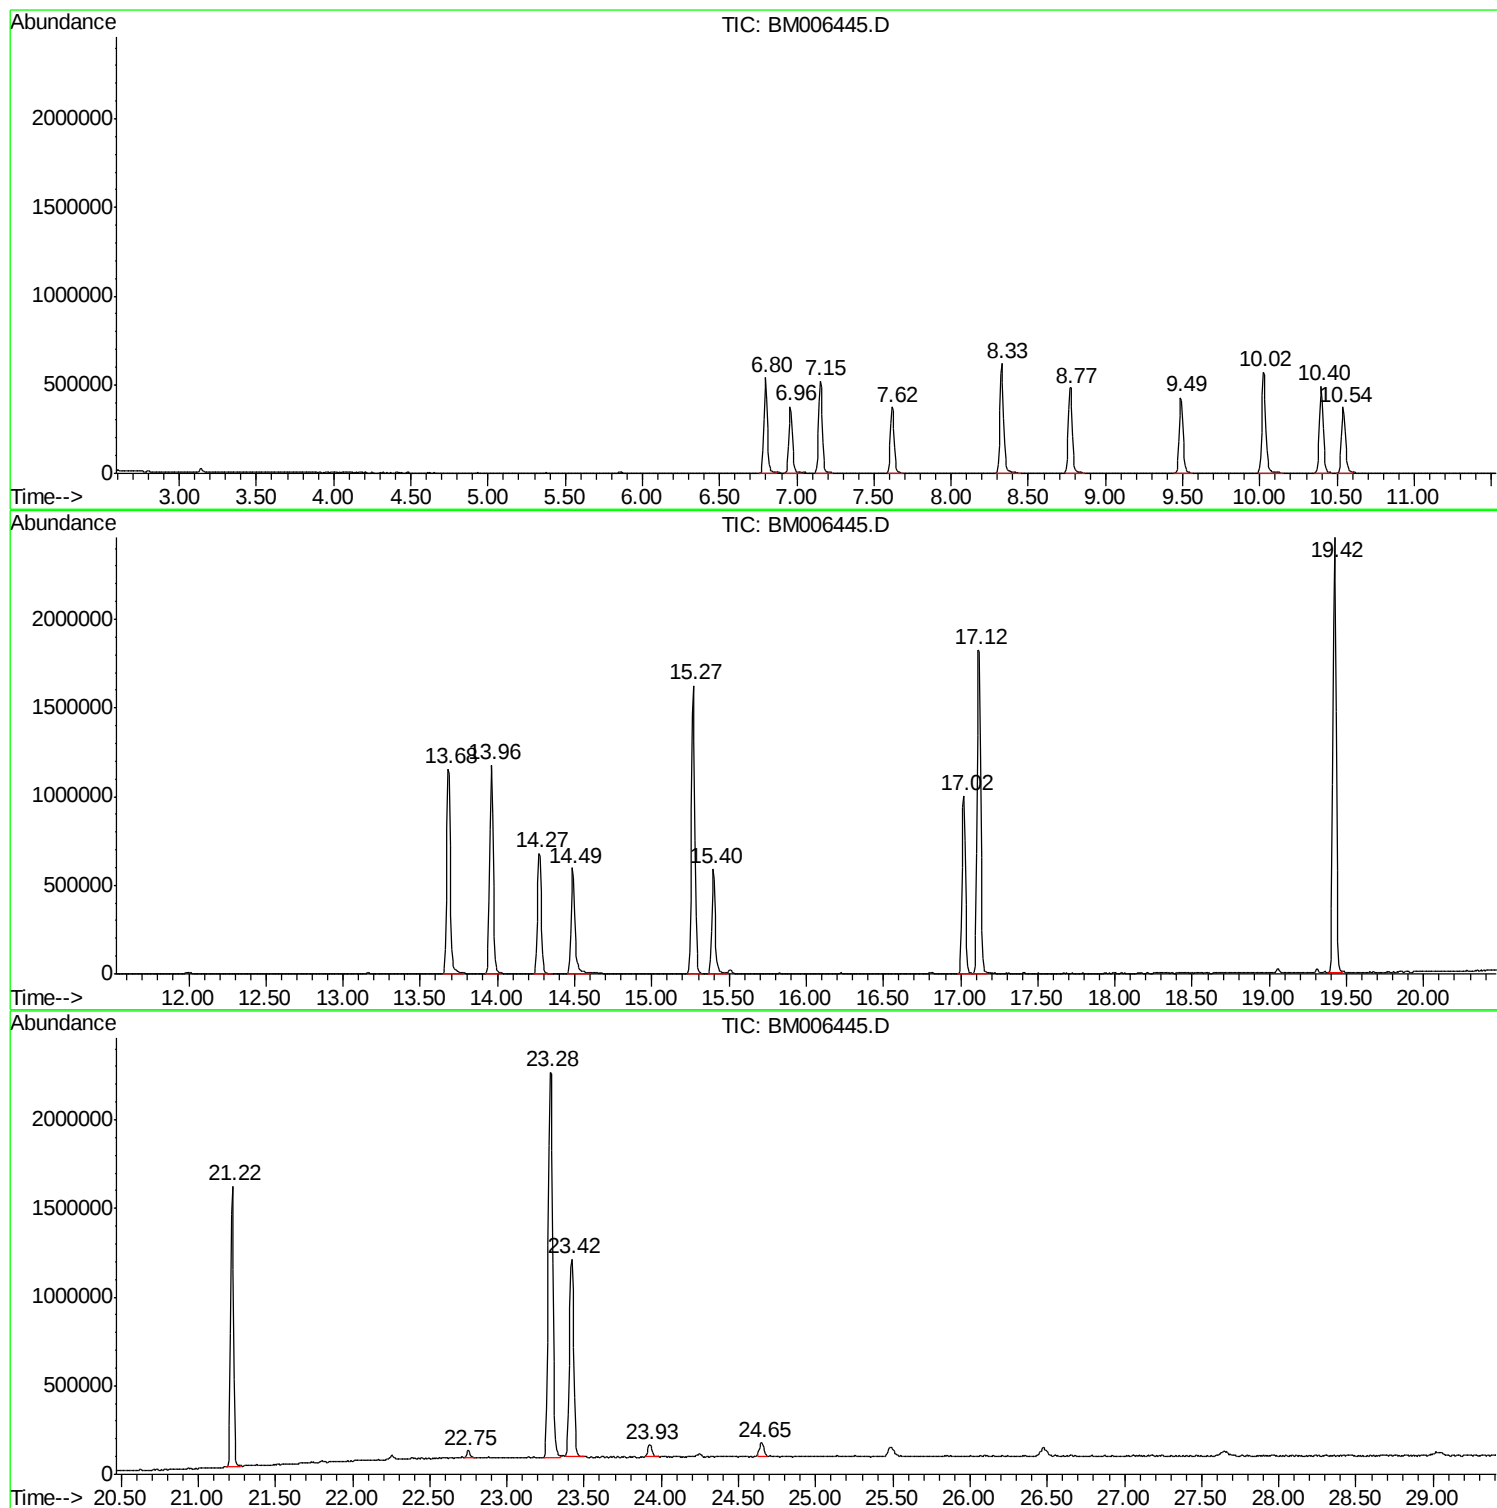

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006445.D
Acq On : 15 Jul 2016 16:50
Operator : UM/SJ
Sample : PB92126BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK26

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006445.D
Acq On : 15 Jul 2016 16:50
Operator : UM/SJ
Sample : PB92126BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK26

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc