

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
 Data File : BM006446.D
 Acq On : 15 Jul 2016 17:27
 Operator : UM/SJ
 Sample : PB92040BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.798	709	716	731	rBV	541521	873359	20.41%	2.480%
2	6.957	737	743	755	rBV	387026	613014	14.32%	1.741%
3	7.151	769	776	791	rBV	540844	868390	20.29%	2.466%
4	7.616	849	855	866	rBV	379834	627775	14.67%	1.783%
5	8.328	969	976	996	rVB	642637	1070036	25.00%	3.039%
6	8.775	1043	1052	1063	rBV	507621	879556	20.55%	2.498%
7	9.486	1166	1173	1187	rBV	449448	762866	17.82%	2.167%
8	10.022	1257	1264	1279	rBV	577220	1057516	24.71%	3.003%
9	10.398	1321	1328	1345	rVB	500050	873604	20.41%	2.481%
10	10.539	1345	1352	1364	rBV	381894	698987	16.33%	1.985%
11	13.680	1880	1886	1903	rBV	1221036	1890950	44.18%	5.371%
12	13.963	1926	1934	1948	rBV	1251164	2010320	46.97%	5.710%
13	14.269	1978	1986	1997	rBV3	719140	1177396	27.51%	3.344%
14	14.486	2017	2023	2046	rBV	616828	1023070	23.90%	2.906%
15	15.268	2149	2156	2167	rVB	1687905	2580559	60.29%	7.329%
16	15.398	2173	2178	2192	rBV	635381	942876	22.03%	2.678%
17	17.021	2448	2454	2464	rBV	1028515	1543029	36.05%	4.382%
18	17.121	2464	2471	2484	rVV	1939639	3001301	70.12%	8.524%
19	19.421	2855	2862	2876	rBV2	2523548	3769022	88.06%	10.705%
20	21.221	3162	3168	3176	rBV	1587873	2131020	49.79%	6.052%
21	22.744	3424	3427	3434	rVB	39553	59171	1.38%	0.168%
22	23.280	3511	3518	3528	rBV2	2200177	4279992	100.00%	12.156%
23	23.421	3535	3542	3550	rVB	1107236	2137300	49.94%	6.070%
24	23.927	3623	3628	3638	rVB2	83660	153447	3.59%	0.436%
25	24.650	3745	3751	3759	rVB3	80346	184936	4.32%	0.525%


Sum of corrected areas: 35209492

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
Data File : BM006446.D
Acq On : 15 Jul 2016 17:27
Operator : UM/SJ
Sample : PB92040BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK40

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

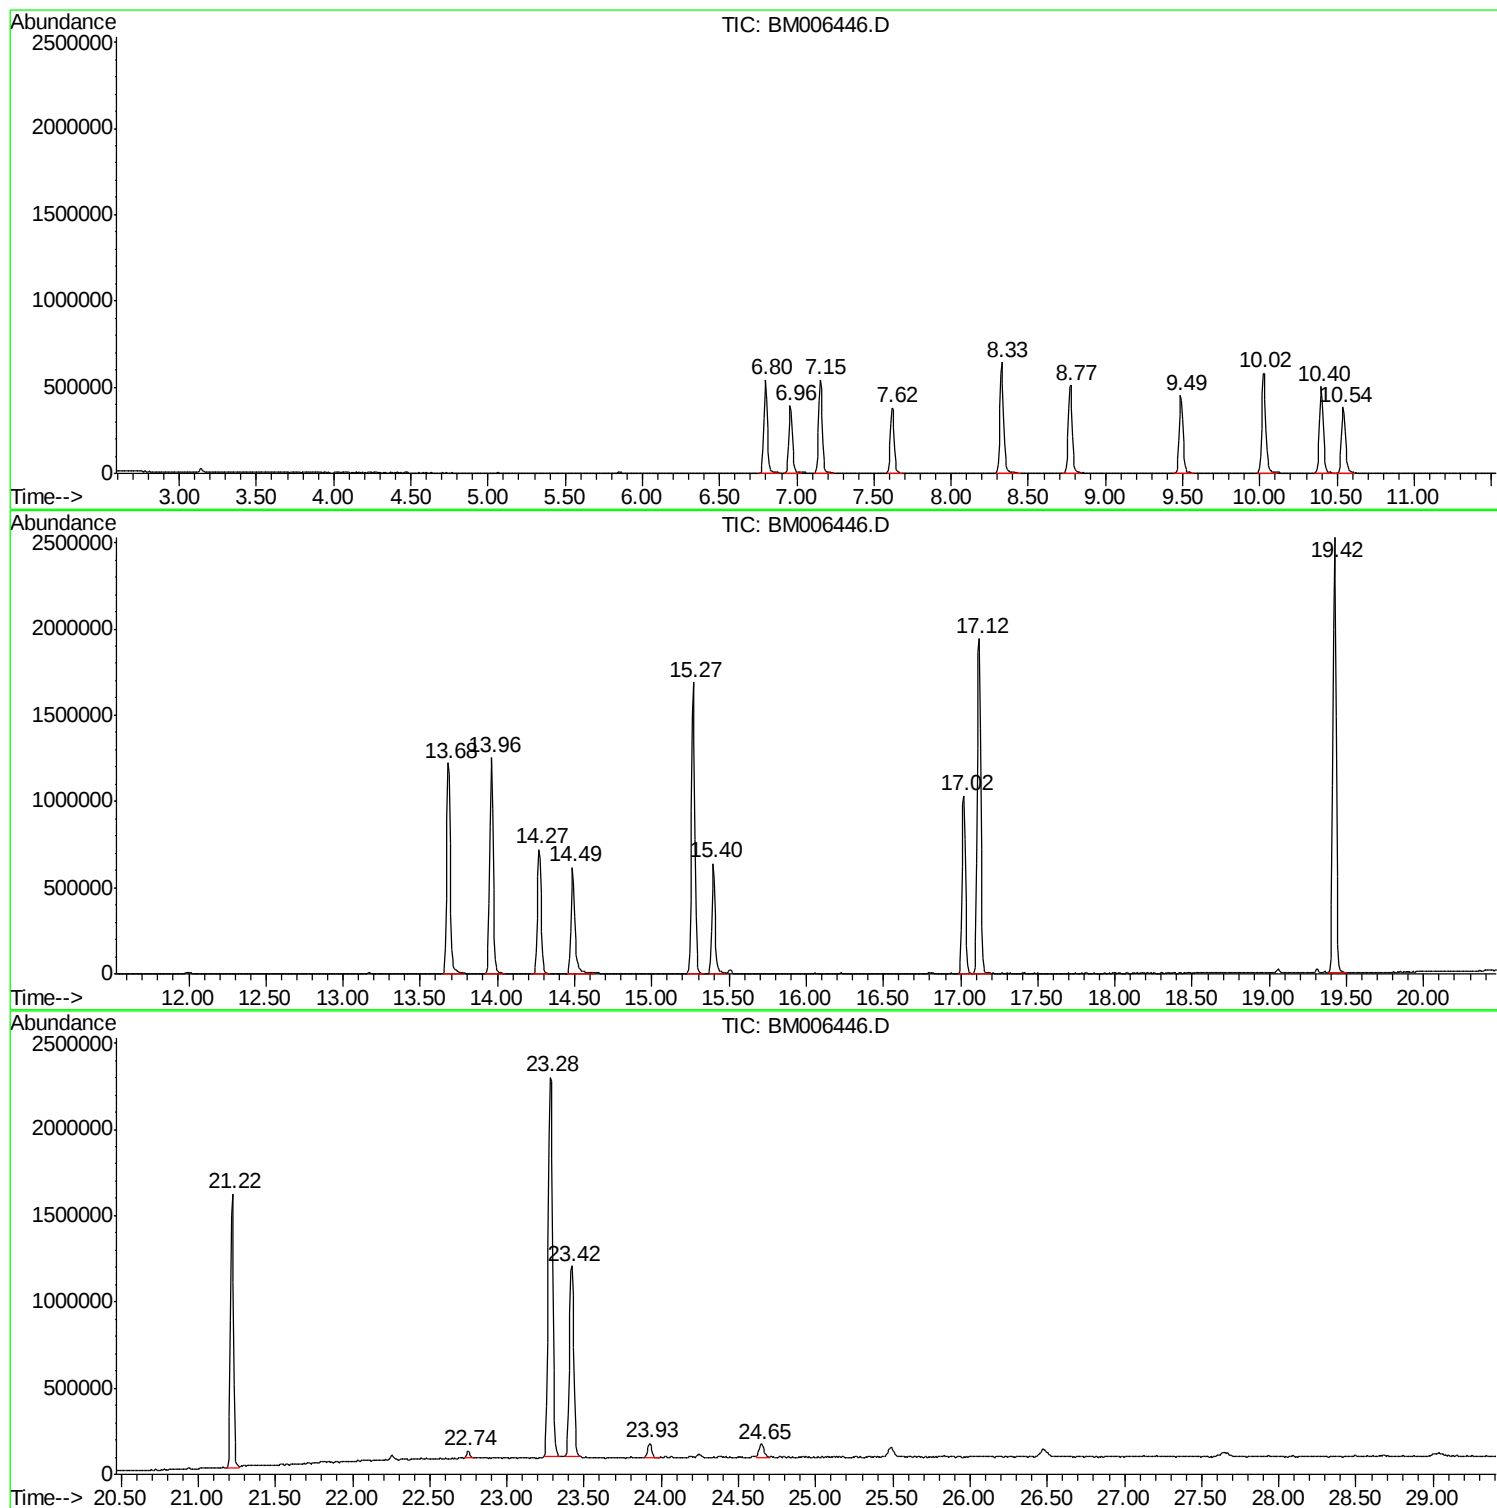

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006446.D
Acq On : 15 Jul 2016 17:27
Operator : UM/SJ
Sample : PB92040BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK40

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006446.D
Acq On : 15 Jul 2016 17:27
Operator : UM/SJ
Sample : PB92040BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK40

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc