

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
 Data File : BM006456.D
 Acq On : 15 Jul 2016 23:35
 Operator : UM/SJ
 Sample : H3992-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.798	709	716	731	rBV	417364	696904	22.77%	2.082%
2	6.957	736	743	756	rBV	307742	499242	16.31%	1.492%
3	7.151	770	776	790	rVB	419716	695112	22.71%	2.077%
4	7.616	848	855	864	rBV	543189	888895	29.05%	2.656%
5	8.328	970	976	988	rBV	490249	809523	26.45%	2.419%
6	8.769	1044	1051	1061	rBV	413759	687345	22.46%	2.054%
7	9.486	1166	1173	1181	rBV	336728	575436	18.80%	1.719%
8	10.022	1257	1264	1285	rBV	468569	854210	27.91%	2.552%
9	10.398	1321	1328	1345	rBV	707240	1264348	41.32%	3.777%
10	10.539	1345	1352	1371	rVV	460506	834413	27.27%	2.493%
11	13.680	1880	1886	1890	rBV	876069	1289698	42.14%	3.853%
12	13.727	1890	1894	1911	rVB	461917	708678	23.16%	2.117%
13	13.957	1923	1933	1946	rBV	993052	1552031	50.72%	4.637%
14	14.268	1979	1986	2000	rVB2	1048770	1713512	55.99%	5.119%
15	14.486	2017	2023	2042	rBV	289188	543891	17.77%	1.625%
16	15.133	2127	2133	2139	rBV	36317	52533	1.72%	0.157%
17	15.268	2149	2156	2164	rBV	1235858	1952887	63.81%	5.835%
18	15.398	2172	2178	2189	rBV	298537	454345	14.85%	1.357%
19	15.998	2273	2280	2288	rBV2	46702	107447	3.51%	0.321%
20	16.786	2410	2414	2420	rBV2	51846	79923	2.61%	0.239%
21	17.021	2447	2454	2464	rBV2	1416821	2195904	71.76%	6.561%
22	17.115	2464	2470	2480	rVB2	1408899	2154632	70.41%	6.437%
23	17.521	2535	2539	2544	rBV	30712	39098	1.28%	0.117%
24	19.421	2856	2862	2876	rVB	1833507	2731865	89.27%	8.162%
25	20.933	3115	3119	3130	rBV3	101228	204063	6.67%	0.610%
26	21.133	3149	3153	3157	rBV	188562	209451	6.84%	0.626%
27	21.215	3161	3167	3181	rBV	2221836	3060258	100.00%	9.143%
28	22.250	3340	3343	3346	rVB3	35473	44648	1.46%	0.133%
29	22.374	3361	3364	3371	rVB	51087	64409	2.10%	0.192%
30	22.744	3423	3427	3432	rVB3	51533	80206	2.62%	0.240%
31	23.274	3510	3517	3531	rVB2	1530565	3026202	98.89%	9.041%
32	23.415	3533	3541	3553	rVB	1510339	3058018	99.93%	9.136%
33	23.915	3622	3626	3636	rVB2	91302	169628	5.54%	0.507%
34	24.638	3744	3749	3756	rVB2	81546	172250	5.63%	0.515%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
Data File : BM006456.D
Acq On : 15 Jul 2016 23:35
Operator : UM/SJ
Sample : H3992-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ88

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION


Sum of corrected areas: 33471005

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
Data File : BM006456.D
Acq On : 15 Jul 2016 23:35
Operator : UM/SJ
Sample : H3992-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ88

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

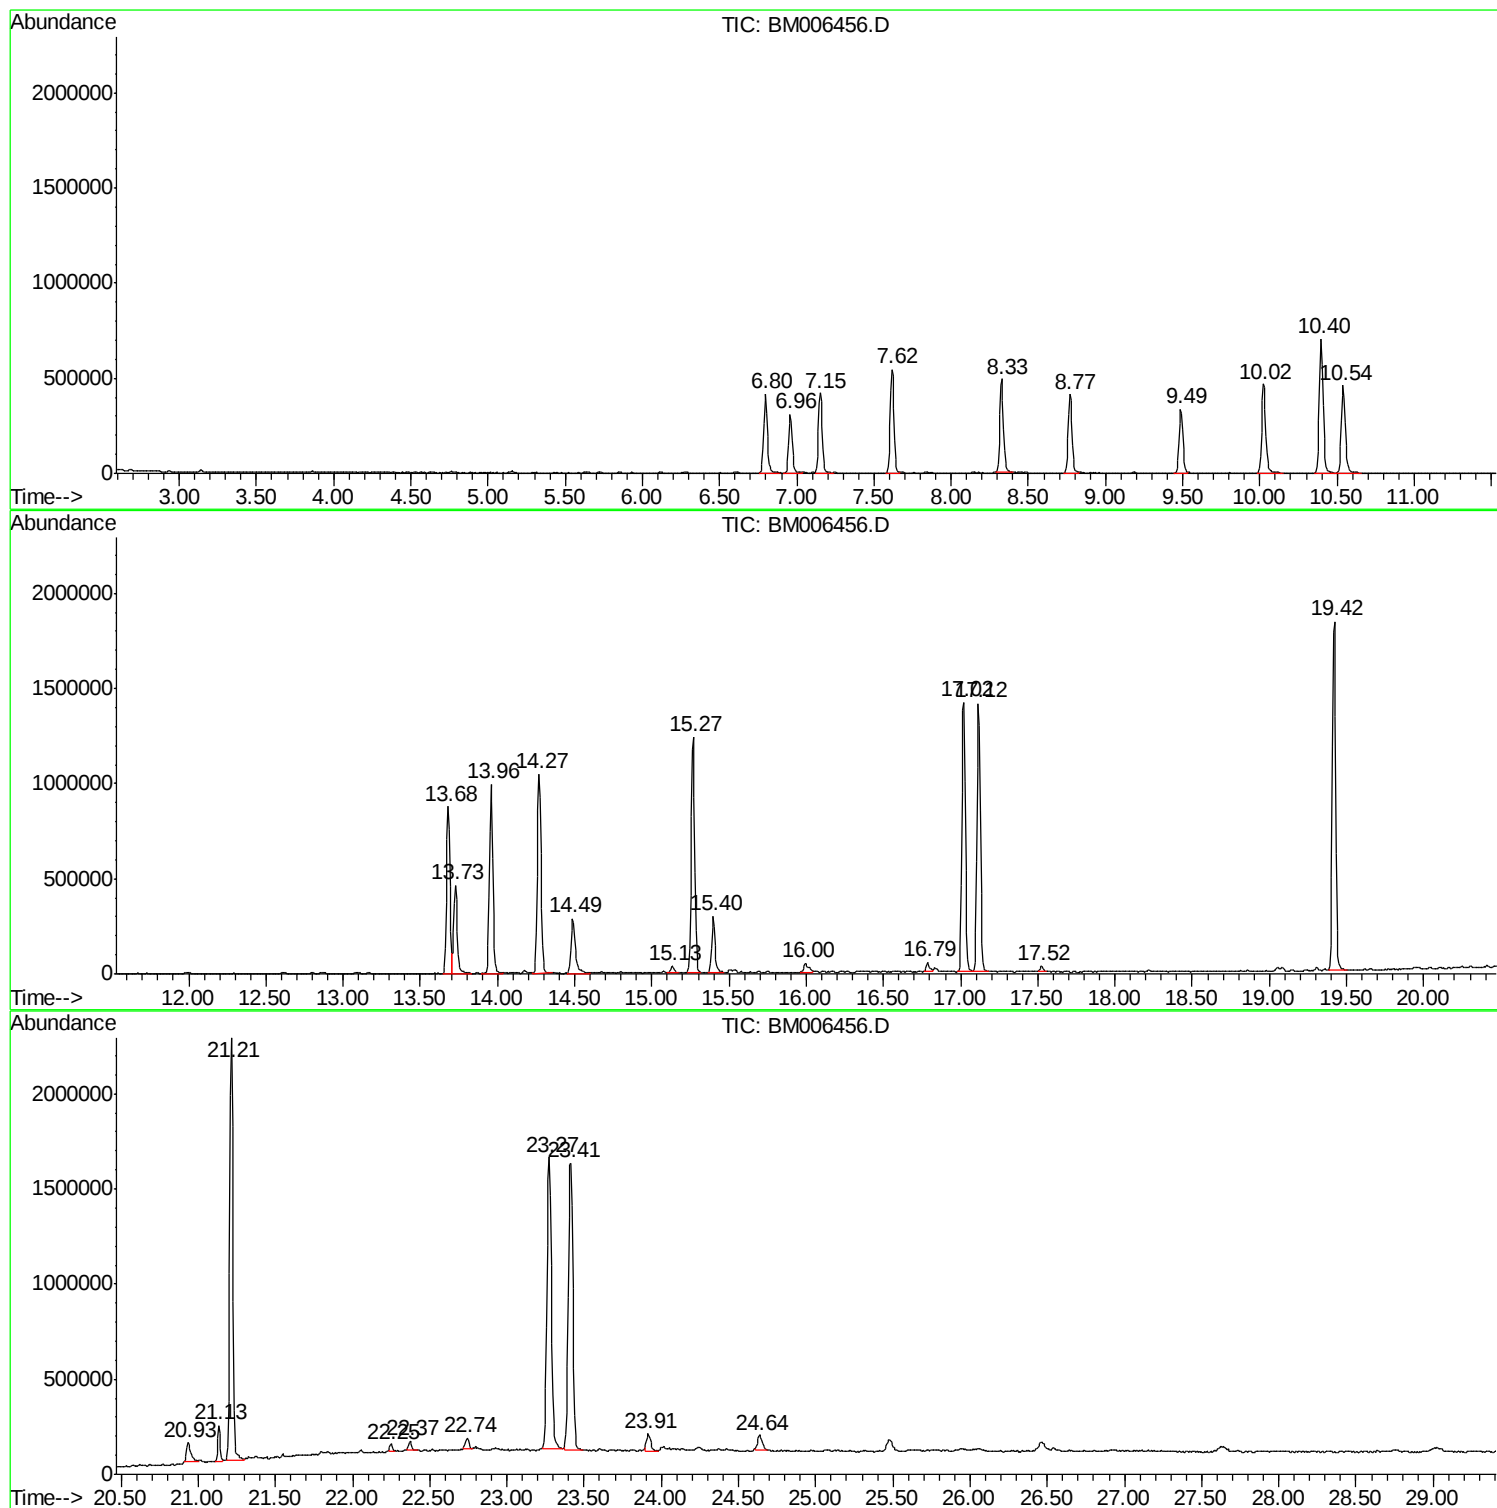

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006456.D
Acq On : 15 Jul 2016 23:35
Operator : UM/SJ
Sample : H3992-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ88

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006456.D
Acq On : 15 Jul 2016 23:35
Operator : UM/SJ
Sample : H3992-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ88

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc