

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
 Data File : BM006466.D
 Acq On : 16 Jul 2016 05:39
 Operator : UM/SJ
 Sample : H3992-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ97

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	709	715	729	rBV	371974	633321	19.57%	1.953%
2	6.957	737	743	756	rBV	278850	437046	13.50%	1.348%
3	7.151	769	776	789	rBV	381048	617498	19.08%	1.904%
4	7.616	847	855	865	rBV	551000	910764	28.14%	2.809%
5	8.322	970	975	992	rVB	443611	758979	23.45%	2.341%
6	8.769	1044	1051	1069	rBV	356571	627159	19.38%	1.934%
7	9.487	1165	1173	1186	rBV	303895	528157	16.32%	1.629%
8	10.022	1257	1264	1276	rBV	424176	763735	23.59%	2.355%
9	10.398	1320	1328	1339	rBV	719036	1313177	40.57%	4.050%
10	10.539	1345	1352	1368	rBV	419822	801775	24.77%	2.473%
11	13.680	1879	1886	1890	rBV	831728	1205091	37.23%	3.716%
12	13.727	1890	1894	1911	rVB	737566	1121129	34.64%	3.458%
13	13.957	1926	1933	1947	rBV	898442	1397331	43.17%	4.309%
14	14.269	1979	1986	1995	rBV2	1074241	1786364	55.19%	5.509%
15	14.486	2017	2023	2035	rBV	313657	548539	16.95%	1.692%
16	15.263	2149	2155	2163	rBV	1165512	1802168	55.68%	5.558%
17	15.398	2171	2178	2189	rBV	316044	488654	15.10%	1.507%
18	17.015	2447	2453	2464	rBV2	1519163	2321234	71.71%	7.159%
19	17.115	2464	2470	2482	rVB2	1376362	2069512	63.94%	6.382%
20	19.080	2801	2804	2810	rVB	34468	47757	1.48%	0.147%
21	19.415	2855	2861	2873	rBV2	1747998	2548201	78.72%	7.859%
22	20.939	3116	3120	3129	rBV8	23043	44650	1.38%	0.138%
23	21.133	3150	3153	3156	rVB2	31591	36381	1.12%	0.112%
24	21.215	3161	3167	3172	rBV	2456665	3230958	99.82%	9.964%
25	22.250	3339	3343	3348	rBV3	38788	60855	1.88%	0.188%
26	22.744	3424	3427	3433	rVB3	45041	73699	2.28%	0.227%
27	23.274	3510	3517	3529	rVV2	1428083	2719469	84.01%	8.387%
28	23.415	3533	3541	3553	rVB	1679071	3236896	100.00%	9.982%
29	23.921	3622	3627	3633	rVB4	75802	138310	4.27%	0.427%
30	24.638	3744	3749	3757	rVB2	72158	157179	4.86%	0.485%


Sum of corrected areas: 32425988

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071516\
Data File : BM006466.D
Acq On : 16 Jul 2016 05:39
Operator : UM/SJ
Sample : H3992-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ97

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

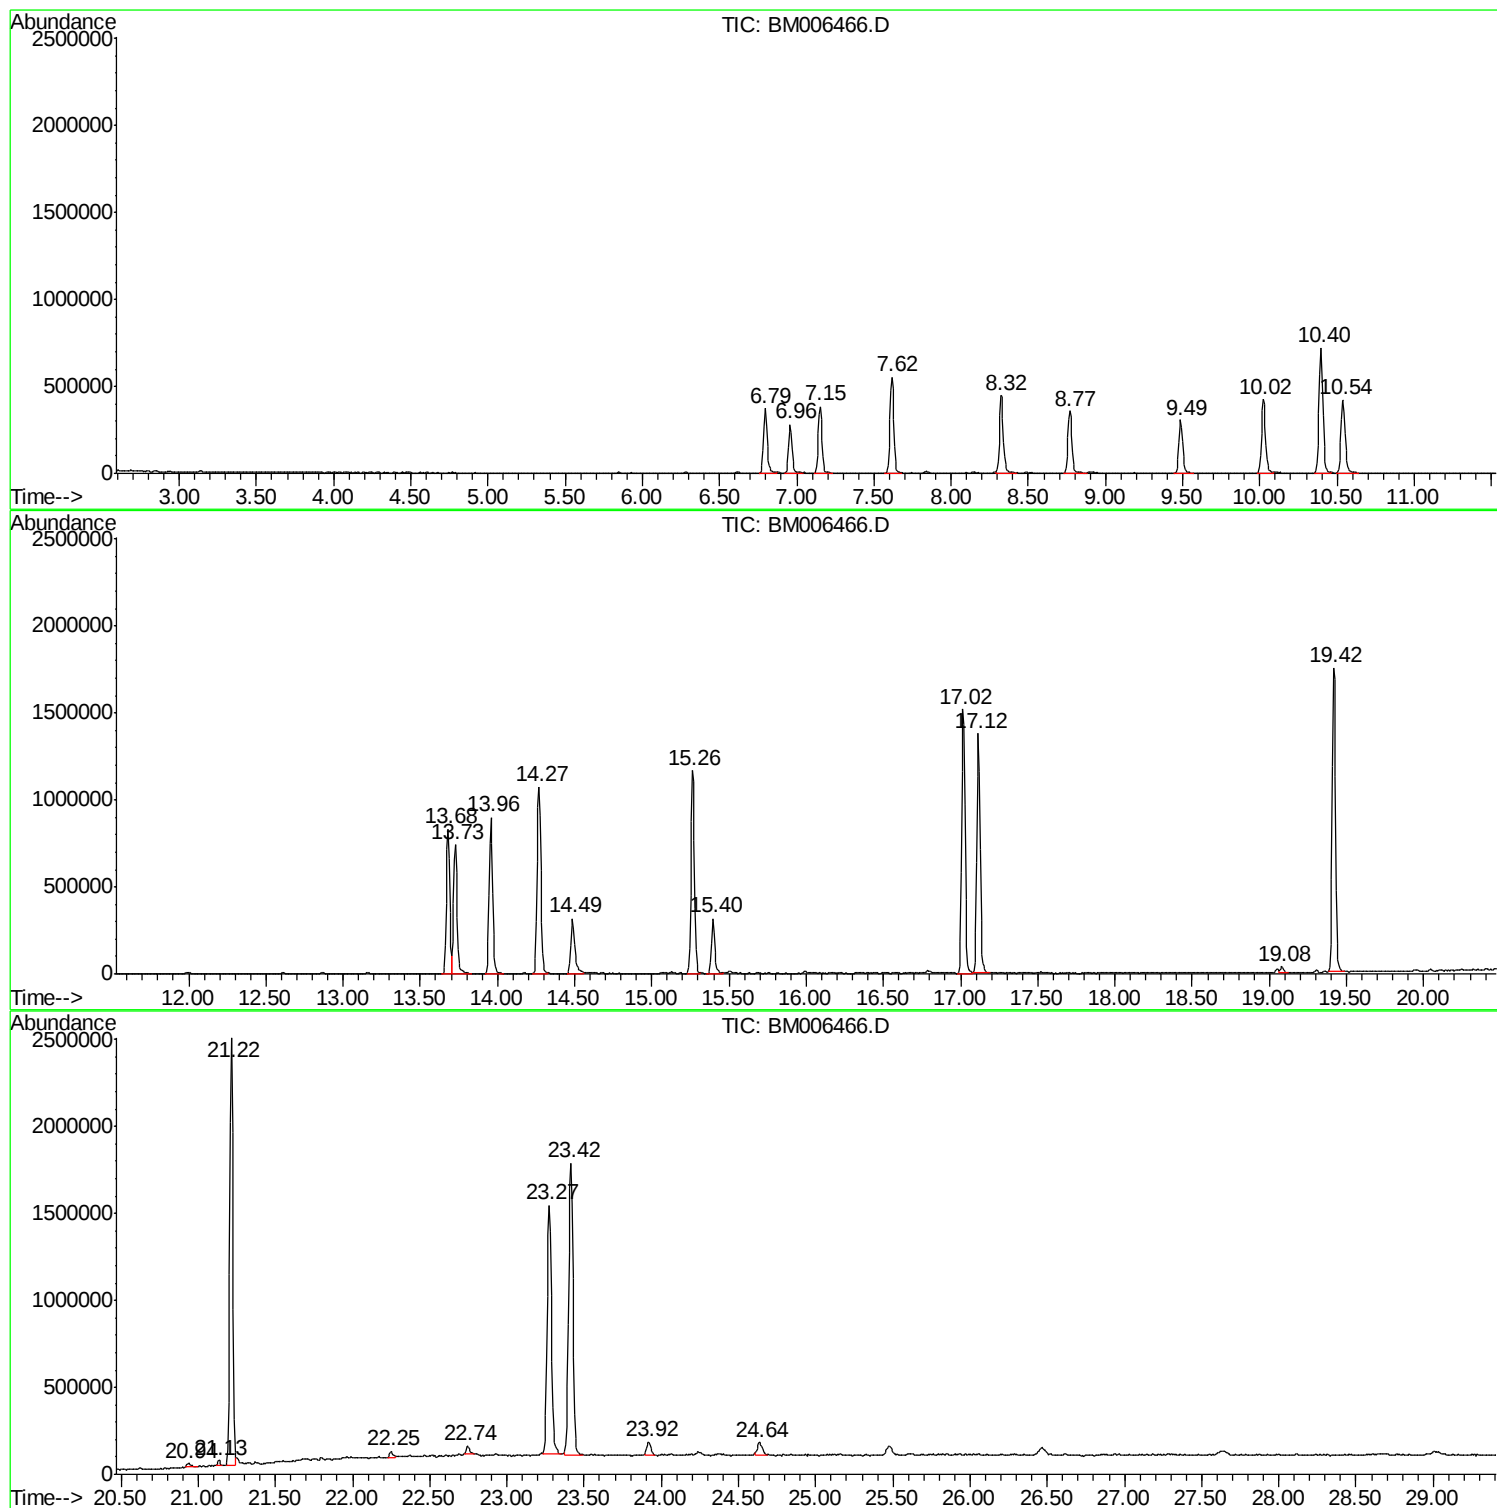

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006466.D
Acq On : 16 Jul 2016 05:39
Operator : UM/SJ
Sample : H3992-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ97

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071516\
Data File : BM006466.D
Acq On : 16 Jul 2016 05:39
Operator : UM/SJ
Sample : H3992-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ97

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc