


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071521\
Data File : BM030987.D
Acq On : 15 Jul 2021 20:26
Operator : CG/JU
Sample : PB137577BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK577

Manual Integrations
APPROVED

mohammad
7/16/2021 10:56:45 AM

Quant Time: Jul 16 04:05:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 16:14:04 2021
Response via : Initial Calibration

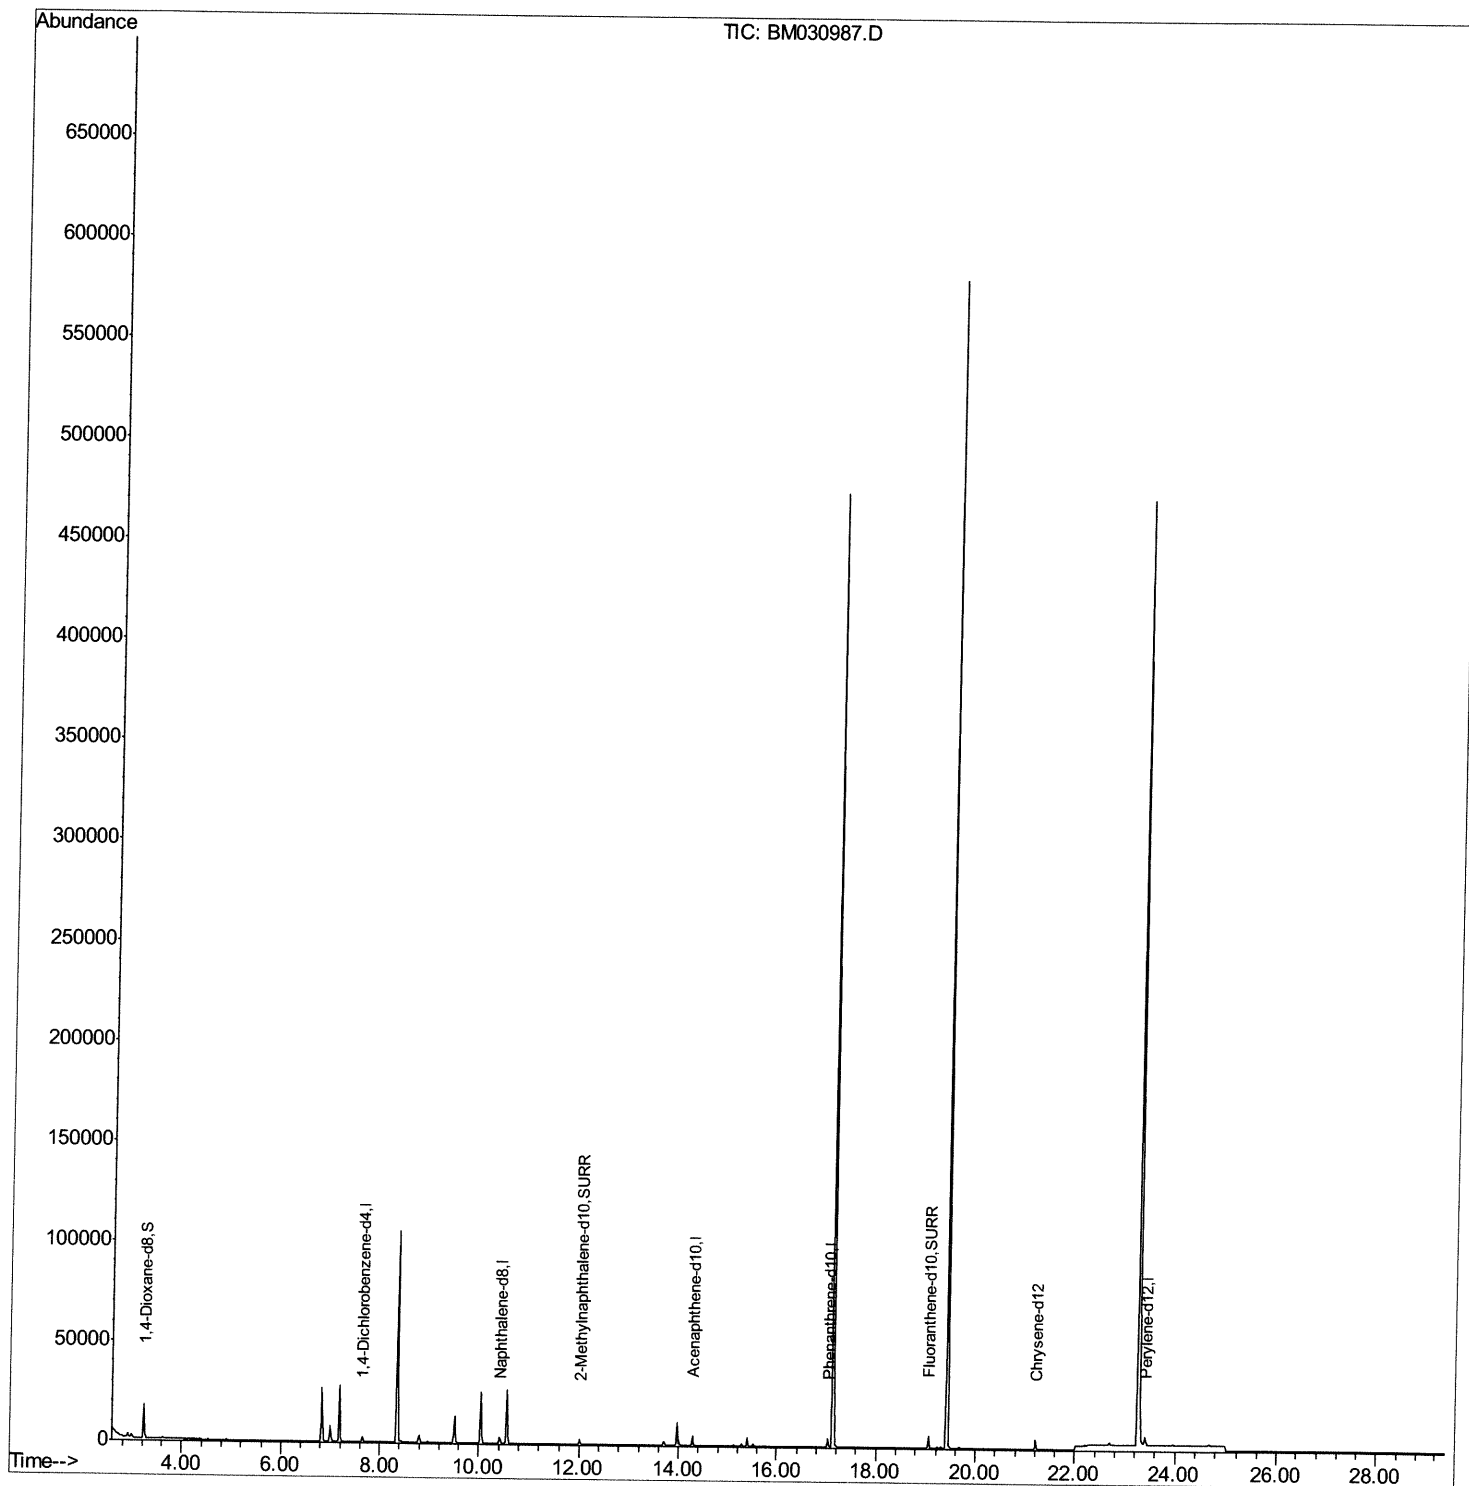

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071521\
 Data File : BM030987.D
 Acq On : 15 Jul 2021 20:26
 Operator : CG/JU
 Sample : PB137577BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK577

Manual Integrations
APPROVED

mohammad
 7/16/2021 10:56:45 AM

Quant Time: Jul 16 03:33:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 15 16:14:04 2021
 Response via : Initial Calibration

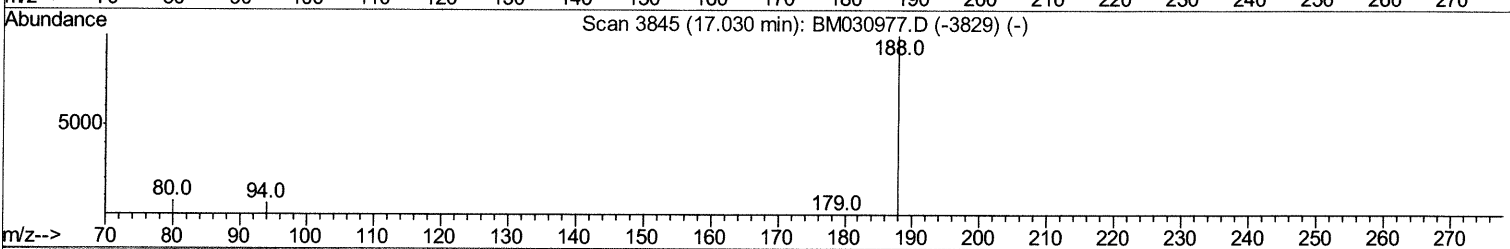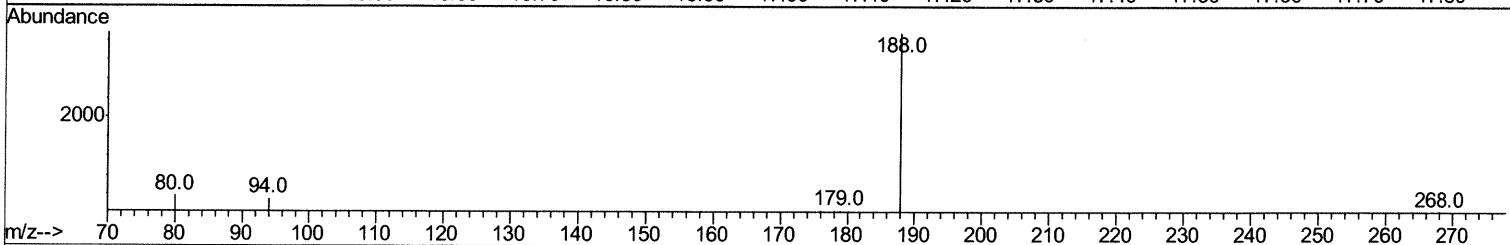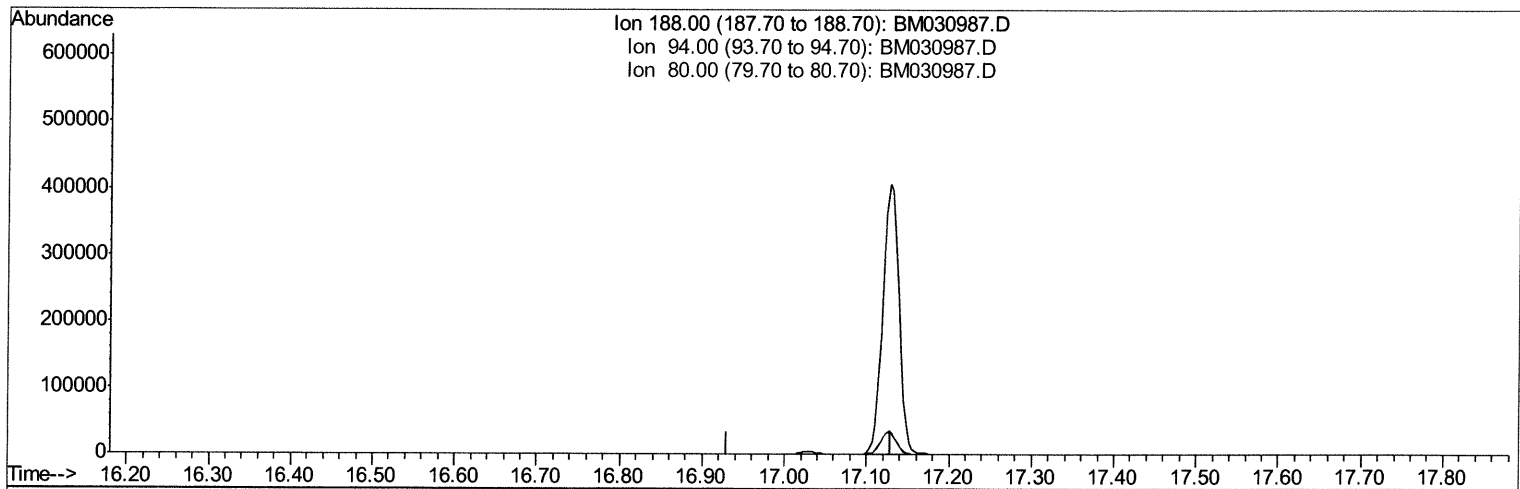

TIC: BM030987.D

(13) Phenanthrene-d10 (I)

17.030min (-17.030) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.70	0.00#
80.00	8.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071521\
Data File : BM030987.D
Acq On : 15 Jul 2021 20:26
Operator : CG/JU
Sample : PB137577BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK577

Manual Integrations
APPROVED

mohammad
7/16/2021 10:56:45 AM

Quant Time: Jul 16 03:33:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 16:14:04 2021
Response via : Initial Calibration

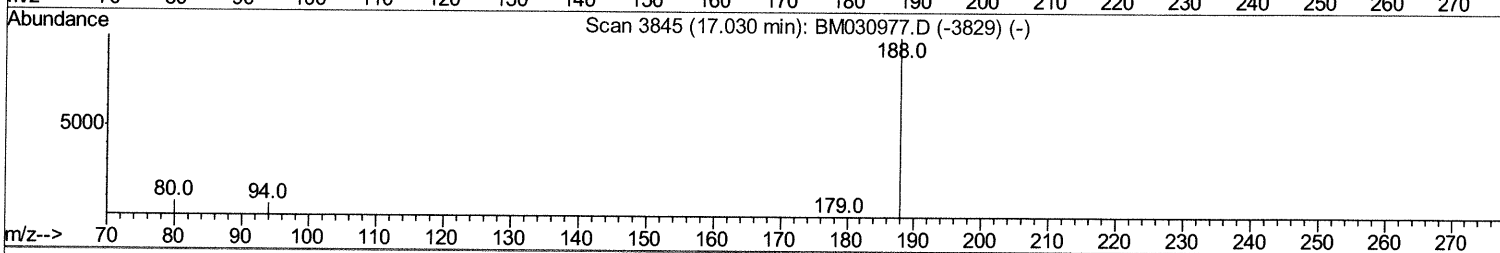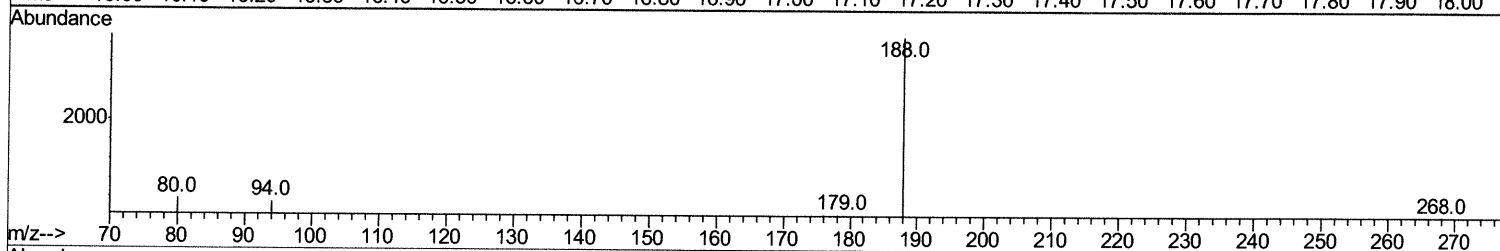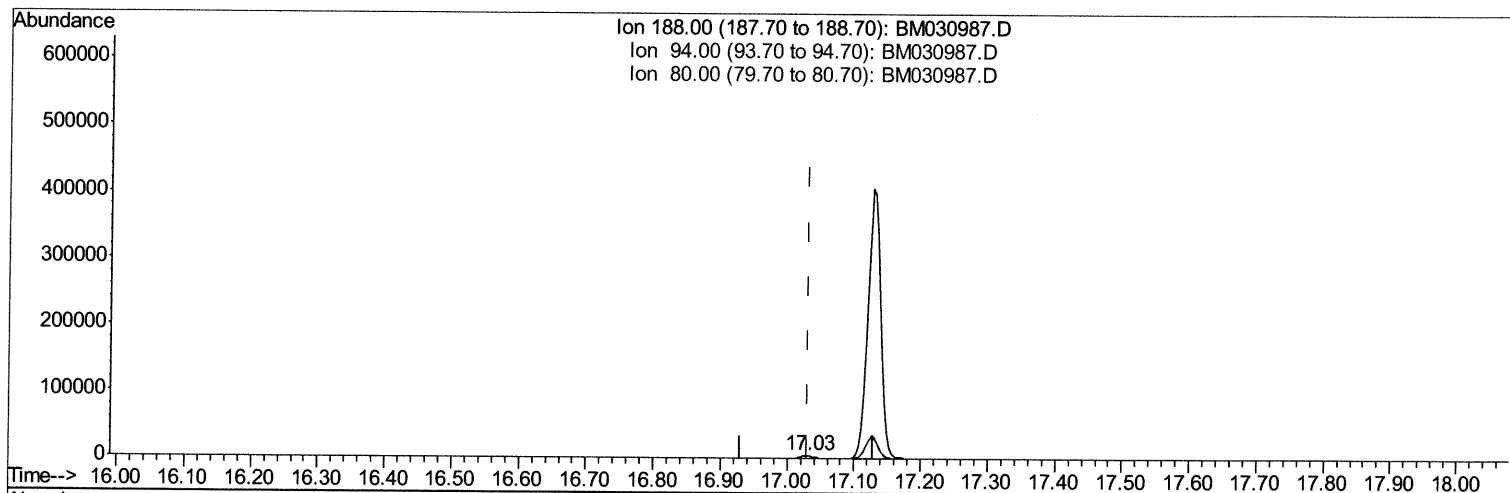

TIC: BM030987.D

(13) Phenanthrene-d10 (I)

17.030min (-0.000) 0.40ng/ul m 07/20/21 JU

response 5133

Ion	Exp%	Act%
188.00	100	100
94.00	8.70	8.33
80.00	8.50	9.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071521\
 Data File : BM030987.D
 Acq On : 15 Jul 2021 20:26
 Operator : CG/JU
 Sample : PB137577BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK577

Manual Integrations
 APPROVED

mohammad
 7/16/2021 10:56:45 AM

Quant Time: Jul 16 04:05:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 15 16:14:04 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	1140	0.40	ng/ul	0.00
4) Naphthalene-d8	10.42	136	3793	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.28	164	2618	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.03	188	5133m >	0.40	ng/ul >	0.00
17) Chrysene-d12	21.21	240	4504	0.40	ng/ul	0.00
23) Perylene-d12	23.40	264	5047	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	10498	8.96	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.01	152	2889	0.44	ng/ul	0.00
18) Fluoranthene-d10	19.06	212	6925	0.46	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed