
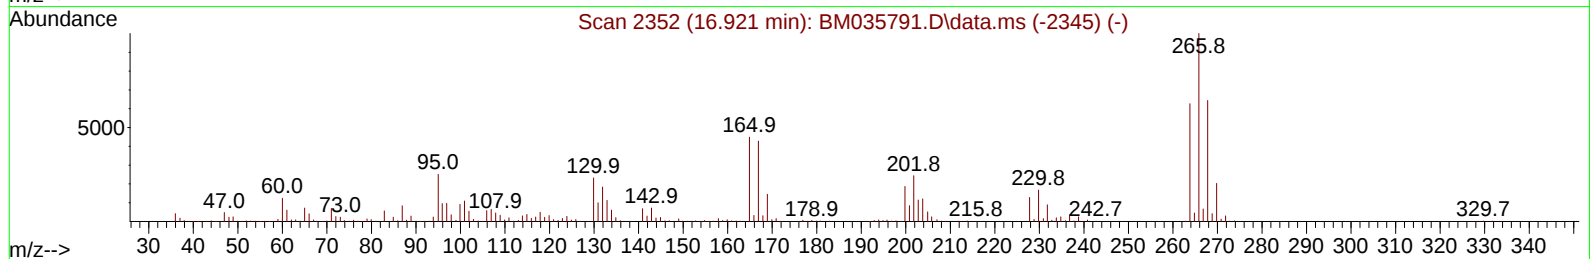
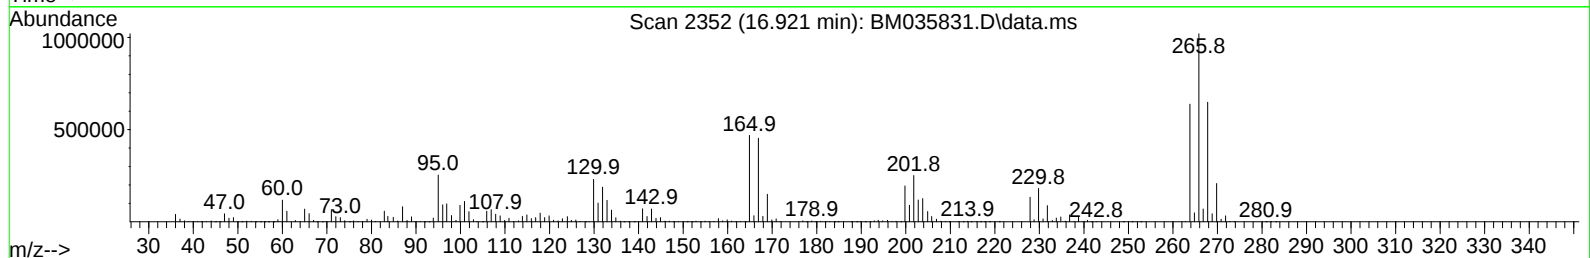


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035831.D
Acq On : 15 Jul 2022 15:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 05:08:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 14 01:21:21 2022
Response via : Initial Calibration

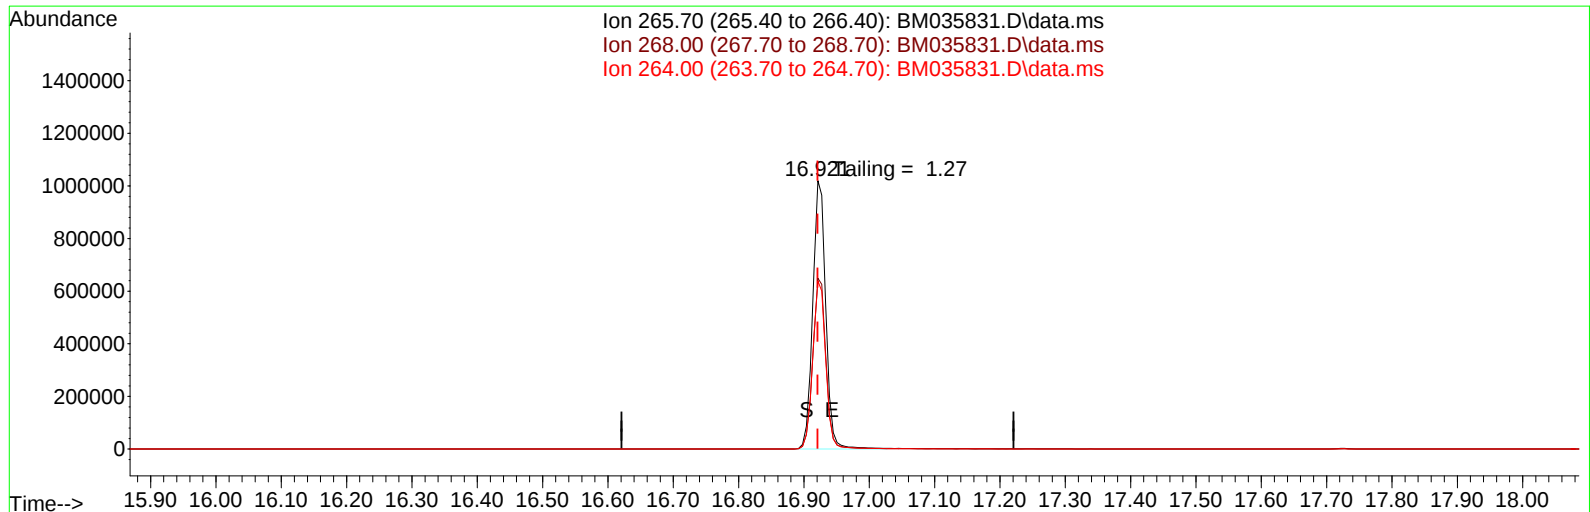

TIC: BM035831.D\data.ms

(70) Pentachlorophenol (C)




16.921min (+ 0.000) 140687.72 ng

response 1417194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.60
264.00	63.30	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035831.D
 Acq On : 15 Jul 2022 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 05:08:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 14 01:21:21 2022
 Response via : Initial Calibration

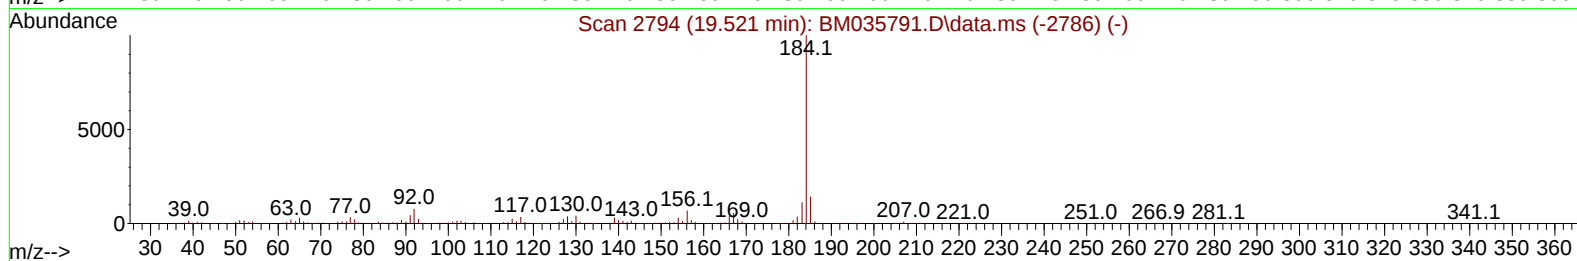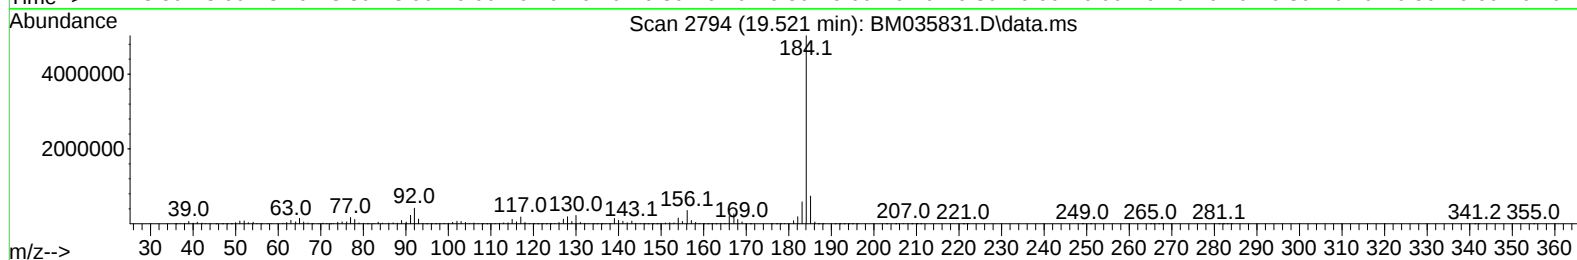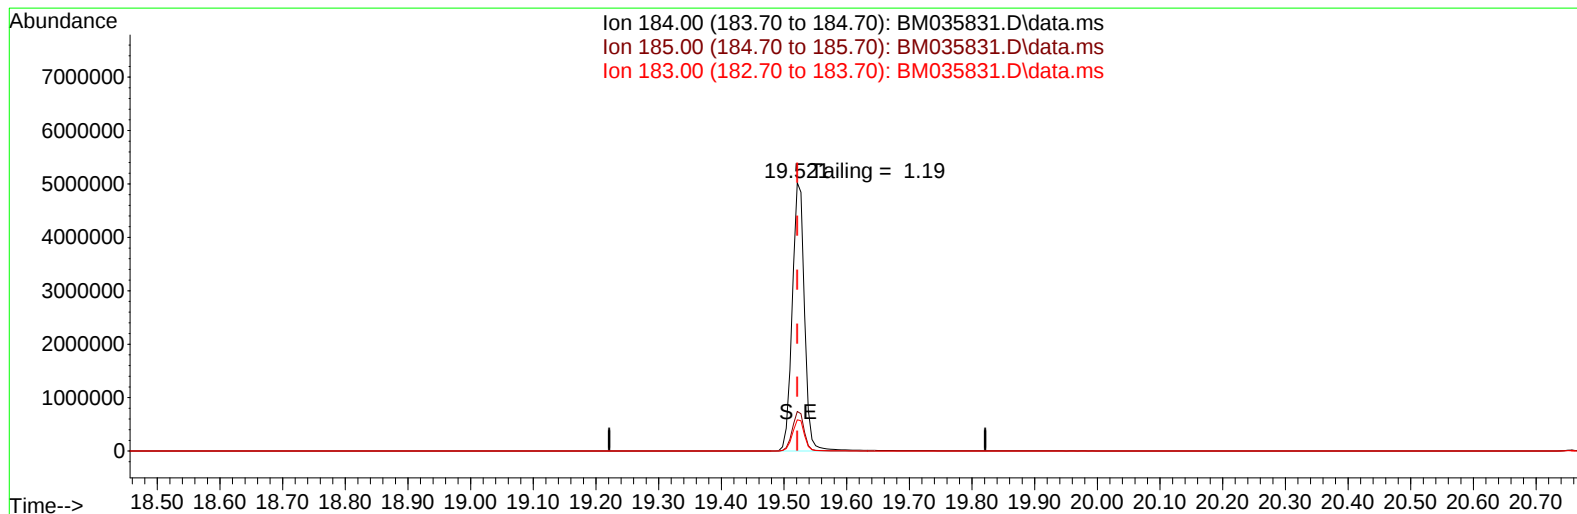

TIC: BM035831.D\data.ms

(77) Benzidine**19.521min (+ 0.000) 217785.81 ng****response 6905930**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.71
183.00	11.90	11.63
0.00	0.00	0.00