

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035825.D
 Acq On : 15 Jul 2022 10:19
 Operator : CG/JU
 Sample : PB146220BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146220BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	397	404	416	rBV	5473076	7596161	40.05%	9.370%
2	7.069	669	677	694	rBV	5233649	7968488	42.02%	9.829%
3	7.904	812	819	826	rBV	1270429	1944100	10.25%	2.398%
4	9.069	1009	1017	1026	rBV	3206182	5209148	27.47%	6.425%
5	10.710	1288	1296	1303	rBV	1719144	2769135	14.60%	3.416%
6	13.168	1707	1714	1722	rBV	8795749	12211605	64.39%	15.063%
7	14.539	1939	1947	1960	rBV	2259412	3414118	18.00%	4.211%
8	16.021	2192	2199	2218	rBV	6125049	8658443	45.65%	10.680%
9	17.274	2406	2412	2419	rBV	2824701	3800707	20.04%	4.688%
10	19.903	2853	2859	2868	rBV	15508933	18965800	100.00%	23.394%
11	21.450	3117	3122	3133	rBV	3357995	4226080	22.28%	5.213%
12	23.832	3520	3527	3537	rVB2	2167227	4308120	22.72%	5.314%




Sum of corrected areas: 81071905

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035825.D
Acq On : 15 Jul 2022 10:19
Operator : CG/JU
Sample : PB146220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

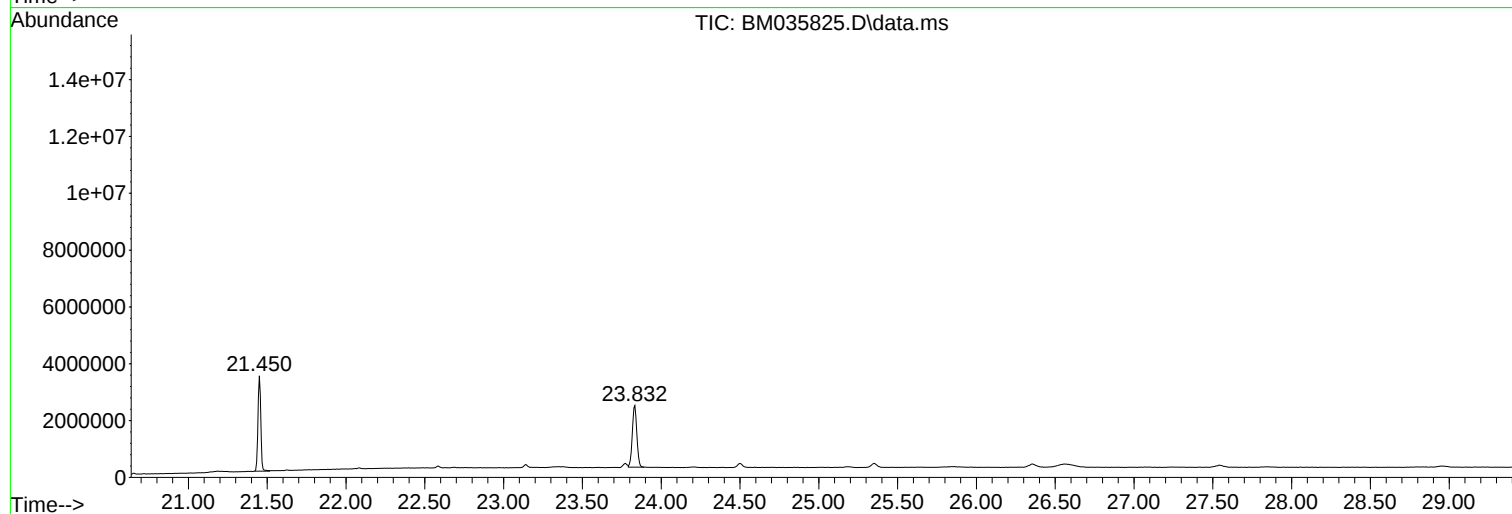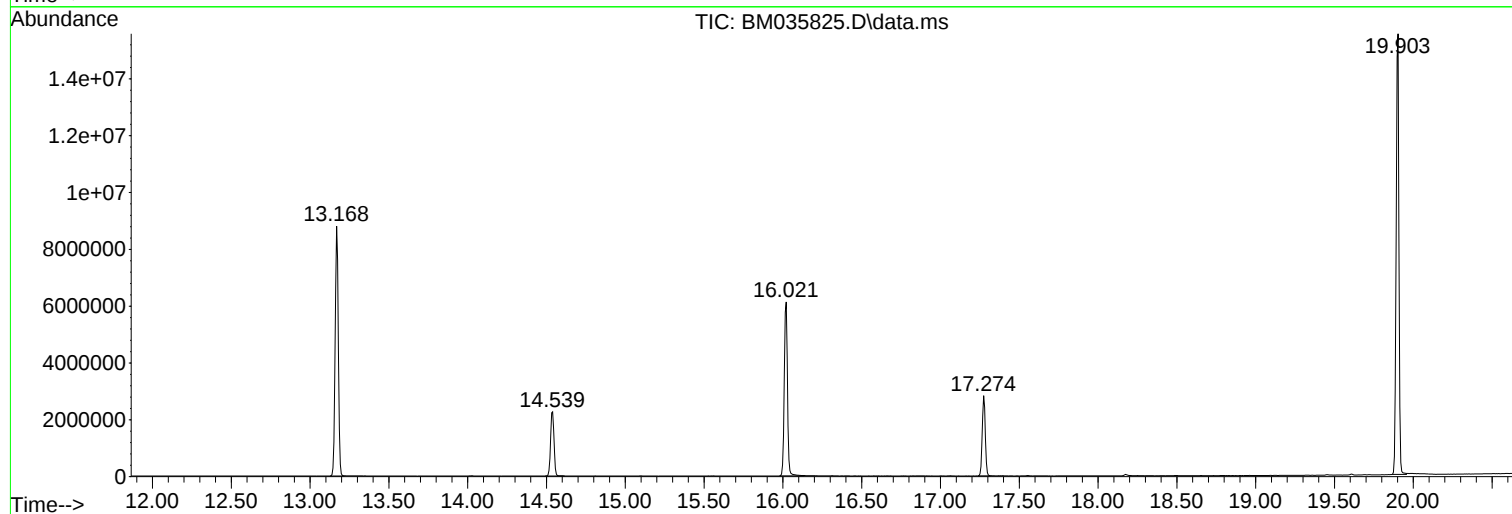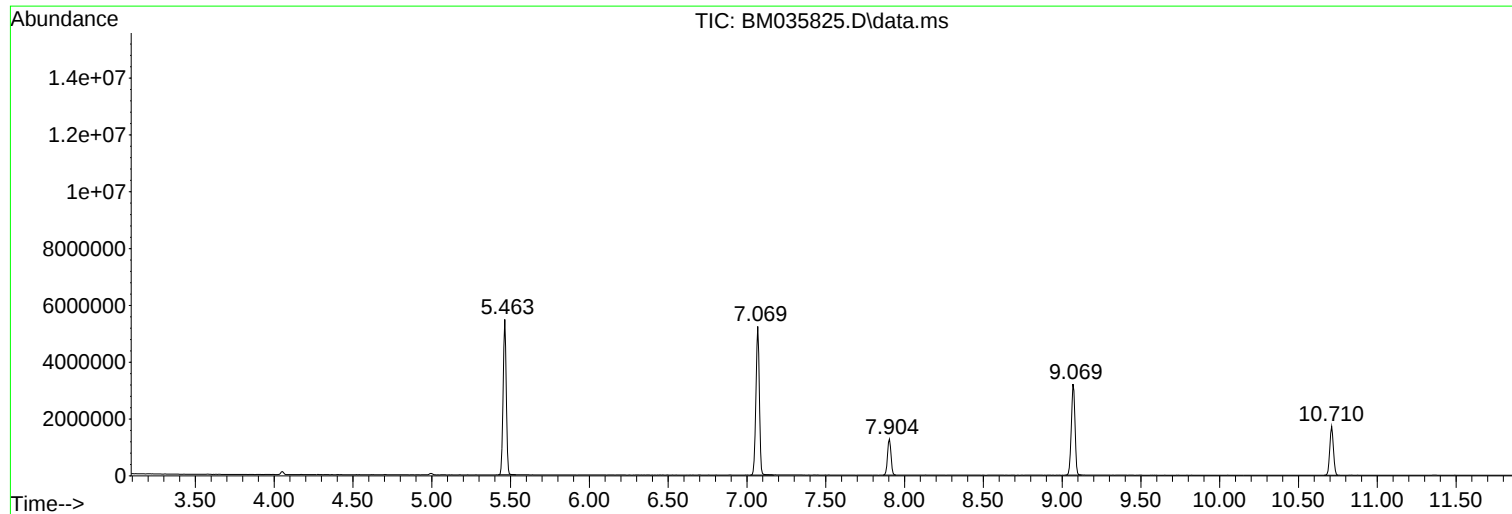

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035825.D
Acq On : 15 Jul 2022 10:19
Operator : CG/JU
Sample : PB146220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035825.D
Acq On : 15 Jul 2022 10:19
Operator : CG/JU
Sample : PB146220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------