

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035833.D
 Acq On : 15 Jul 2022 16:57
 Operator : CG/JU
 Sample : PB146152BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146152BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	397	404	417	rBV	7595764	10794307	40.15%	9.130%
2	7.075	669	678	692	rBV	7274312	11595544	43.13%	9.808%
3	7.904	811	819	827	rBV	1764480	2648460	9.85%	2.240%
4	9.075	1009	1018	1028	rBV	4714889	7559773	28.12%	6.394%
5	10.710	1287	1296	1313	rBV	2410151	4011782	14.92%	3.393%
6	13.174	1703	1715	1729	rBV	13028728	18792578	69.90%	15.895%
7	14.539	1940	1947	1955	rBV	3627608	5263154	19.58%	4.452%
8	16.021	2191	2199	2220	rBV	9739468	13647808	50.76%	11.544%
9	17.274	2406	2412	2425	rBV	4295579	5953389	22.14%	5.036%
10	19.903	2852	2859	2872	rBV	21992568	26885854	100.00%	22.741%
11	21.450	3117	3122	3132	rBV	4607352	5539554	20.60%	4.685%
12	23.768	3512	3516	3520	rBV	165400	277001	1.03%	0.234%
13	23.833	3520	3527	3540	rVB2	2486328	4902639	18.24%	4.147%
14	24.497	3635	3640	3650	rVB	171297	356066	1.32%	0.301%




Sum of corrected areas: 118227909

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035833.D
Acq On : 15 Jul 2022 16:57
Operator : CG/JU
Sample : PB146152BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146152BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

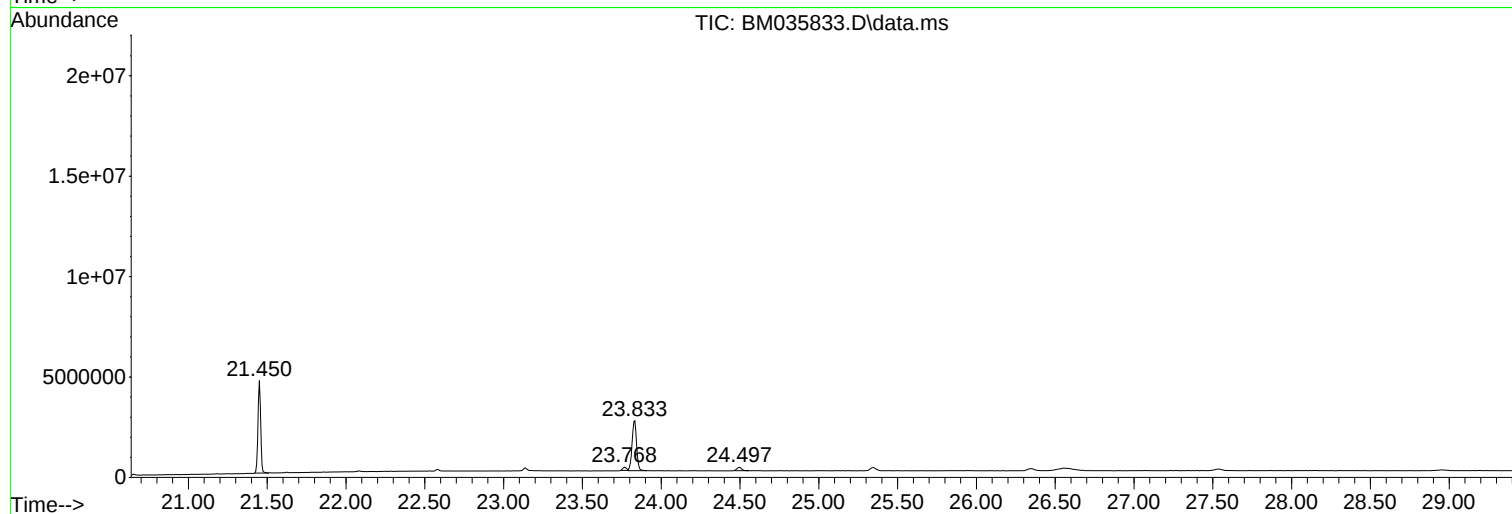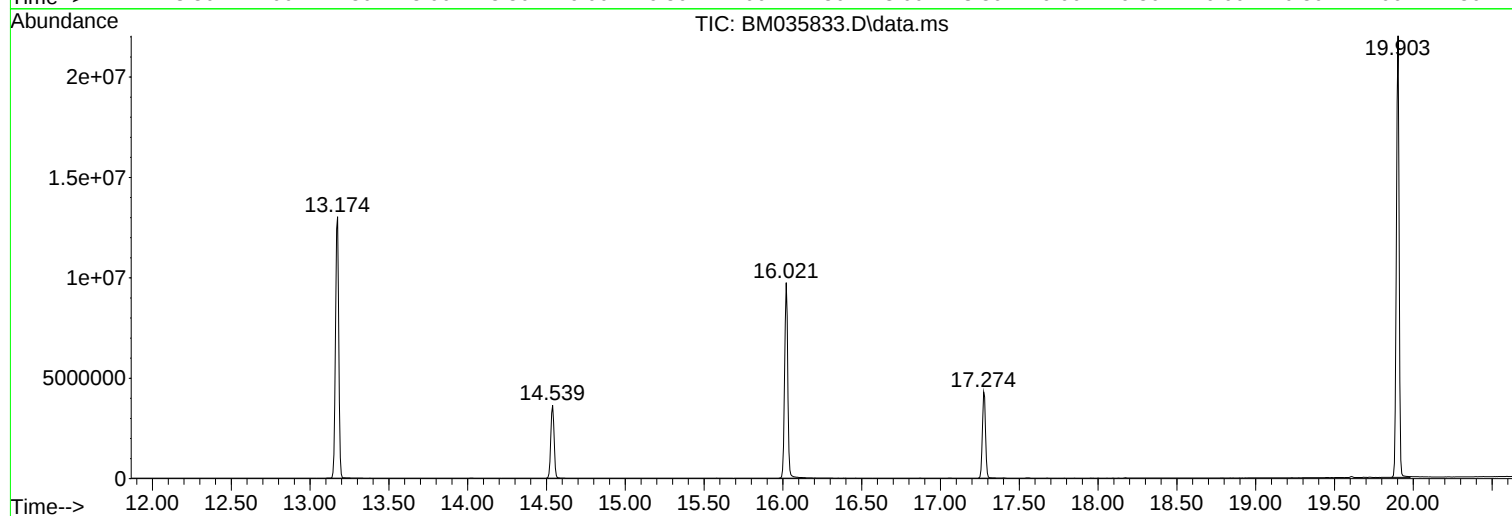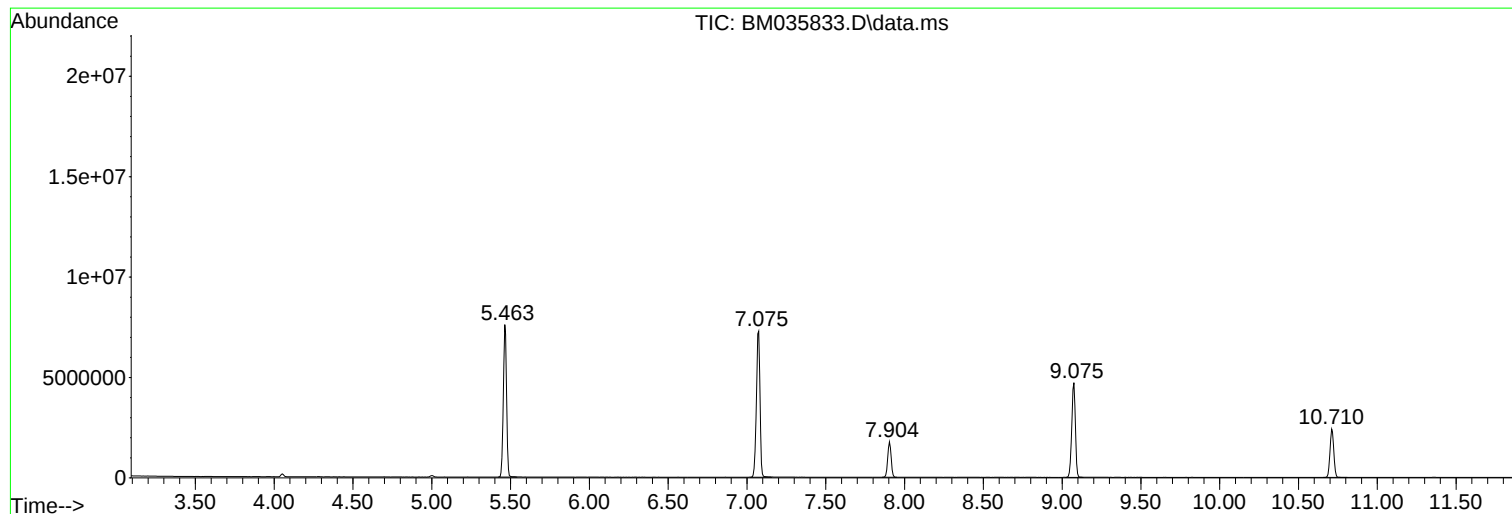

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035833.D
Acq On : 15 Jul 2022 16:57
Operator : CG/JU
Sample : PB146152BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146152BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035833.D
Acq On : 15 Jul 2022 16:57
Operator : CG/JU
Sample : PB146152BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146152BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------