

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035835.D
 Acq On : 15 Jul 2022 18:13
 Operator : CG/JU
 Sample : N3726-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OWS-12-12.5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	397	404	422	rBV	8118895	11579457	54.48%	10.996%
2	7.075	668	678	692	rBV	7865874	12255150	57.66%	11.638%
3	7.904	812	819	826	rVB	1415906	2136303	10.05%	2.029%
4	9.075	1009	1018	1026	rBV	4502364	7299595	34.34%	6.932%
5	10.710	1289	1296	1305	rBV	1829936	3043057	14.32%	2.890%
6	13.175	1707	1715	1729	rBV	11115105	15877183	74.70%	15.077%
7	14.539	1936	1947	1960	rBV	2785804	3892476	18.31%	3.696%
8	16.021	2192	2199	2223	rBV	8983569	12759994	60.04%	12.117%
9	17.274	2406	2412	2422	rBV	3022349	4335379	20.40%	4.117%
10	18.180	2561	2566	2573	rBV	360510	517044	2.43%	0.491%
11	19.456	2779	2783	2792	rBV2	132042	215136	1.01%	0.204%
12	19.903	2853	2859	2867	rBV	16721861	21253792	100.00%	20.183%
13	21.174	3071	3075	3085	rBV	643541	934799	4.40%	0.888%
14	21.450	3116	3122	3130	rBV	3176441	4209020	19.80%	3.997%
15	22.568	3307	3312	3323	rBV2	769829	1338019	6.30%	1.271%
16	23.827	3519	3526	3539	rVB2	1827466	3659539	17.22%	3.475%




Sum of corrected areas: 105305943

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035835.D
Acq On : 15 Jul 2022 18:13
Operator : CG/JU
Sample : N3726-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OWS-12-12.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

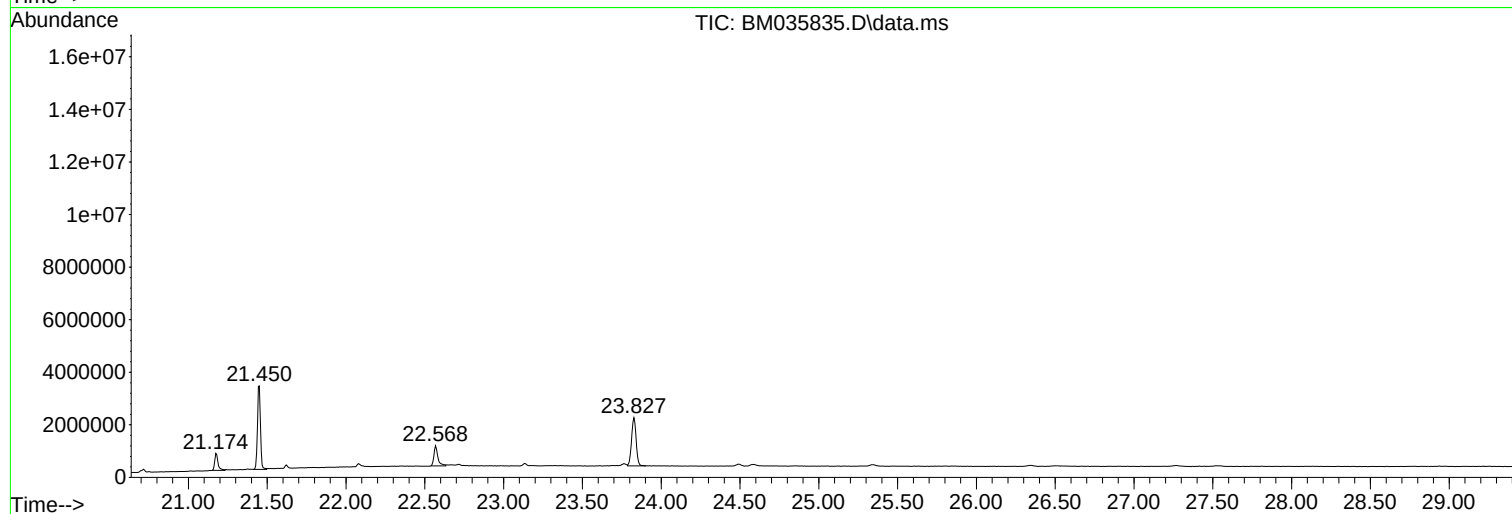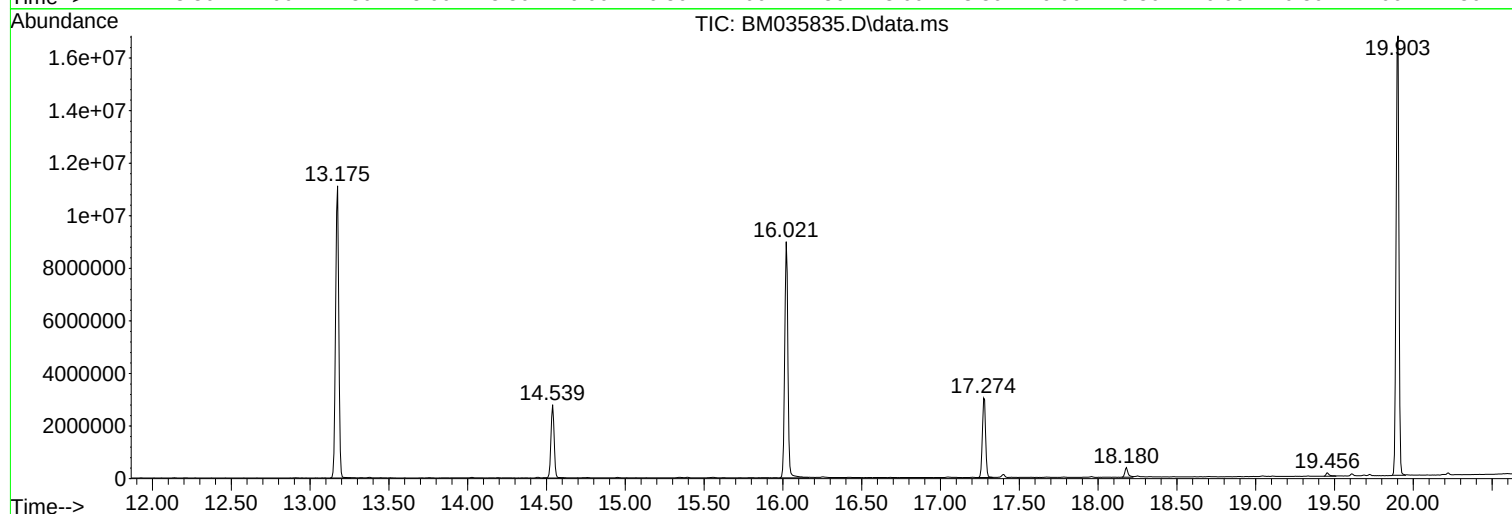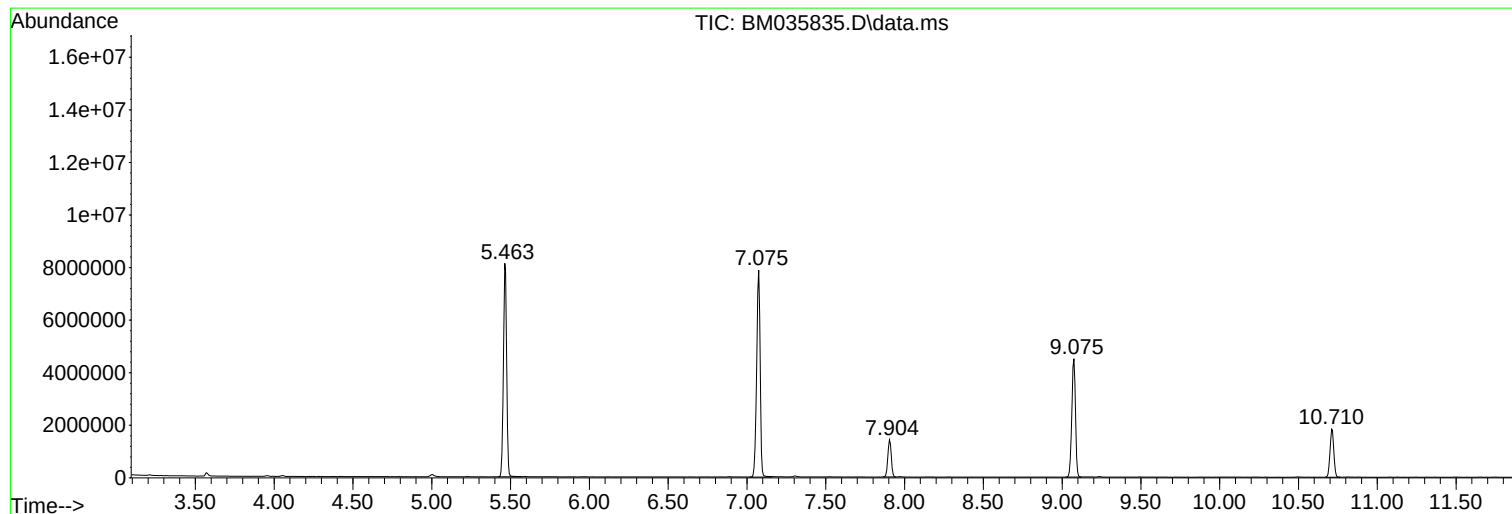

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035835.D
Acq On : 15 Jul 2022 18:13
Operator : CG/JU
Sample : N3726-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OWS-12-12.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035835.D
Acq On : 15 Jul 2022 18:13
Operator : CG/JU
Sample : N3726-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OWS-12-12.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------