

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035839.D
 Acq On : 15 Jul 2022 20:39
 Operator : CG/JU
 Sample : N3726-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SEPTIC-12-12.5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	397	404	412	rBV	6029094	8329641	49.68%	9.686%
2	7.069	667	677	694	rBV	5674223	8716995	51.99%	10.136%
3	7.904	811	819	826	rBV	1332881	2024257	12.07%	2.354%
4	9.069	1009	1017	1026	rBV	3300181	5380592	32.09%	6.257%
5	10.710	1288	1296	1305	rVB	1762486	2892658	17.25%	3.364%
6	13.169	1707	1714	1727	rBV	8220734	11923577	71.11%	13.865%
7	14.539	1939	1947	1963	rBV	2536470	3759365	22.42%	4.371%
8	16.021	2192	2199	2230	rBV	6637497	9363499	55.84%	10.888%
9	17.274	2404	2412	2423	rBV	3193133	4438344	26.47%	5.161%
10	18.174	2561	2565	2574	rBV	195439	267486	1.60%	0.311%
11	19.898	2852	2858	2871	rBV	13621892	16767472	100.00%	19.497%
12	21.174	3071	3075	3083	rBV	274984	407278	2.43%	0.474%
13	21.445	3116	3121	3130	rBV	3755898	4770361	28.45%	5.547%
14	22.568	3307	3312	3325	rBV	1423800	2242535	13.37%	2.608%
15	23.827	3519	3526	3539	rVB2	2398601	4715956	28.13%	5.484%




Sum of corrected areas: 86000016

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035839.D
Acq On : 15 Jul 2022 20:39
Operator : CG/JU
Sample : N3726-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SEPTIC-12-12.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

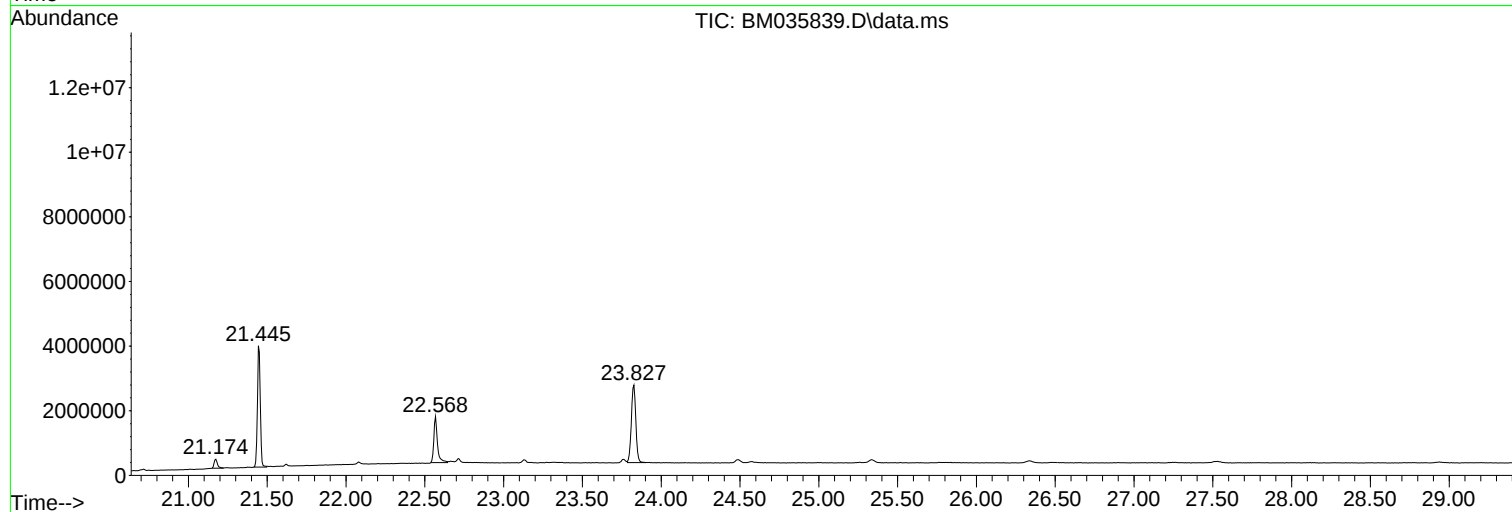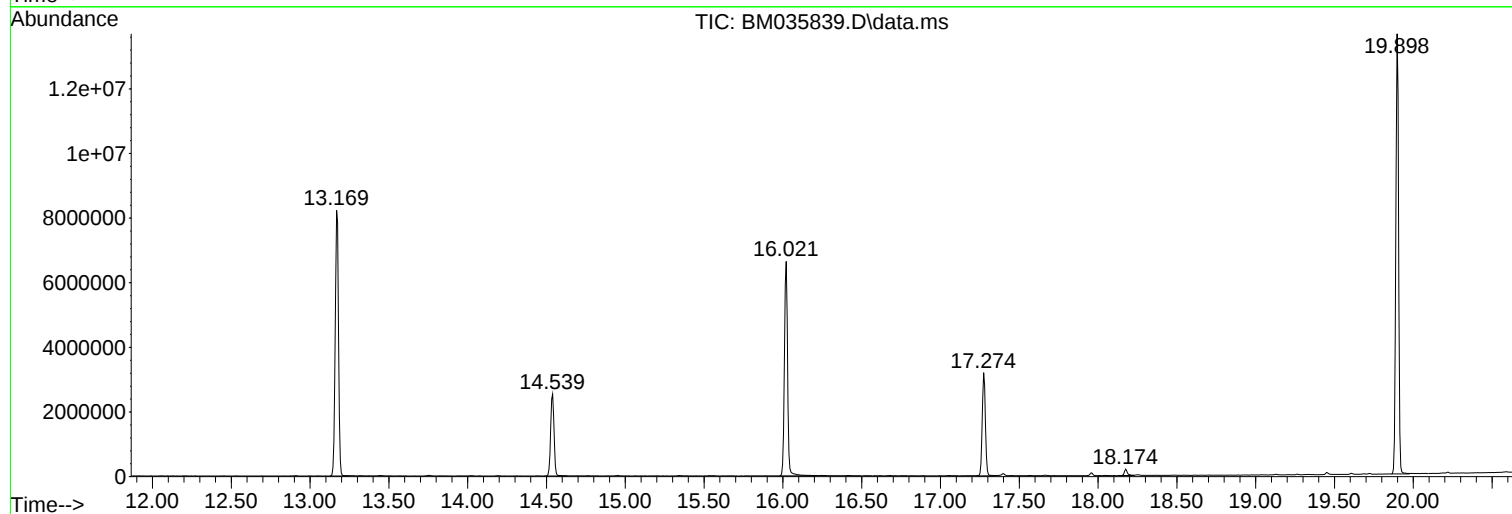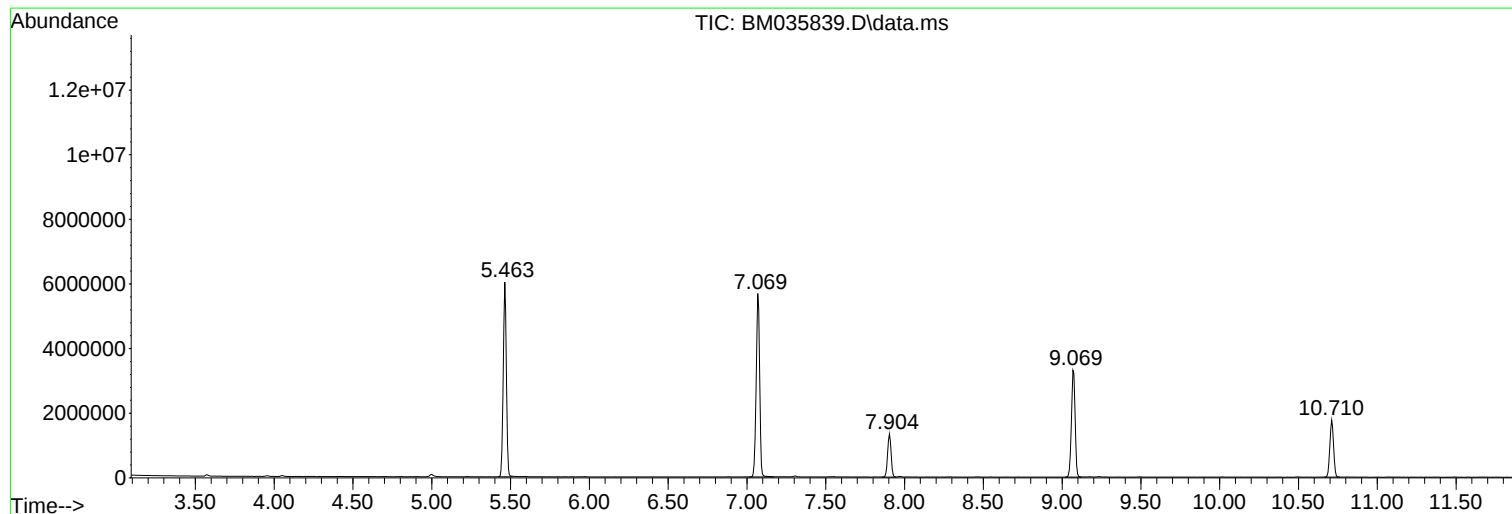

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035839.D
Acq On : 15 Jul 2022 20:39
Operator : CG/JU
Sample : N3726-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SEPTIC-12-12.5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 9-Octadecenamide, (Z)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.568	9.40 ng	2242540	Chrysene-d12	21.445

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	97
2		13-Docosenamide, (Z)-	337	C22H43NO	000112-84-5	96
3		Palmitoleamide	253	C16H31NO	106010-22-4	90
4		Hexadecanamide	255	C16H33NO	000629-54-9	72
5		Tetradecanamide	227	C14H29NO	000638-58-4	64

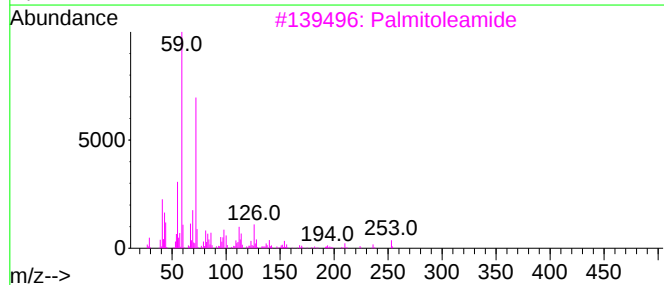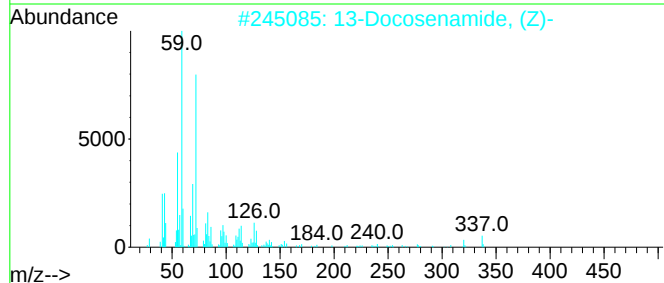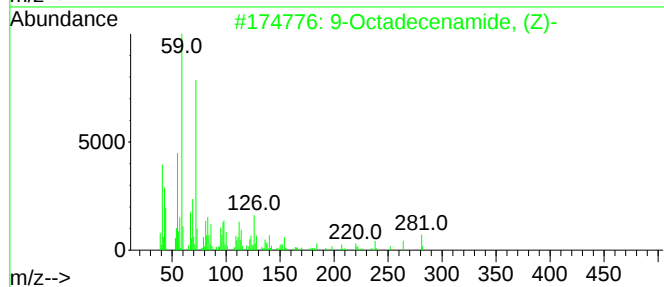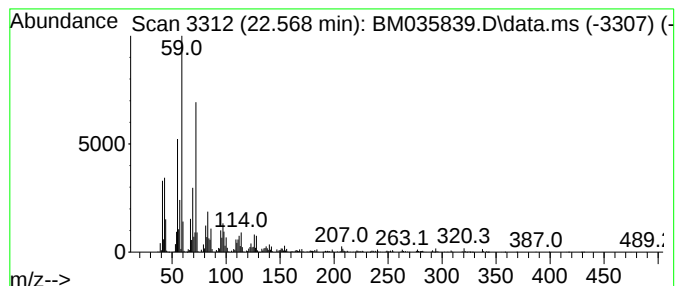

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035839.D
Acq On : 15 Jul 2022 20:39
Operator : CG/JU
Sample : N3726-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SEPTIC-12-12.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
9-Octadecenamid...	22.568	9.4	ng	2242540	5	21.445	4770360	20.0