


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035823.D
 Acq On : 15 Jul 2022 09:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 14 01:21:21 2022

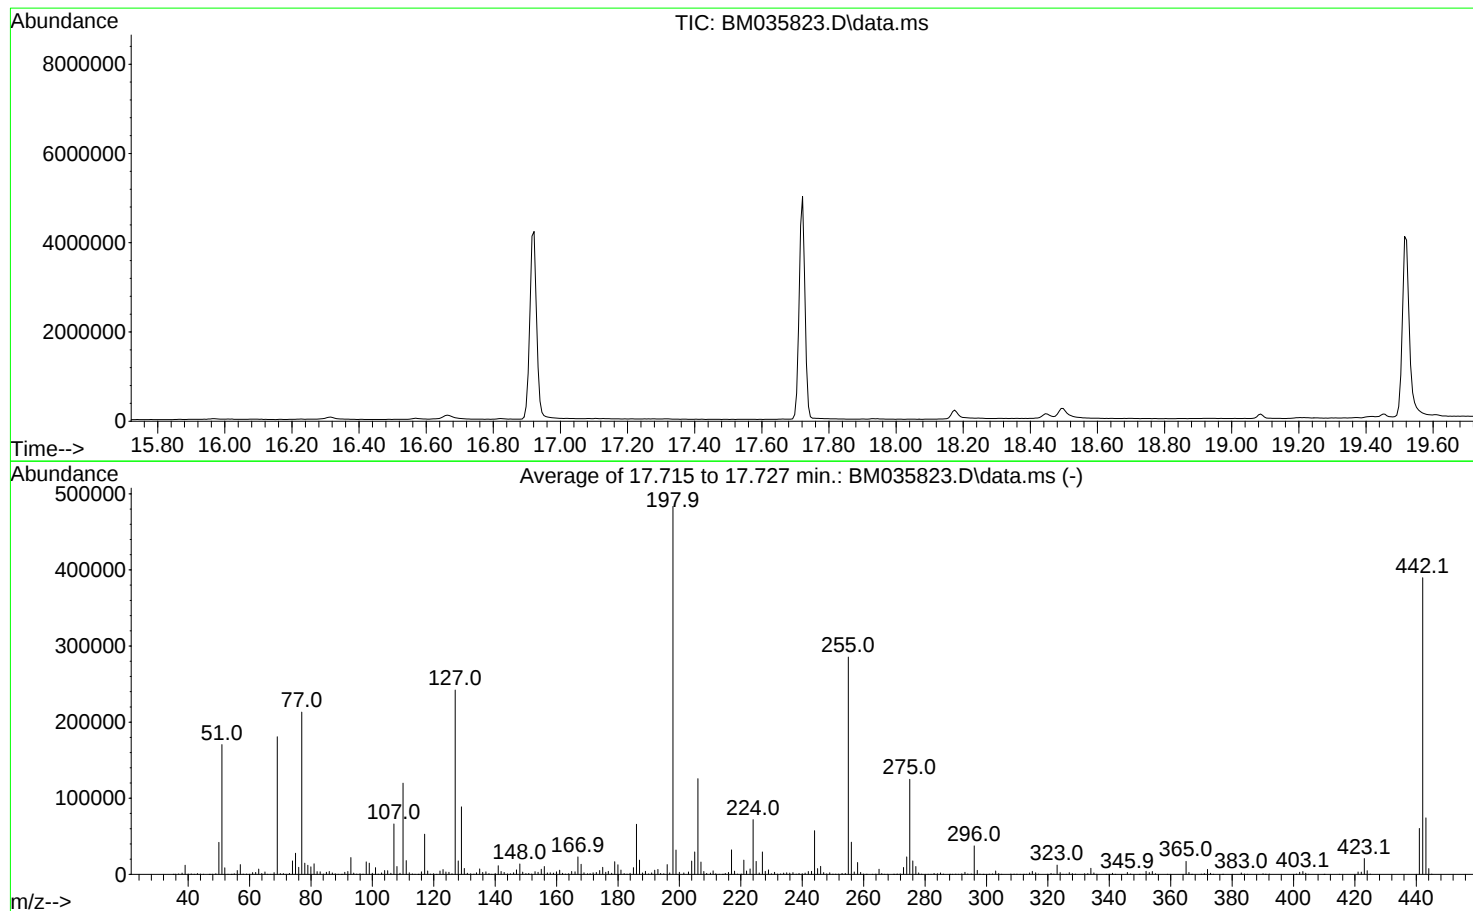




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	170418	PASS
68	69	0.00	2	1.3	2408	PASS
69	198	0.00	100	37.4	180798	PASS
70	69	0.00	2	0.6	1010	PASS
127	198	10	80	50.1	242257	PASS
197	198	0.00	2	0.4	1992	PASS
198	198	100	100	100.0	483307	PASS
199	198	5	9	6.6	32005	PASS
275	198	10	60	25.9	124965	PASS
365	198	1	100	3.5	17103	PASS
441	198	0.01	100	12.5	60299	PASS
442	442	50	100	100.0	389824	PASS
443	442	15	24	19.0	74163	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035823.D
 Acq On : 15 Jul 2022 09:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 16 05:03:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 14 01:21:21 2022
 Response via : Initial Calibration

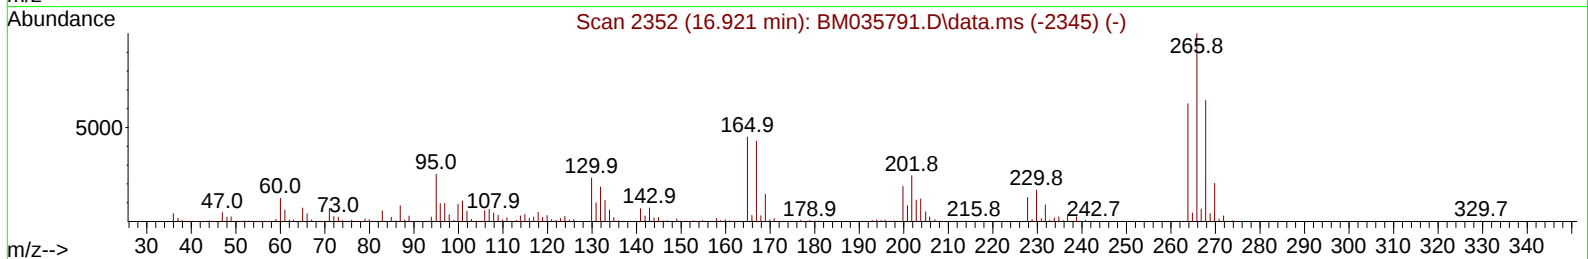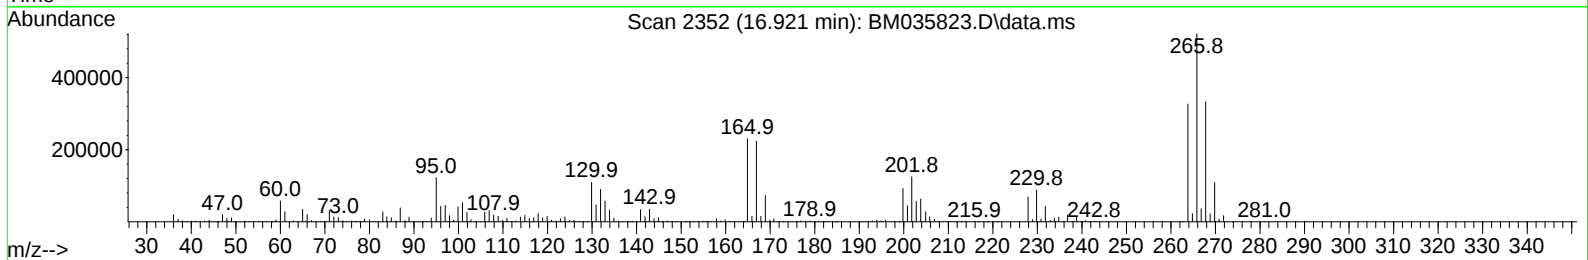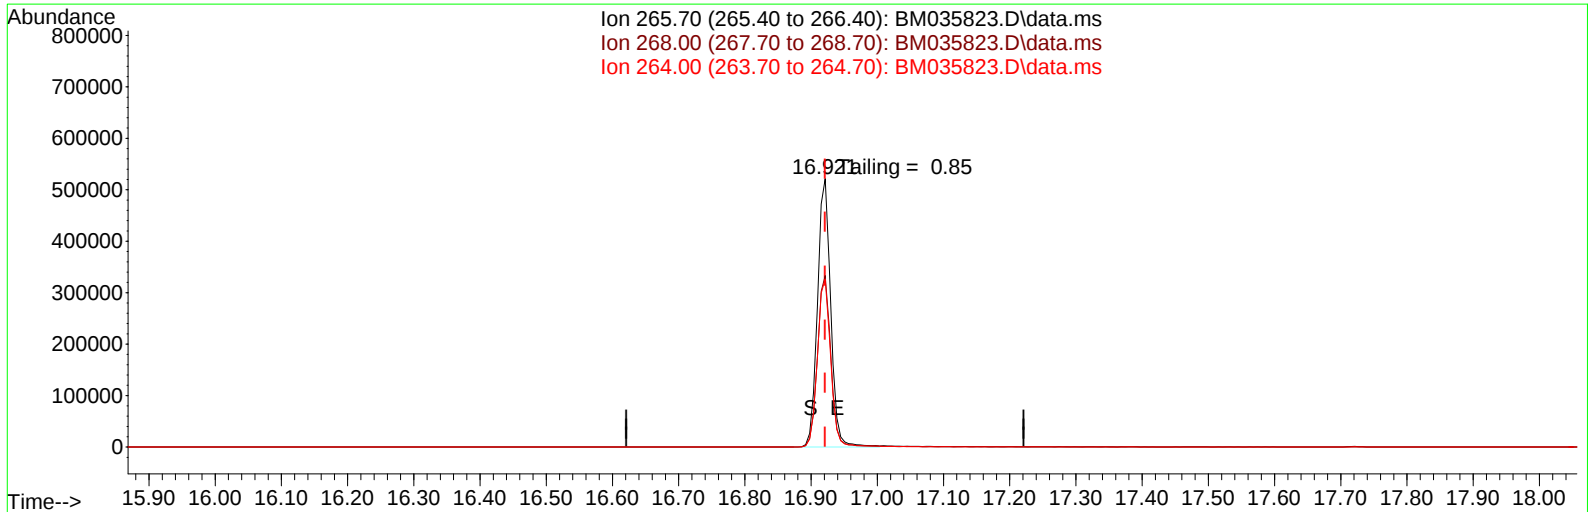

TIC: BM035823.D\data.ms

(70) Pentachlorophenol (C)

16.921min (+ 0.000) 128752.55 ng




response 725119

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.83
264.00	63.30	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035823.D
Acq On : 15 Jul 2022 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 16 05:03:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 14 01:21:21 2022
Response via : Initial Calibration

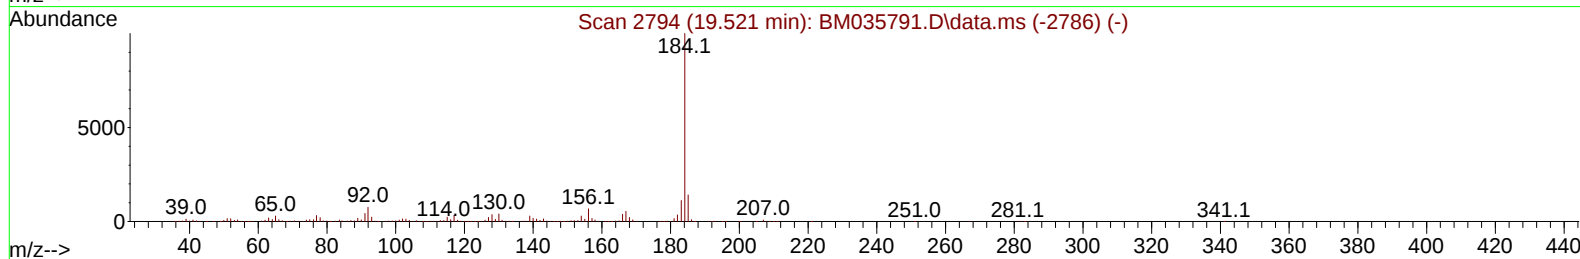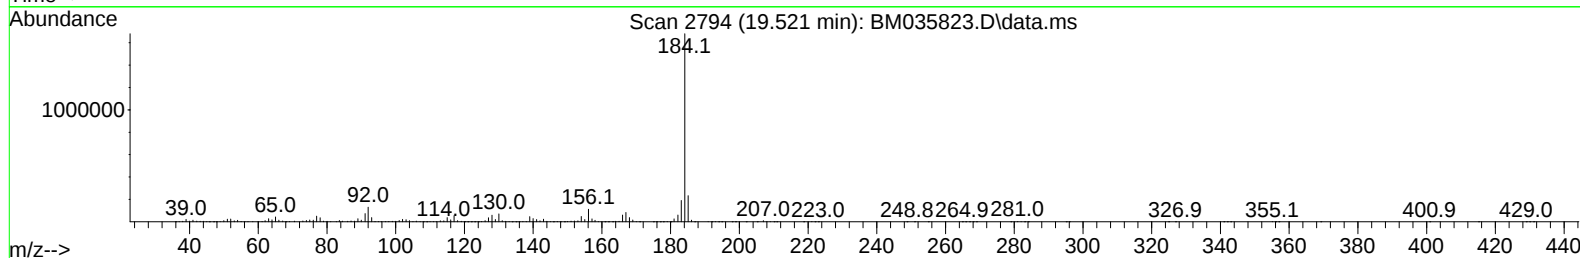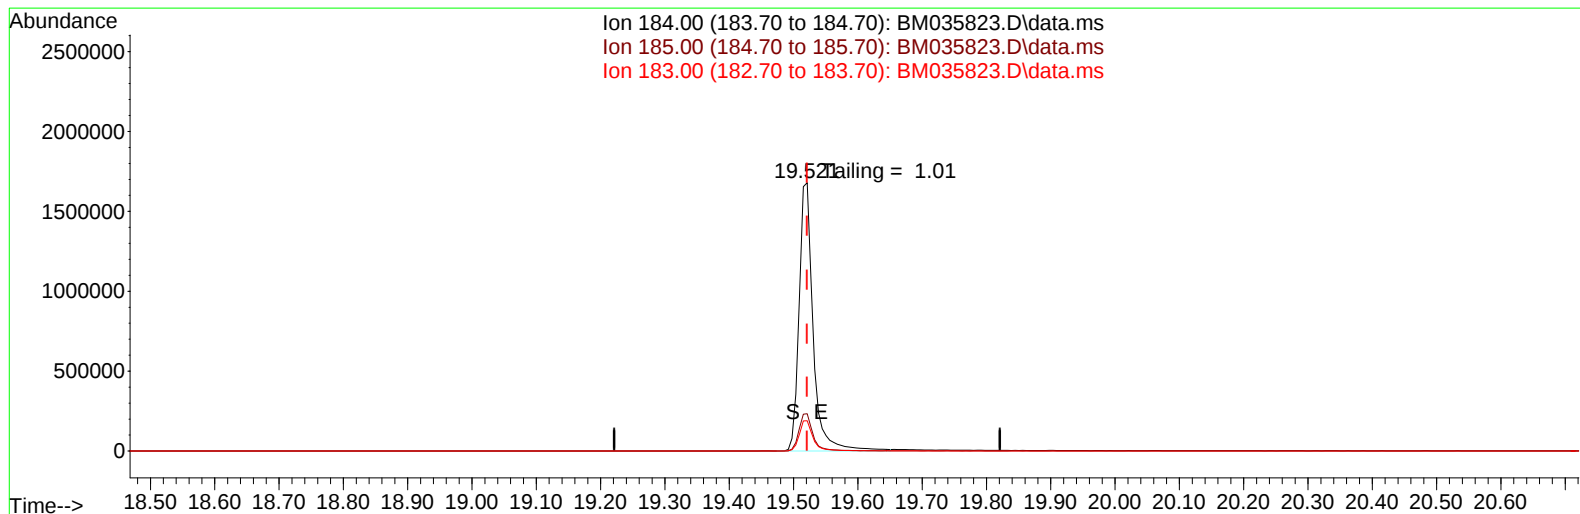

TIC: BM035823.D\data.ms

(77) Benzidine

19.521min (+ 0.000) 152725.98 ng

response 2582880

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.91
183.00	11.90	11.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/15/2022	BNA_M	<u>BM035823.D</u>
Compound Name	Response	Retention Time
DDT	1878883	20.756
DDD	22966	20.309
DDE	1485	19.803
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24451	1903334	1.28

Instrument :
BNA_M
ClientSampleId :
DFTPP