
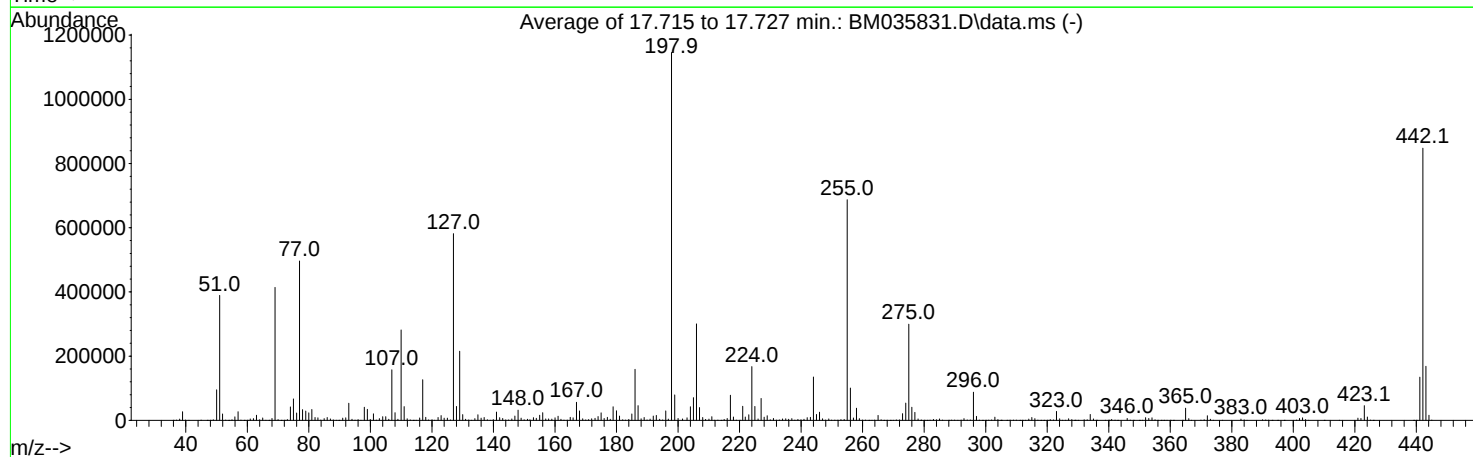


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035831.D
 Acq On : 15 Jul 2022 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 14 01:21:21 2022

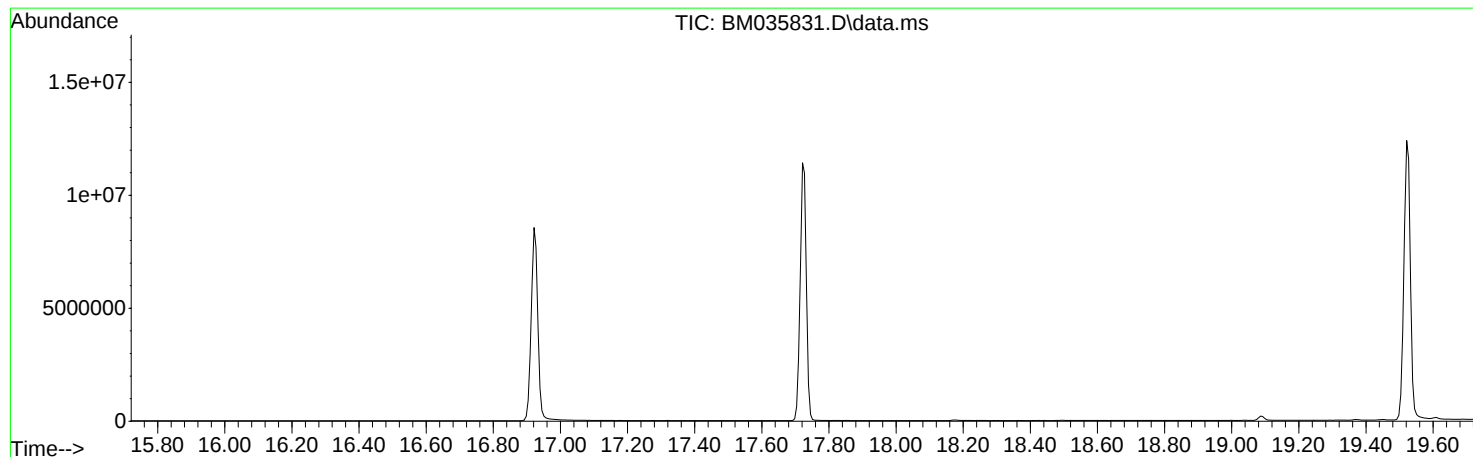




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	389108	PASS
68	69	0.00	2	1.4	6005	PASS
69	198	0.00	100	36.2	414310	PASS
70	69	0.00	2	0.6	2329	PASS
127	198	10	80	50.8	581653	PASS
197	198	0.00	2	0.4	4190	PASS
198	198	100	100	100.0	1145835	PASS
199	198	5	9	6.9	79296	PASS
275	198	10	60	26.2	299712	PASS
365	198	1	100	3.3	38056	PASS
441	198	0.01	100	11.8	134827	PASS
442	442	50	100	100.0	847680	PASS
443	442	15	24	19.9	168664	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
 Data File : BM035831.D
 Acq On : 15 Jul 2022 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 16 05:08:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 14 01:21:21 2022
 Response via : Initial Calibration

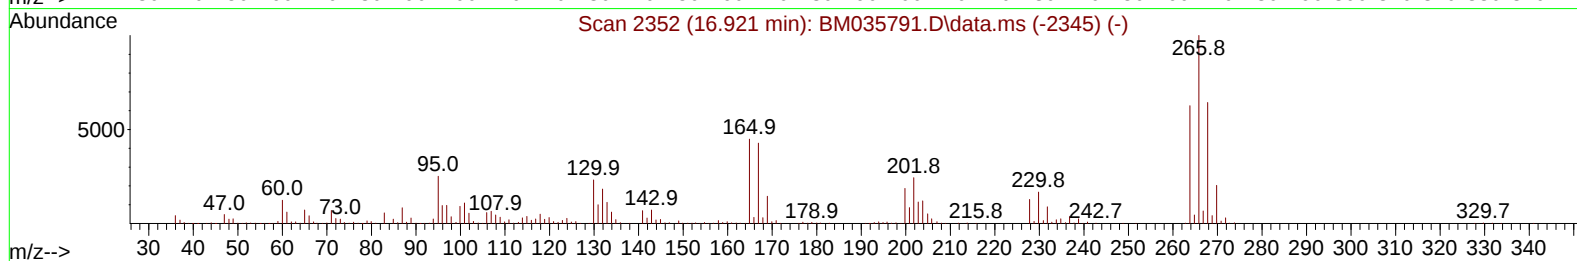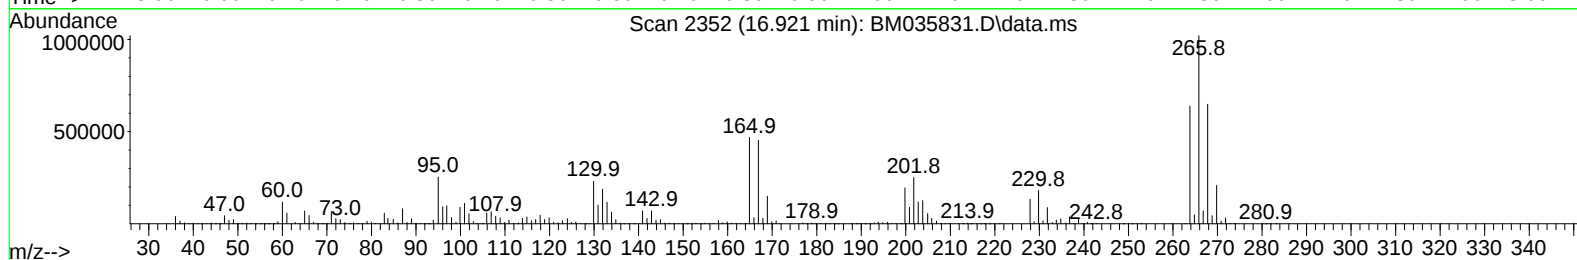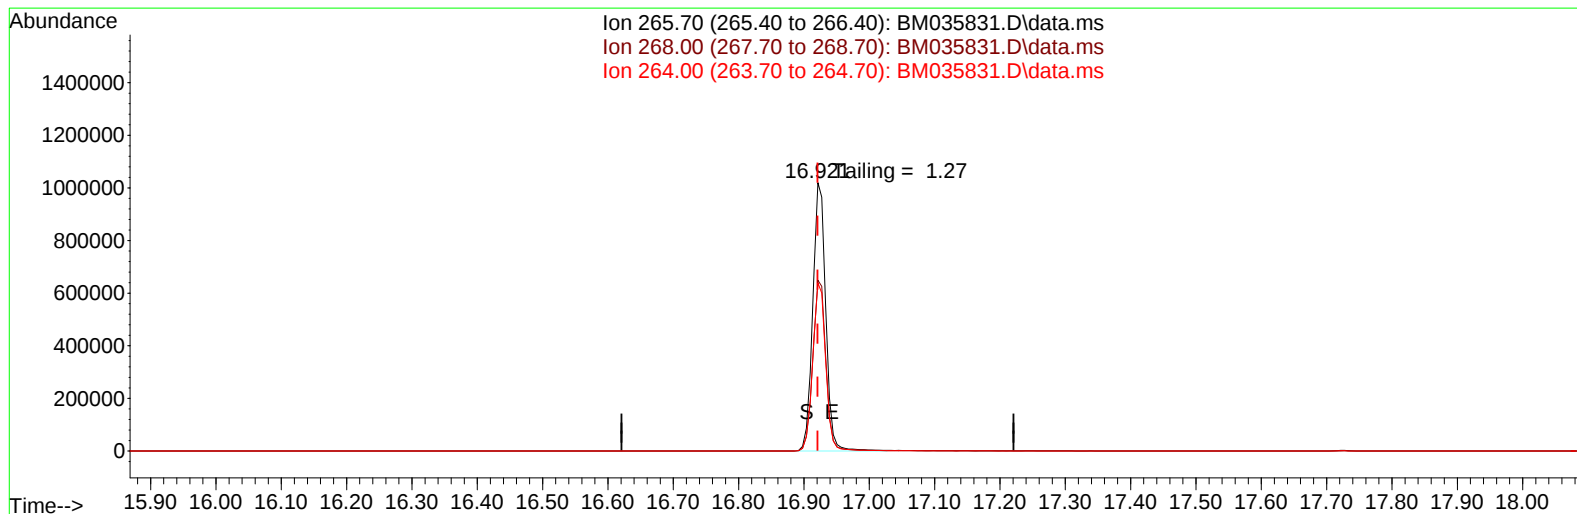

TIC: BM035831.D\data.ms

(70) Pentachlorophenol (C)

16.921min (+ 0.000) 140687.72 ng




response 1417194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.60
264.00	63.30	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071522\
Data File : BM035831.D
Acq On : 15 Jul 2022 15:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 16 05:08:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 14 01:21:21 2022
Response via : Initial Calibration

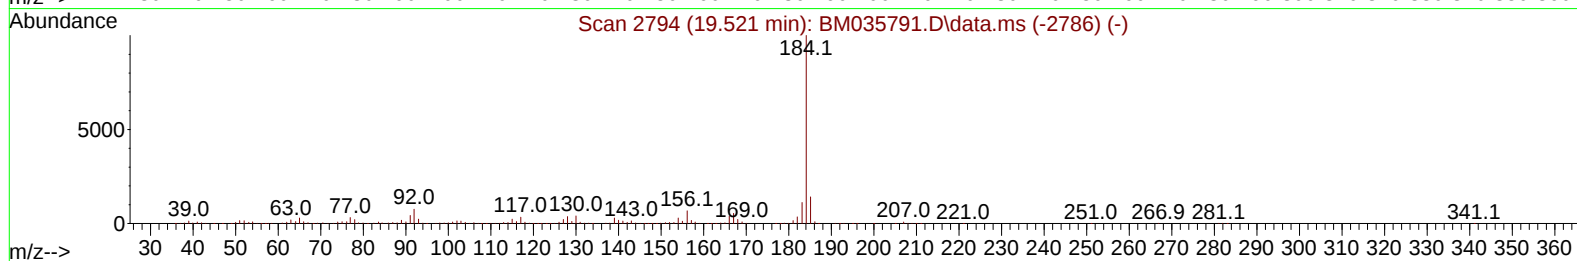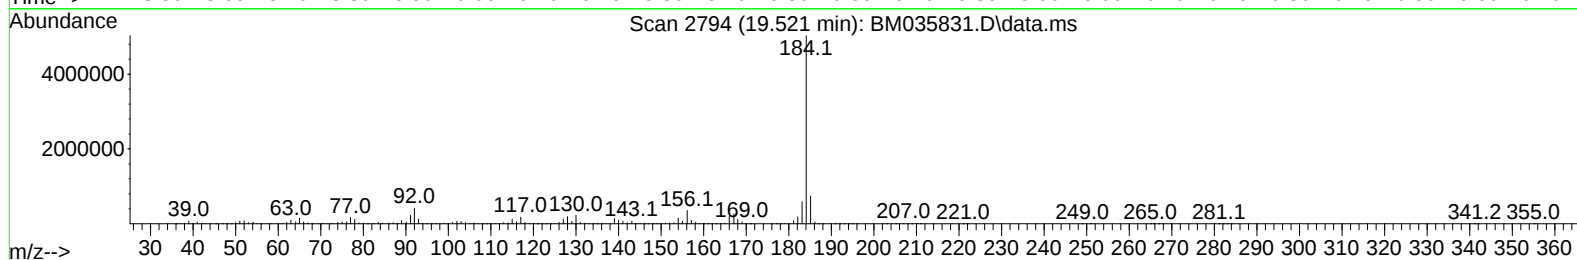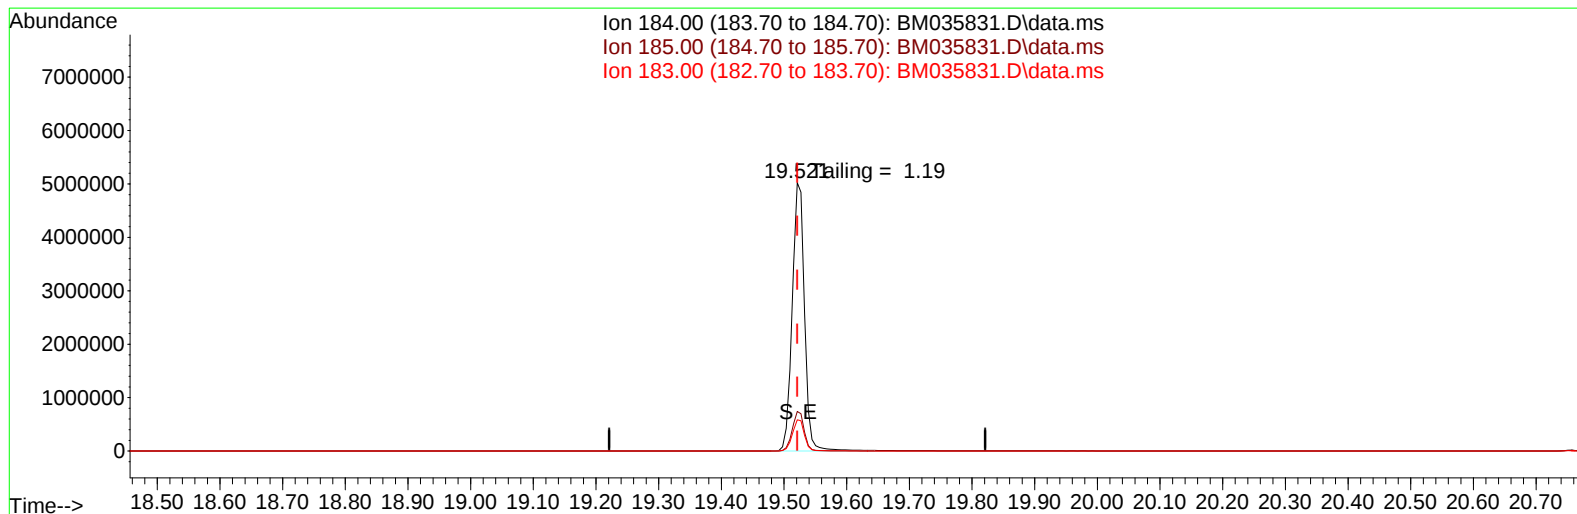

TIC: BM035831.D\data.ms

(77) Benzidine

19.521min (+ 0.000) 217785.81 ng

response 6905930

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.71
183.00	11.90	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/15/2022	BNA_M	<u>BM035831.D</u>
Compound Name	Response	Retention Time
DDT	3711903	20.756
DDD	36782	20.309
DDE	5819	19.809
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42601	3754504	1.13

Instrument :
BNA_M
ClientSampleId :
DFTPP