

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071615\
 Data File : BM001945.D
 Acq On : 16 Jul 2015 14:28
 Operator : TP/UM
 Sample : G2998-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01F5

Quant Time: Jul 17 00:38:01 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 17 00:28:51 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	57529	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	257174	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	175163	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	423827	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	532061	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	536016	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	6330	5.38	ng/uL	0.00
5) Phenol-d5	6.82	99	147765	31.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	87554	34.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	122159	32.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	129377	33.54	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	61571	32.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	72350	33.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	133167	30.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	161035	36.37	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	461613	32.67	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	499298	29.38	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	72629	30.36	ng/ul	0.00
57) Fluorene-d10	15.30	176	350842	29.06	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	64519	23.51	ng/ul	0.00
70) Anthracene-d10	17.15	188	556670	27.98	ng/ul	0.00
78) Pyrene-d10	19.46	212	586949	24.15	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	595733	21.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.77	163	188835	13.14	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071615\
Data File : BM001945.D
Acq On : 16 Jul 2015 14:28
Operator : TP/UM
Sample : G2998-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
C01F5

Quant Time: Jul 17 00:38:01 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 17 00:28:51 2015
Response via : Initial Calibration

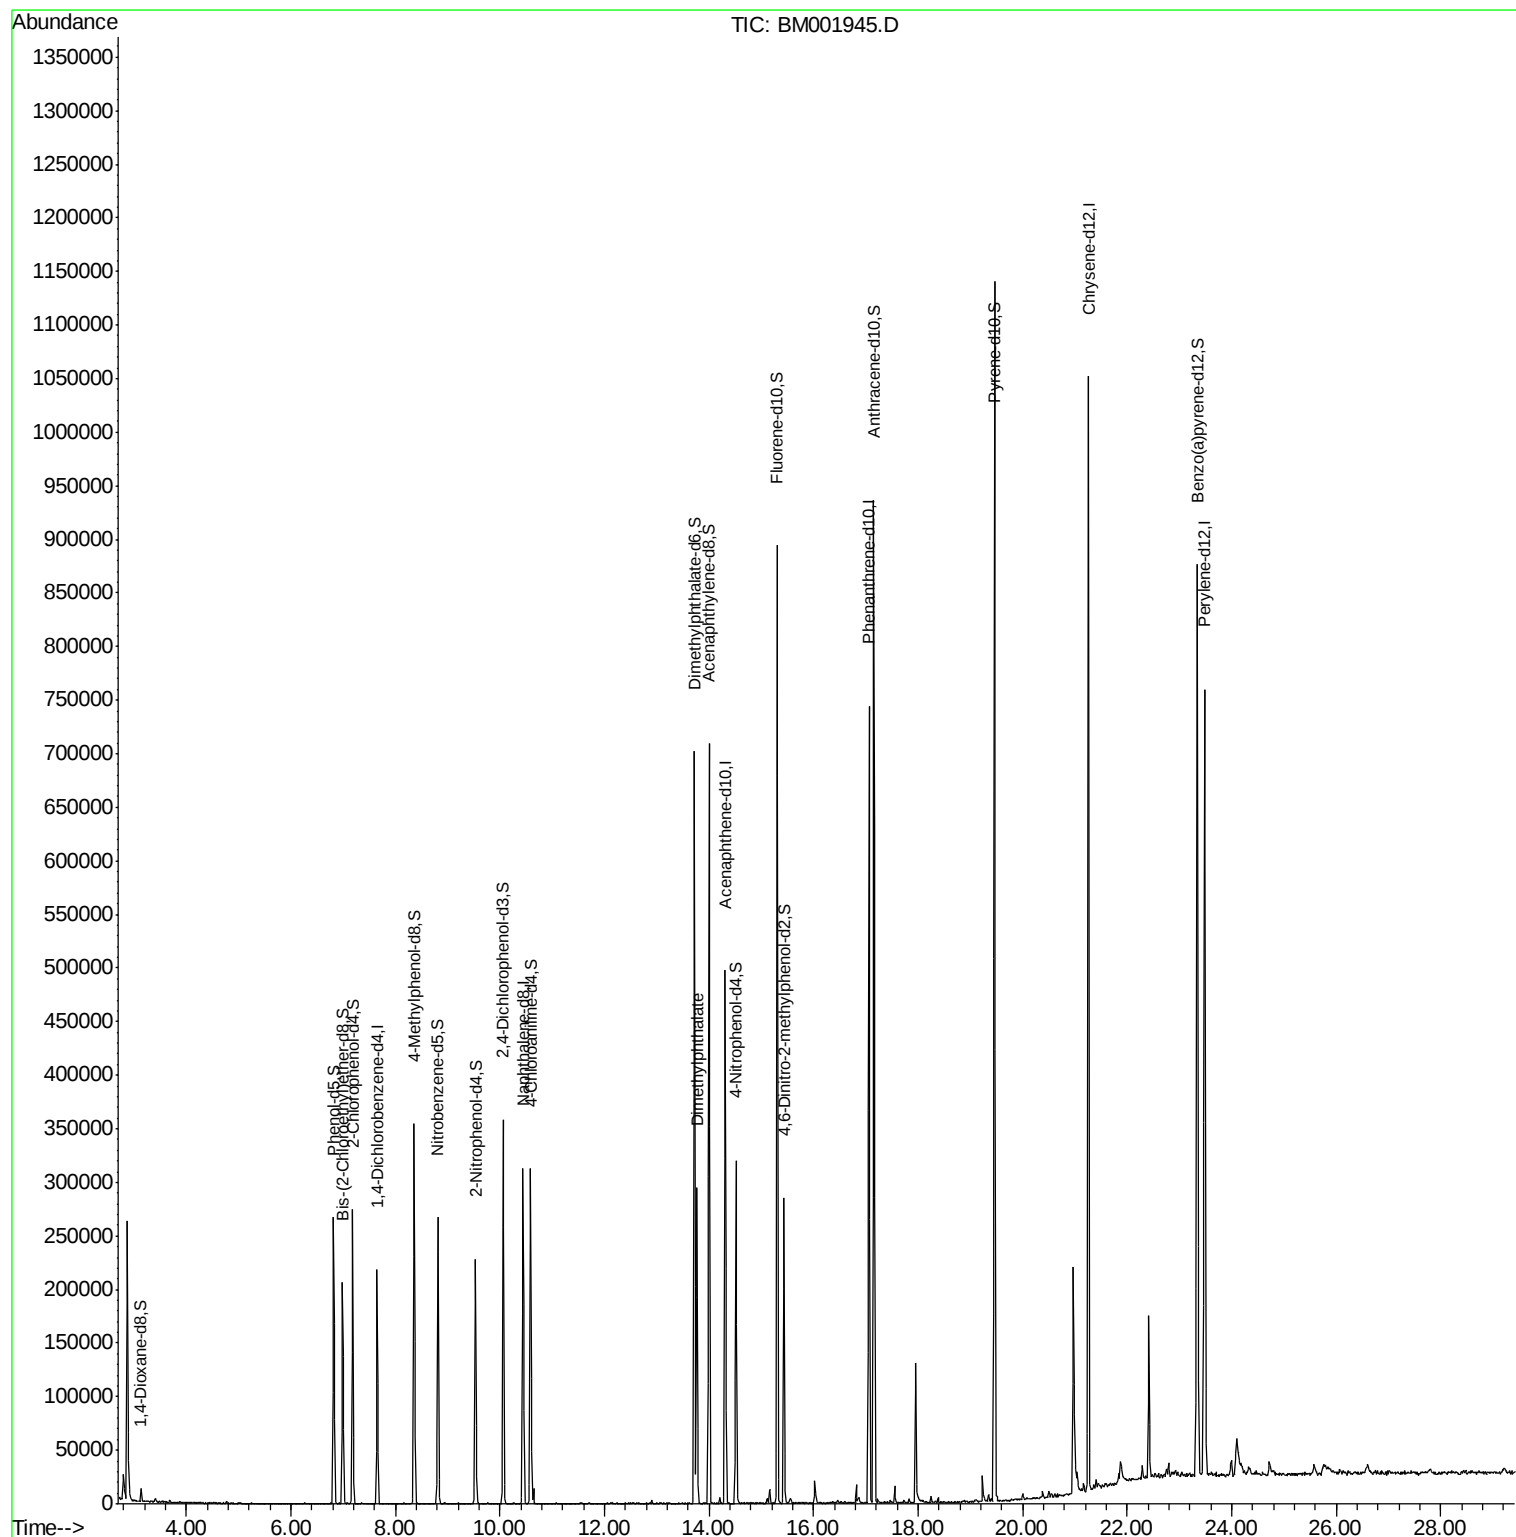

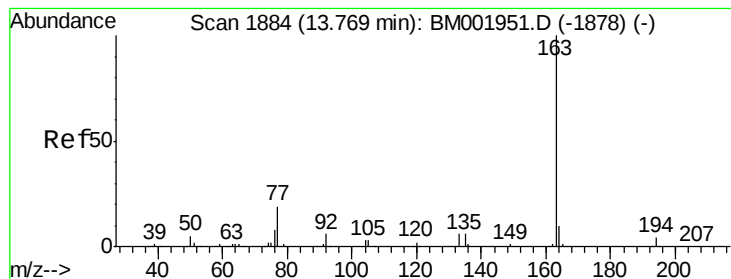

#44

Dimethylphthalate

Concen: 13.14 ng/ul

RT: 13.77 min Scan# 1884

Delta R.T. 0.00 min

Lab File: BM001945.D


Acq: 16 Jul 2015 14:28

Instrument :

BNA_M

ClientSampleId :

C01F5

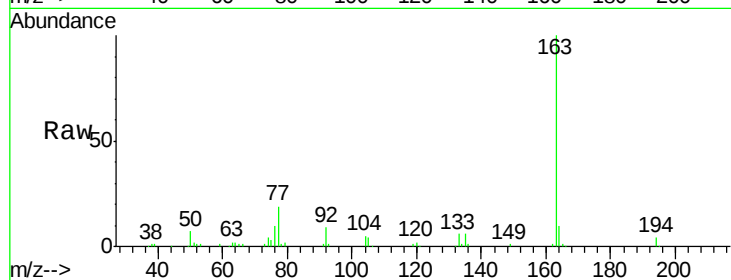


Tgt Ion:163 Resp: 188835

Ion Ratio Lower Upper

163 100

194 4.4 3.3 4.9

164 10.1 7.6 11.4

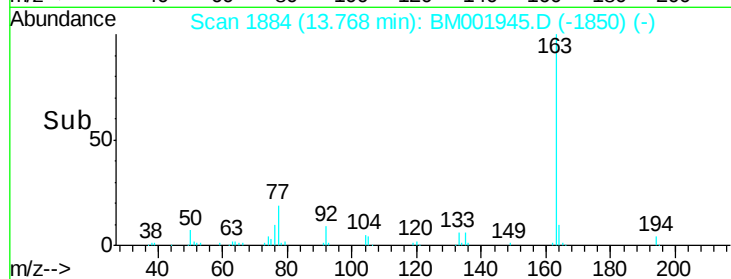

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

