


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071615\
 Data File : BM001942.D
 Acq On : 16 Jul 2015 11:38
 Operator : TP/UM
 Sample : DFTPP76
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP76

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042815.M
 Title : SVOA CALIBRATION
 Last Update : Tue Apr 28 06:36:34 2015

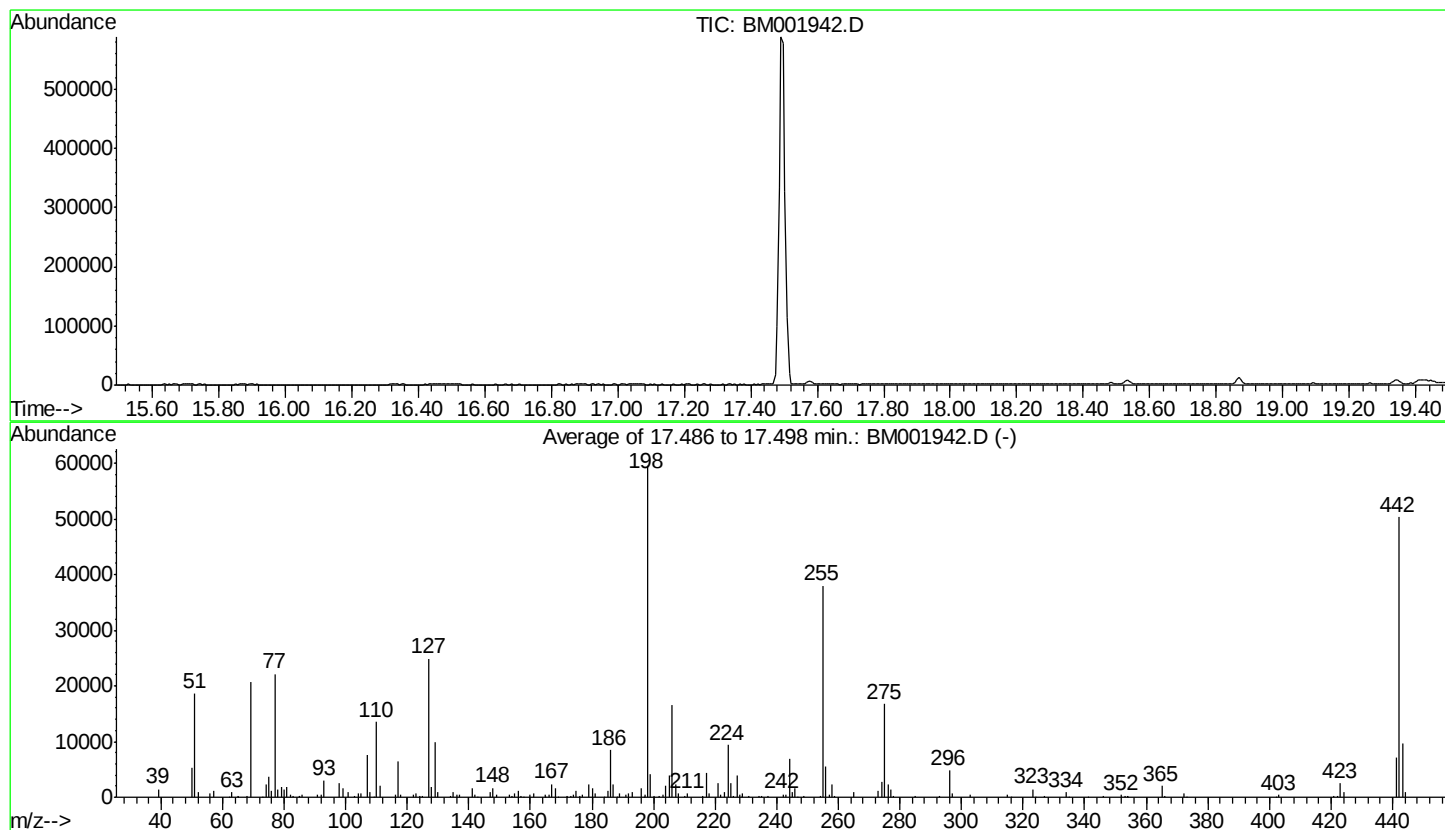

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	18617	PASS
68	69	0.00	2	0.7	151	PASS
69	198	0.00	100	34.8	20752	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	24877	PASS
197	198	0.00	2	0.7	435	PASS
198	198	100	100	100.0	59576	PASS
199	198	5	9	6.8	4046	PASS
275	198	10	60	28.2	16788	PASS
365	198	1	100	3.3	1968	PASS
441	443	0.01	100	74.0	7126	PASS
442	198	50	100	84.5	50344	PASS
443	442	15	24	19.1	9631	PASS

m/z	Abundance
39.00	1059.0
39.90	371.0
43.90	557.0
50.00	4099.0
51.10	15277.0
52.00	804.0
55.90	413.0
57.00	987.0
63.10	708.0
64.90	339.0
68.00	455.0
69.00	16728.0
73.00	380.0
74.00	1934.0
75.00	2750.0
76.00	772.0
77.00	17336.0
78.00	1226.0
79.00	1390.0
80.00	896.0
81.00	1288.0
81.90	381.0
82.90	325.0
86.00	416.0
91.00	404.0
92.00	372.0
93.00	2288.0
98.00	1842.0
99.00	1342.0
101.00	750.0
104.00	505.0
104.90	413.0
107.00	5762.0
108.00	734.0
110.00	9852.0
111.00	1645.0
116.00	367.0
117.00	4966.0
117.90	392.0
122.00	471.0
122.90	536.0
125.00	357.0
127.00	17832.0
128.00	1368.0
129.00	7306.0
129.90	639.0
134.90	644.0
136.00	320.0
137.00	330.0
140.90	1229.0
147.00	772.0
147.90	1185.0
149.10	387.0
153.00	377.0
155.00	713.0
156.00	775.0
159.90	338.0
160.90	500.0
164.80	324.0
167.00	1699.0
168.00	1324.0
174.00	398.0
174.90	749.0
177.10	502.0
179.00	1470.0
180.00	1027.0
181.00	439.0
185.10	823.0
186.00	5484.0
187.00	1478.0
188.90	533.0
190.90	311.0
192.00	387.0
193.00	589.0
196.00	1209.0
196.70	322.0
197.10	301.0
197.90	41480.0
198.90	2773.0
202.90	332.0
204.10	1238.0
205.10	2802.0
206.00	11155.0
207.00	2260.0
208.10	413.0
211.00	483.0
217.00	2976.0
218.00	463.0
221.10	1357.0
222.00	459.0
223.00	583.0

Instrument :
BNA_M
ClientSampleId :
DFTPP76

224.00	6589.0
225.00	1746.0
226.00	302.0
227.00	2535.0
227.90	417.0
228.80	473.0
242.00	324.0
244.00	4259.0
245.00	781.0
246.00	1175.0
254.20	348.0
255.00	23728.0
256.00	3503.0
257.00	388.0
258.00	1516.0
264.90	641.0
273.00	654.0
274.00	1621.0
275.00	10381.0
276.00	1444.0
276.90	889.0
296.00	2737.0
296.90	436.0
302.90	313.0
323.00	942.0
334.00	524.0
353.90	312.0
365.10	890.0
372.00	536.0
423.10	1189.0
424.00	645.0
441.10	3611.0
442.00	24728.0
443.10	5344.0
444.00	553.0

Instrument :

BNA_M

ClientSampleId :

DFTPP76

m/z	Abundance
39.10	1714.0
40.00	359.0
44.00	668.0
50.00	6399.0
51.00	21936.0
52.00	1076.0
56.00	676.0
57.00	1495.0
62.10	309.0
63.00	949.0
65.10	525.0
69.00	24464.0
73.00	512.0
74.00	2612.0
75.00	4320.0
76.00	1303.0
77.10	27272.0
78.00	1784.0
79.00	1920.0
80.00	1419.0
81.00	2185.0
82.00	599.0
82.90	529.0
84.90	461.0
86.00	686.0
91.00	687.0
91.90	591.0
93.00	3385.0
98.00	2902.0
99.00	2093.0
100.90	1202.0
102.80	421.0
103.90	864.0
105.00	803.0
107.00	9140.0
108.00	1159.0
109.00	308.0
110.00	15910.0
111.00	2439.0
116.00	433.0
117.00	7914.0
118.00	687.0
122.00	613.0
123.00	1098.0
123.90	418.0
124.90	350.0
127.00	30144.0
128.00	2363.0
129.00	12128.0
129.90	1009.0
134.00	422.0
135.00	950.0
135.90	469.0
137.10	477.0
141.00	2220.0
141.90	643.0
142.80	312.0
147.00	985.0
148.00	2014.0
149.00	565.0
152.90	492.0
154.00	398.0
155.00	930.0
156.00	1396.0
160.00	410.0
161.00	785.0
165.00	623.0
166.10	554.0
167.00	3291.0
168.00	1970.0
169.00	353.0
171.80	445.0
172.90	312.0
174.00	713.0
175.00	1364.0
177.00	555.0
179.00	2826.0
180.00	1879.0
181.00	820.0
183.90	337.0
185.00	1364.0
186.00	10232.0
187.00	3023.0
187.90	357.0
188.90	696.0
190.90	403.0
192.00	800.0
193.00	1042.0
196.00	2082.0
197.10	599.0
198.00	69160.0

Instrument :
BNA_M
ClientSampleId :
DFTPP76

199.00	5150.0
200.00	413.0
201.60	390.0
203.00	581.0
204.10	2707.0
205.00	4051.0
206.10	19008.0
207.00	3198.0
208.00	777.0
210.00	405.0
211.00	662.0
215.90	482.0
217.00	5156.0
218.00	765.0
221.10	3410.0
223.00	1071.0
224.10	11026.0
225.00	2758.0
226.10	332.0
227.00	4794.0
228.00	575.0
229.00	1104.0
230.90	451.0
236.90	534.0
242.00	466.0
243.00	568.0
244.00	7989.0
245.00	961.0
246.00	1778.0
254.20	450.0
255.00	44344.0
256.00	6672.0
257.00	599.0
258.00	2400.0
258.90	484.0
265.00	895.0
273.00	1539.0
274.00	3194.0
275.00	19192.0
276.00	2606.0
277.00	1830.0
278.00	374.0
284.90	394.0
292.90	351.0
296.00	5499.0
297.00	672.0
303.00	701.0
315.00	739.0
316.10	320.0
323.00	1672.0
323.90	302.0
334.00	994.0
335.00	315.0
341.00	365.0
352.00	484.0
353.00	409.0
354.10	525.0
365.00	2190.0
365.90	379.0
372.10	678.0
403.00	430.0
422.00	451.0
423.00	2938.0
424.00	987.0
441.00	7721.0
442.10	56080.0
443.10	10842.0
444.00	920.0

Instrument :
BNA_M
ClientSampleId :
DFTPP76

m/z	Abundance
39.10	1451.0
40.00	325.0
43.90	570.0
50.10	5206.0
51.00	18640.0
52.00	1061.0
56.00	693.0
57.00	1170.0
63.00	789.0
65.00	329.0
69.00	21064.0
73.00	320.0
74.00	2458.0
75.00	3696.0
76.00	1225.0
77.10	21992.0
78.00	1410.0
79.00	1933.0
79.90	1688.0
81.00	1819.0
82.00	556.0
85.10	398.0
86.00	540.0
91.00	446.0
91.90	506.0
93.00	3052.0
98.00	2527.0
99.00	1630.0
101.00	882.0
102.80	444.0
104.00	684.0
105.00	630.0
107.00	7991.0
108.00	1110.0
110.00	14916.0
111.00	2357.0
116.10	492.0
117.00	6622.0
117.90	618.0
122.00	664.0
123.00	677.0
123.90	442.0
127.00	26656.0
128.00	2120.0
129.00	10400.0
129.90	938.0
133.90	393.0
134.90	1069.0
136.00	415.0
137.00	573.0
141.00	1685.0
142.00	535.0
147.00	913.0
147.90	1957.0
149.00	342.0
152.90	454.0
155.00	782.0
156.00	1259.0
157.10	383.0
157.90	345.0
160.00	526.0
160.90	781.0
165.00	535.0
166.10	646.0
167.00	3159.0
168.00	1657.0
172.00	319.0
173.00	387.0
173.90	607.0
175.00	1213.0
176.00	384.0
176.90	624.0
179.00	2678.0
180.00	1918.0
180.90	835.0
184.90	1259.0
186.00	9638.0
187.00	2355.0
188.90	662.0
191.00	365.0
192.00	1035.0
193.00	1001.0
195.90	1752.0
197.10	405.0
198.00	68088.0
198.90	4216.0
200.00	352.0
203.00	522.0
204.00	2430.0
205.00	4556.0
206.00	19624.0

Instrument :
BNA_M
ClientSampleId :
DFTPP76

207.10	2952.0
208.00	771.0
210.00	338.0
211.10	850.0
215.90	342.0
217.00	4795.0
217.90	660.0
221.10	2816.0
221.80	667.0
223.00	1158.0
224.00	10641.0
225.00	2976.0
227.00	4705.0
227.90	610.0
228.90	911.0
231.00	346.0
234.10	399.0
234.90	418.0
237.00	368.0
242.00	668.0
243.10	732.0
244.10	8140.0
245.00	1273.0
246.00	1955.0
246.80	344.0
248.90	380.0
255.00	45776.0
256.00	6085.0
257.00	536.0
258.00	2883.0
258.90	467.0
265.00	1315.0
273.00	1410.0
274.00	3451.0
275.00	20792.0
276.00	2609.0
277.00	1760.0
292.90	410.0
296.00	6157.0
296.90	958.0
303.00	629.0
315.00	716.0
323.00	1759.0
326.90	427.0
334.00	1157.0
346.00	403.0
352.00	659.0
352.90	335.0
354.10	496.0
365.00	2824.0
365.90	399.0
372.00	1030.0
373.00	309.0
402.00	312.0
403.00	656.0
421.00	470.0
421.90	436.0
423.10	3155.0
424.00	849.0
441.10	10046.0
442.10	70224.0
443.10	12709.0
444.00	1035.0

Instrument :
BNA_M
ClientSampleId :
DFTPP76

m/z	Abundance
39.90	379.0
44.00	668.0
73.00	396.0
167.00	328.0
206.90	500.0

Instrument :
BNA_M
ClientSampleId :
DFTPP76