

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071616\
 Data File : BM006481.D
 Acq On : 16 Jul 2016 16:22
 Operator : UM/SJ
 Sample : H3959-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 18 06:18:05 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 23:20:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	149826	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	645024	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	365036	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	844023	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	990075	20.00	ng/ul	-0.01
83) Perylene-d12	23.41	264	1044779	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	6068	1.71	ng/uL	0.00
5) Phenol-d5	6.79	99	264964	21.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	175080	23.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	219105	22.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	218328	22.38	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	104529	21.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	113883	20.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	201741	19.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	278598	25.56	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	674606	22.58	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	839021	22.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	92873	17.89	ng/ul	0.00
57) Fluorene-d10	15.27	176	599695	22.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	70098	14.36	ng/ul	0.00
70) Anthracene-d10	17.12	188	951210	23.84	ng/ul	0.00
76) Pyrene-d10	19.42	212	1089851	24.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1191535	24.94	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.73	163	380672	12.56	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071616\
Data File : BM006481.D
Acq On : 16 Jul 2016 16:22
Operator : UM/SJ
Sample : H3959-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 18 06:18:05 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 23:20:22 2016
Response via : Initial Calibration

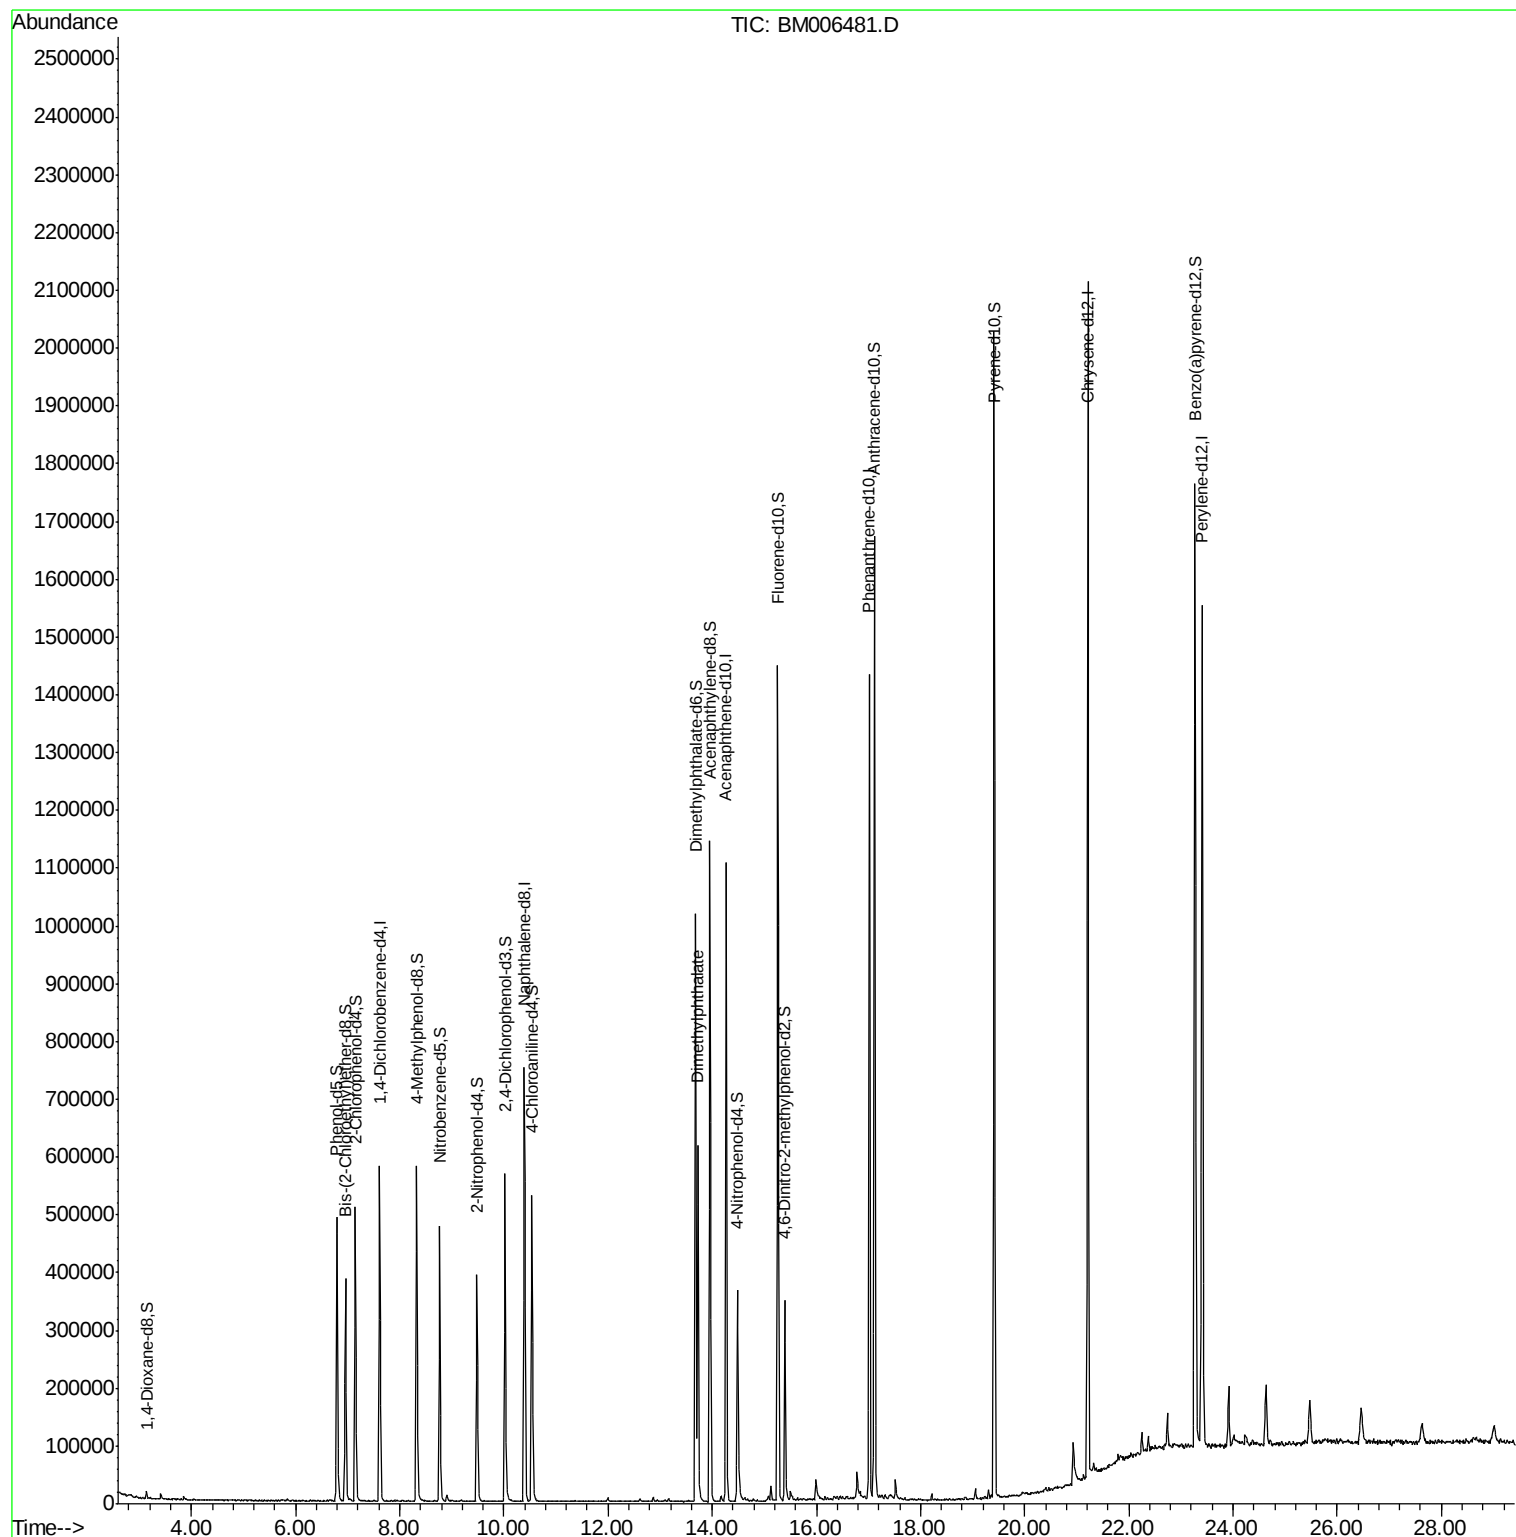

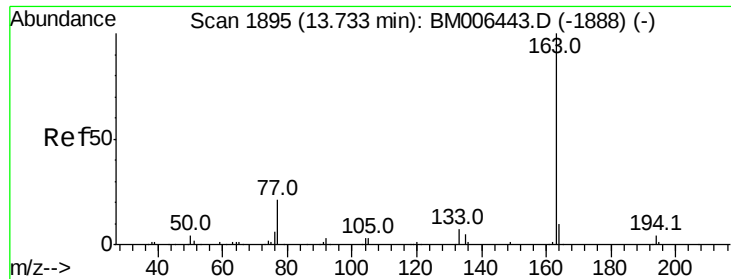

#44

Dimethylphthalate

Concen: 12.56 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BM006481.D

Acq: 16 Jul 2016 16:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 380672

Ion Ratio Lower Upper

163 100

194 3.7 3.4 5.0

164 9.8 7.8 11.8

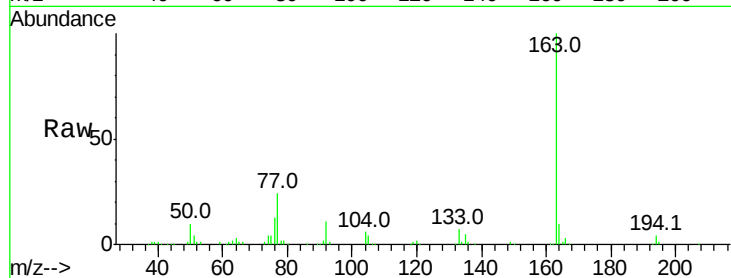

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

