

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071616\
 Data File : BM006498.D
 Acq On : 17 Jul 2016 03:19
 Operator : UM/SJ
 Sample : H3985-14
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 18 06:20:18 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 23:20:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	171280	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	705311	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	392415	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	891015	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	1149357	20.00	ng/ul	-0.01
83) Perylene-d12	23.41	264	1286590	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	10346	2.54	ng/uL	0.00
5) Phenol-d5	6.79	99	464629	33.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	290721	34.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	362746	31.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	365346	32.76	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	176297	32.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	195690	32.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	335554	29.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	470150	39.44	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	1092231	34.01	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1345601	33.89	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	192420	34.49	ng/ul	0.00
57) Fluorene-d10	15.26	176	939452	32.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	147255	28.57	ng/ul	0.00
70) Anthracene-d10	17.12	188	1488492	35.34	ng/ul	0.00
76) Pyrene-d10	19.42	212	1741462	33.42	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	2085710	35.45	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.32	70	10012	1.08	ng/ul#	1
44) Dimethylphthalate	13.73	163	456861	14.02	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071616\
Data File : BM006498.D
Acq On : 17 Jul 2016 03:19
Operator : UM/SJ
Sample : H3985-14
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 18 06:20:18 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 23:20:22 2016
Response via : Initial Calibration




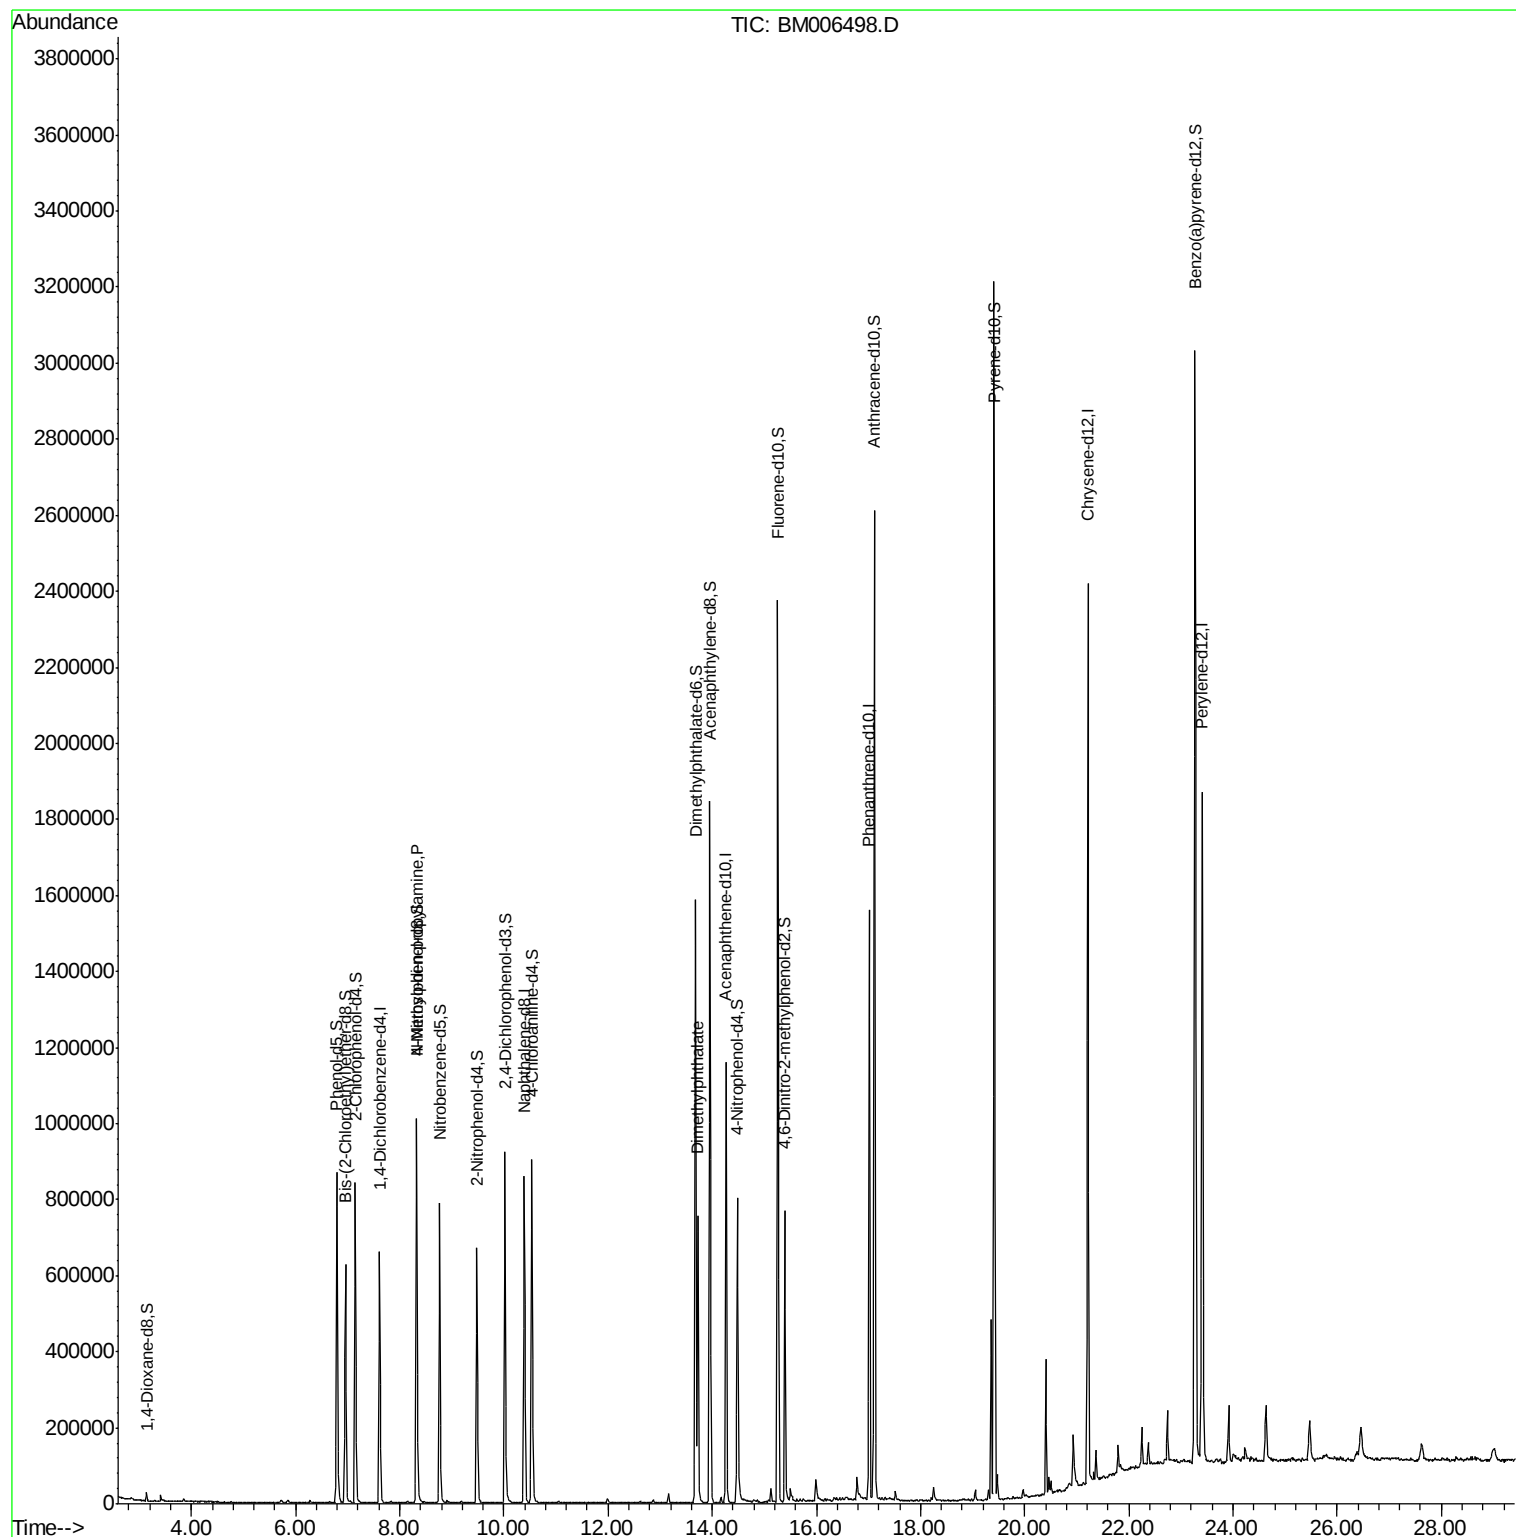


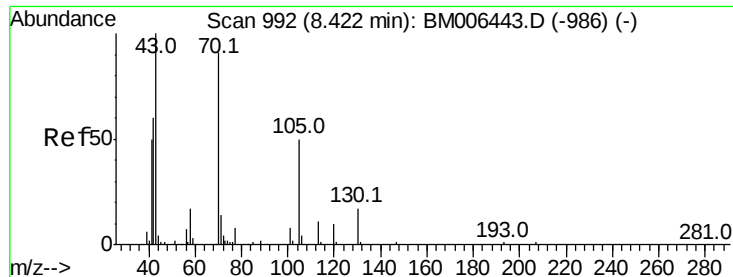

#15
N-Nitroso-di-n-propylamine
Concen: 1.08 ng/ul
RT: 8.32 min Scan# 975
Delta R.T. -0.10 min
Lab File: BM006498.D
Acq: 17 Jul 2016 03:19

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
70	100		
42	382.9	50.6	75.8#
101	0.0	7.9	11.9#
130	0.0	15.8	23.6#

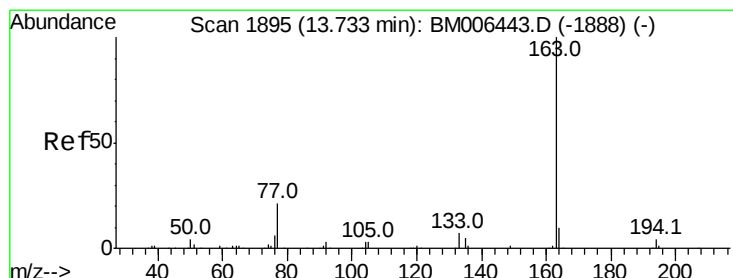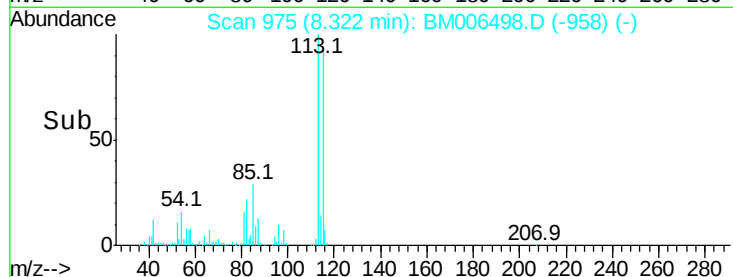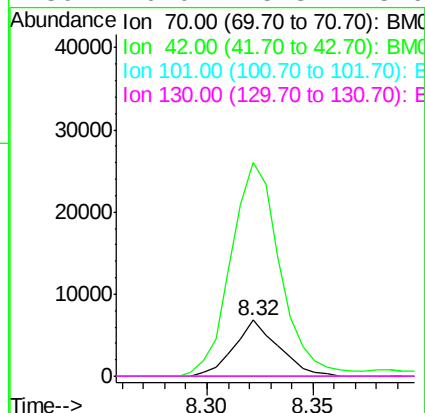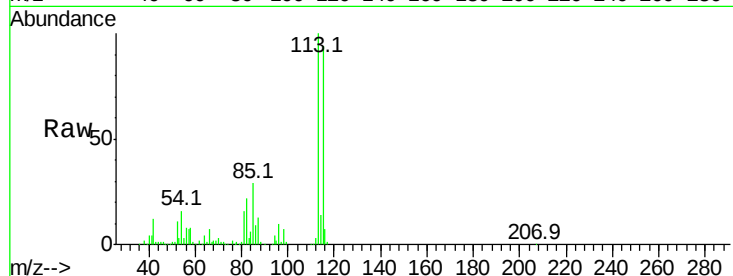

#44
Dimethylphthalate
Concen: 14.02 ng/ul
RT: 13.73 min Scan# 1894
Delta R.T. -0.01 min
Lab File: BM006498.D
Acq: 17 Jul 2016 03:19

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	10.3	7.8	11.8

