

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071616\
 Data File : BM006513.D
 Acq On : 17 Jul 2016 13:00
 Operator : UM/SJ
 Sample : H3985-22
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 18 07:44:37 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 18 07:39:41 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	158132	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	677746	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	376640	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	848513	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	998615	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1038764	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	10613	2.83	ng/uL	0.00
5) Phenol-d5	6.79	99	494153	38.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	313034	39.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	386503	36.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	394568	38.32	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	192462	37.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	213074	36.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	370173	33.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	488747	42.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	1163213	37.73	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1455308	38.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	198173	37.01	ng/ul	0.00
57) Fluorene-d10	15.26	176	1006573	36.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	147625	30.08	ng/ul	0.00
70) Anthracene-d10	17.12	188	1540251	38.40	ng/ul	0.00
76) Pyrene-d10	19.42	212	1726843	38.14	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1856158	39.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	6.82	94	18292	1.34	ng/ul#	81
44) Dimethylphthalate	13.73	163	493758	15.79	ng/ul	99
69) Phenanthrene	17.06	178	88540	1.90	ng/ul	96
71) Anthracene	17.15	178	53541	1.12	ng/ul	100
74) Fluoranthene	19.08	202	184924	3.41	ng/ul	99
77) Pyrene	19.44	202	178071	2.99	ng/ul	98
80) Benzo(a)anthracene	21.25	228	145651	2.39	ng/ul	92
82) Chrysene	21.25	228	145651	2.54	ng/ul	95
85) Benzo(b)fluoranthene	22.76	252	173003	2.79	ng/ul#	96
86) Benzo(k)fluoranthene	22.76	252	173003	2.96	ng/ul	96
88) Benzo(a)pyrene	23.32	252	153338	2.58	ng/ul	99
89) Indeno(1,2,3-cd)pyrene	25.60	276	86906	1.26	ng/ul	96
91) Benzo(g,h,i)perylene	26.27	276	77327	1.26	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071616\
Data File : BM006513.D
Acq On : 17 Jul 2016 13:00
Operator : UM/SJ
Sample : H3985-22
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 18 07:44:37 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 18 07:39:41 2016
Response via : Initial Calibration

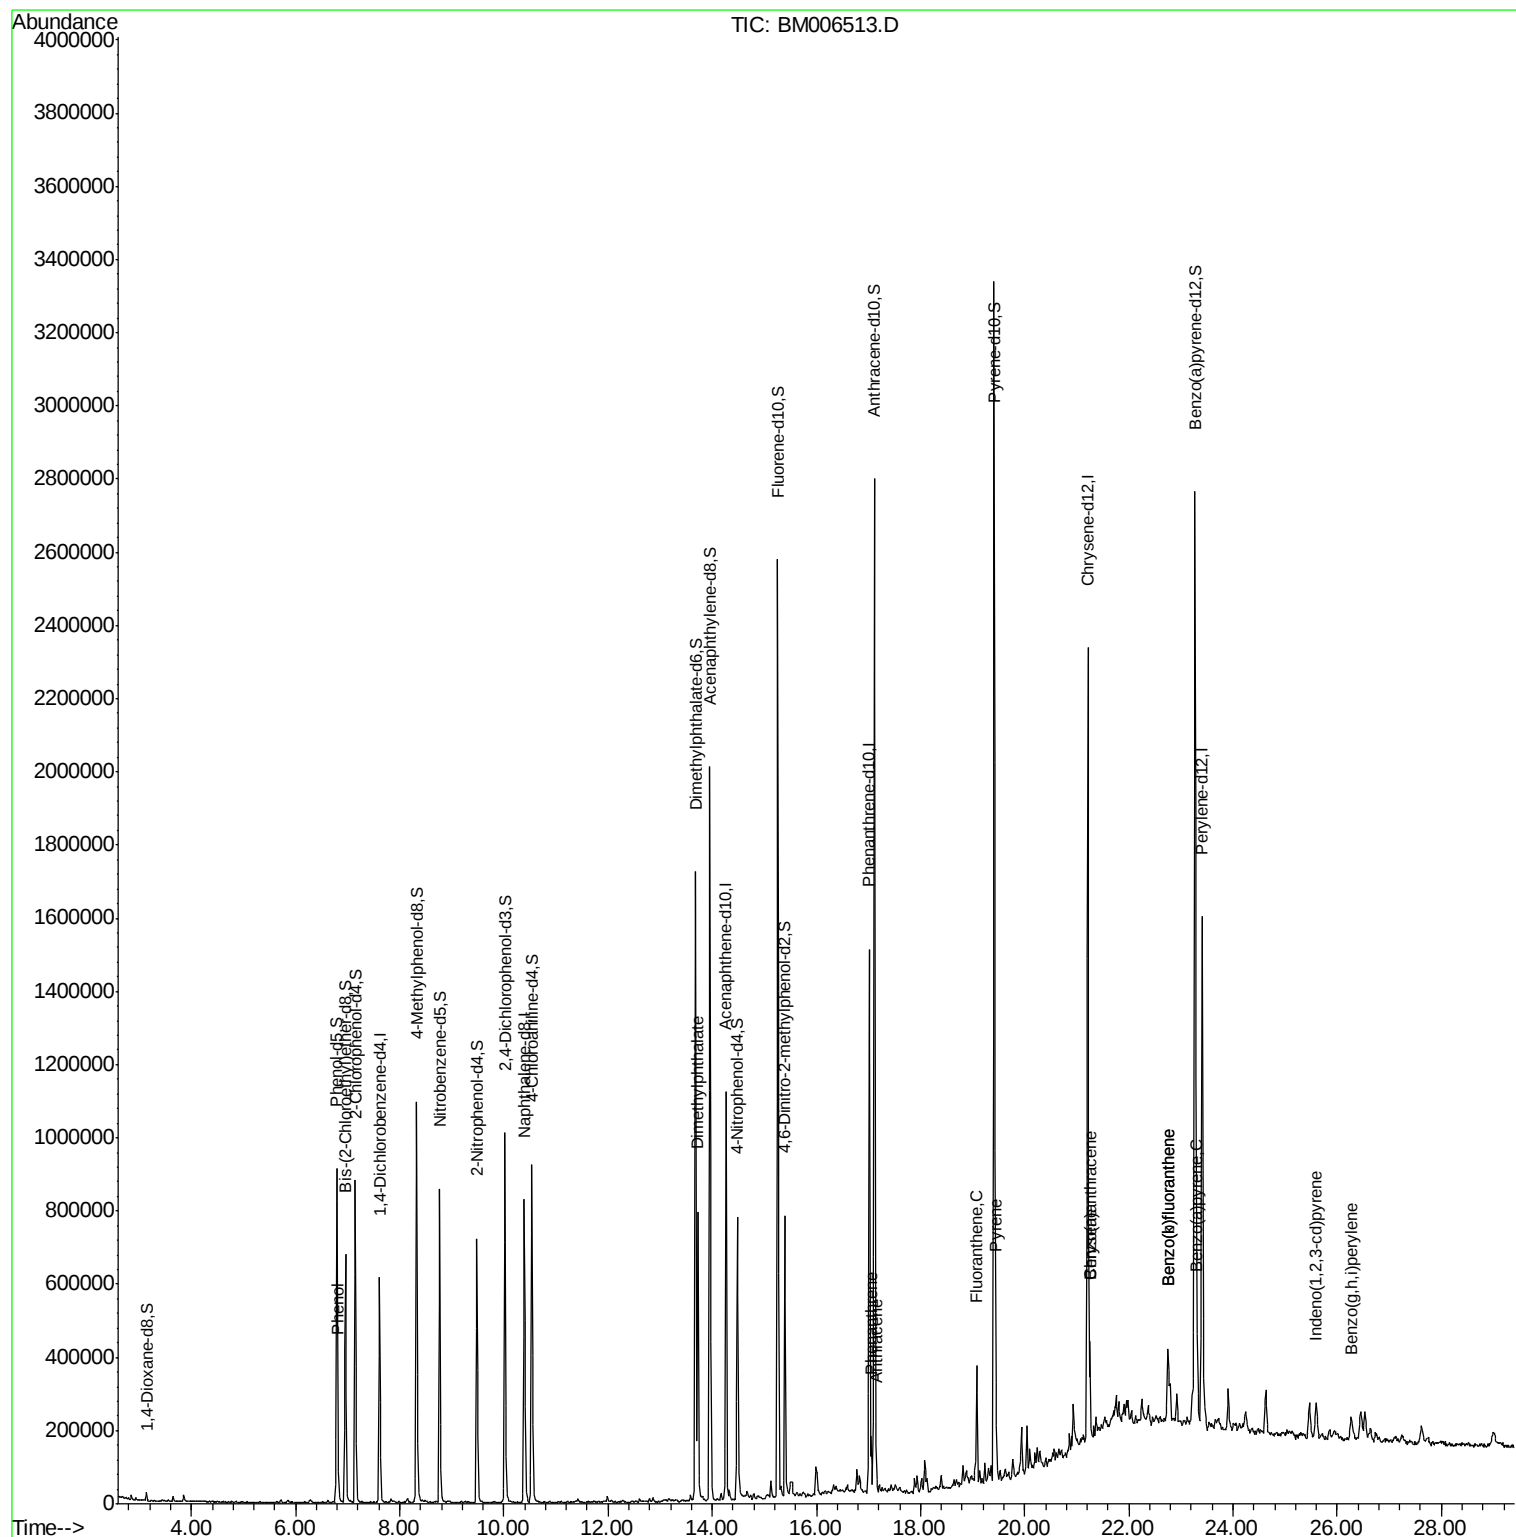

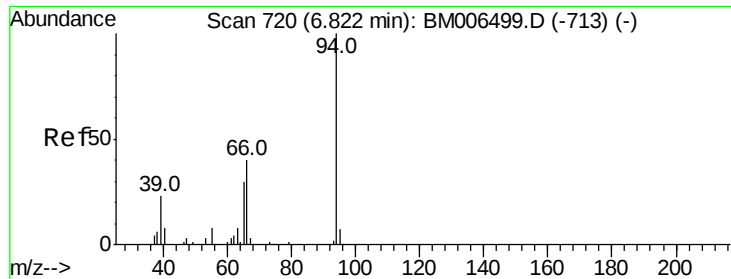

#6

Phenol

Concen: 1.34 ng/ul

RT: 6.82 min Scan# 719

Delta R.T. -0.01 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00

Instrument :

BNA_M

ClientSampleId :





Tot Ion: 94 Resp: 18292

Ion Ratio Lower Upper

94 100

65 33.3 25.8 38.8

66 64.9 35.7 53.5#

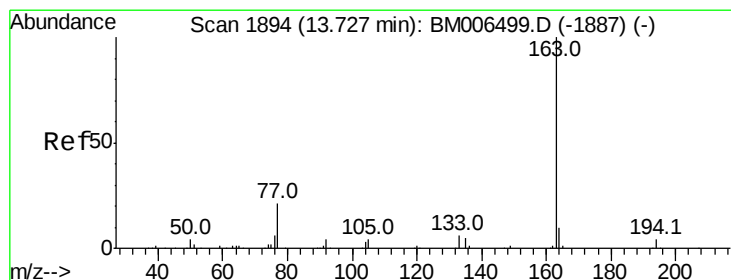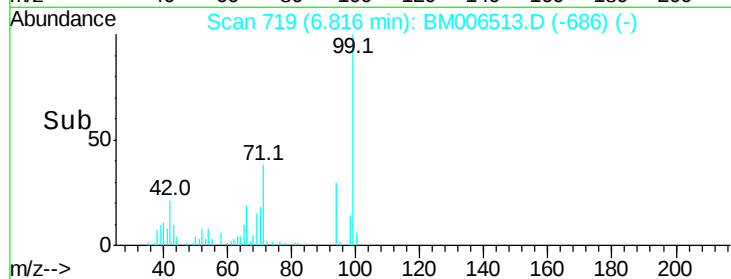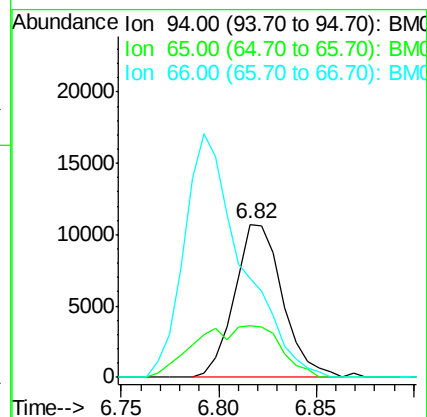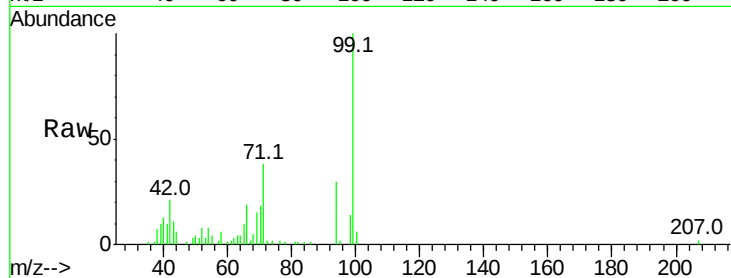

#44

Dimethylphthalate

Concen: 15.79 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. 0.00 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00




Tgt Ion:163 Resp: 493758


Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.2 7.8 11.8

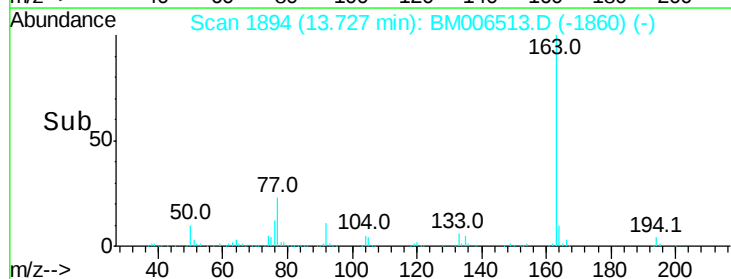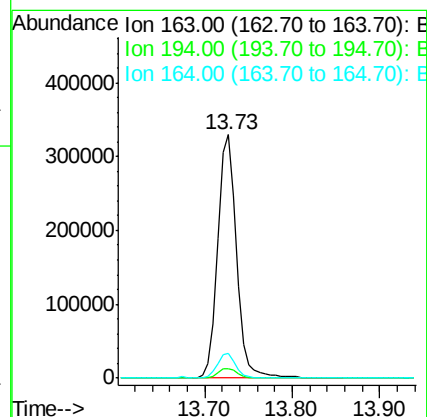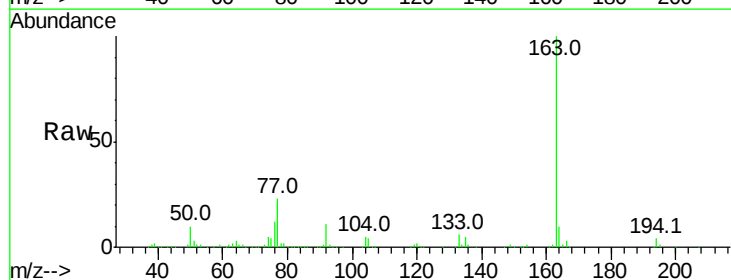

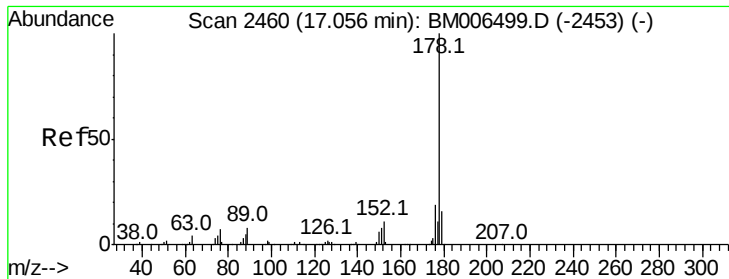

#69

Phenanthrene

Concen: 1.90 ng/ul

RT: 17.06 min Scan# 2460

Delta R.T. 0.00 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00

Instrument :

BNA_M

ClientSampleId :


Tot Ion:178 Resp: 88540

Ion Ratio Lower Upper

178 100

179 16.3 11.9 17.9




176 20.9 15.2 22.8

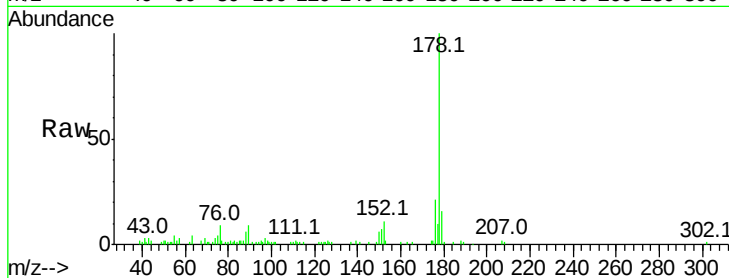

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

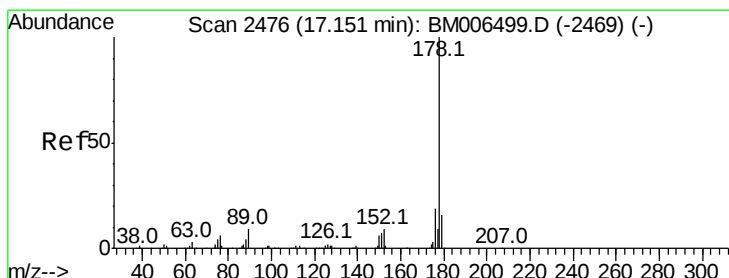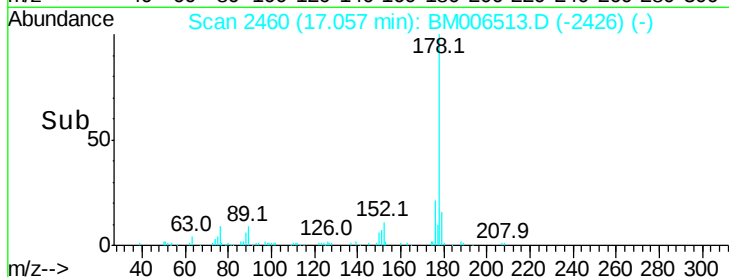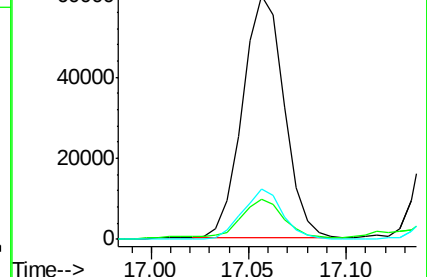

#71

Anthracene

Concen: 1.12 ng/ul

RT: 17.15 min Scan# 2476

Delta R.T. 0.00 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00


Tgt Ion:178 Resp: 53541

Ion Ratio Lower Upper

178 100

179 15.0 12.0 18.0



176 18.9 15.0 22.6

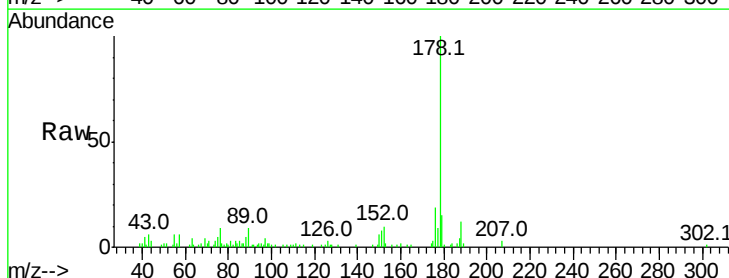


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

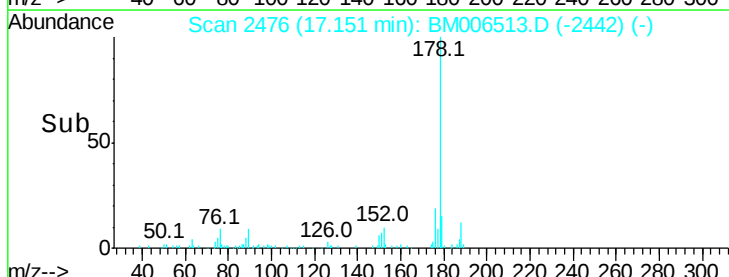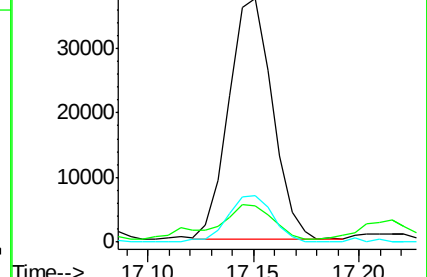

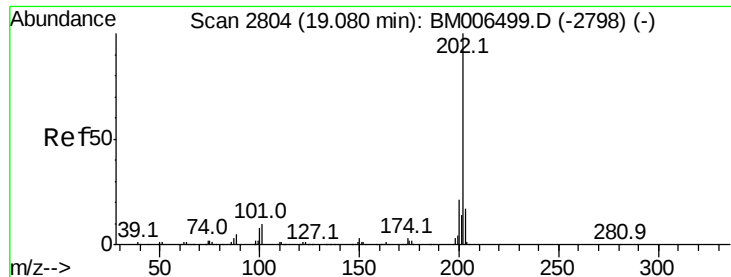

#74

Fluoranthene

Concen: 3.41 ng/ul

RT: 19.08 min Scan# 2804

Delta R.T. 0.00 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 184924

Ion Ratio Lower Upper

202 100

101 11.0 8.6 12.8




100 8.2 6.4 9.6

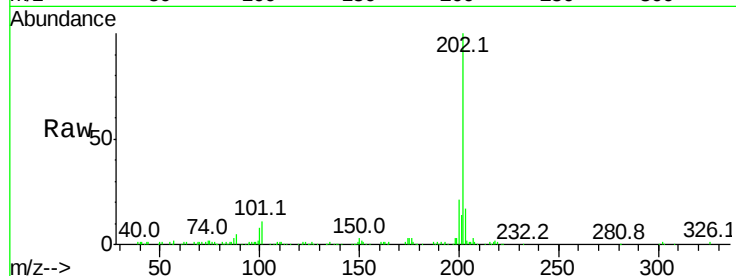

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

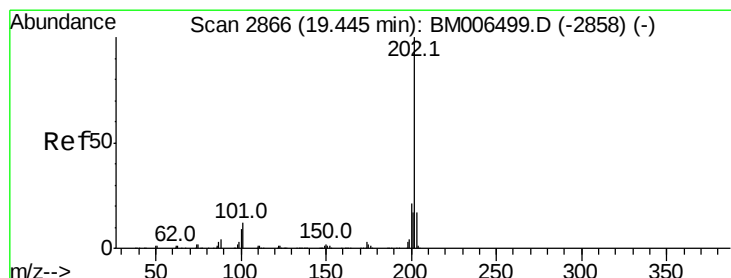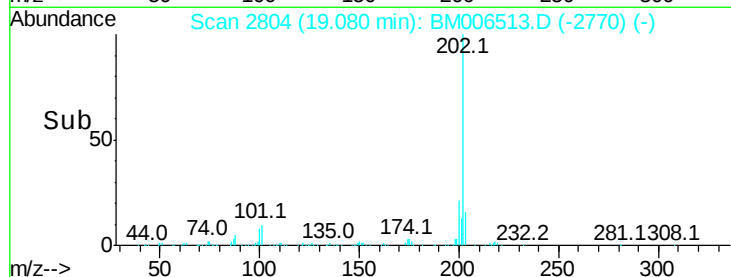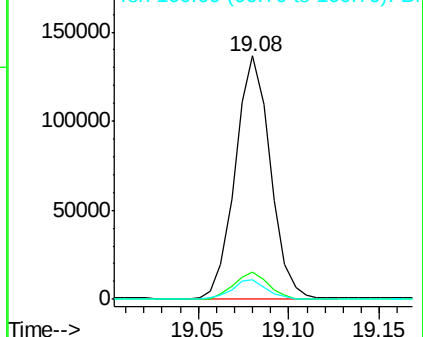

#77

Pyrene

Concen: 2.99 ng/ul

RT: 19.44 min Scan# 2866

Delta R.T. 0.00 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00


Tgt Ion:202 Resp: 178071

Ion Ratio Lower Upper

202 100

101 12.4 10.0 15.0



100 11.2 7.9 11.9

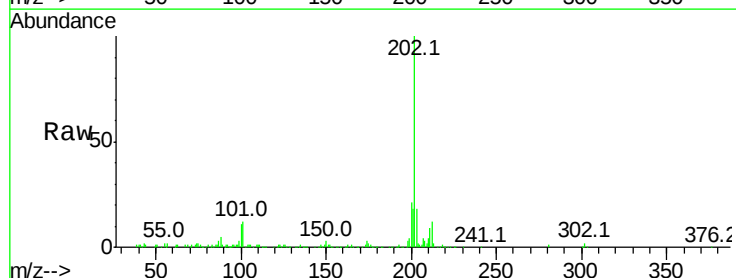


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

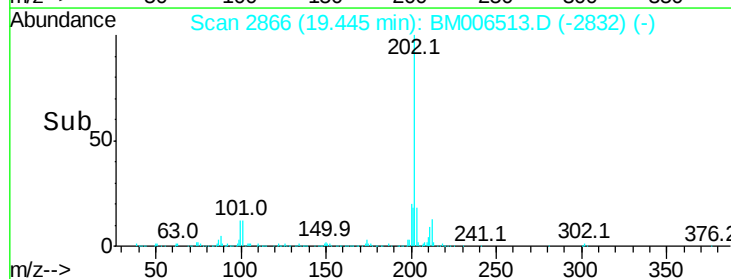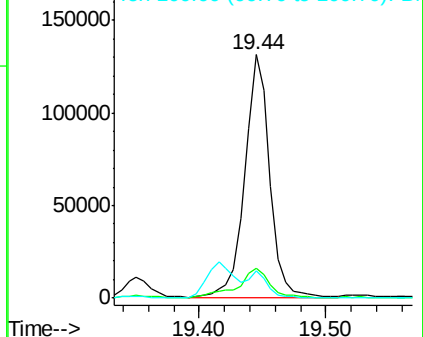

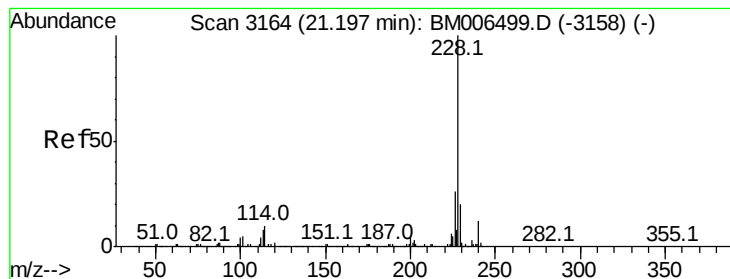

#80

Benzo(a)anthracene

Concen: 2.39 ng/ul

RT: 21.25 min Scan# 3173

Delta R.T. 0.05 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00

Instrument :

BNA_M

ClientSampleId :


Tot Ion:228 Resp: 145651

Ion Ratio Lower Upper

228 100

229 21.9 15.6 23.4




226 32.1 21.4 32.2

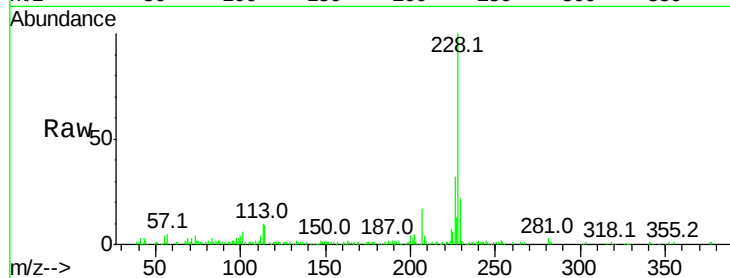

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

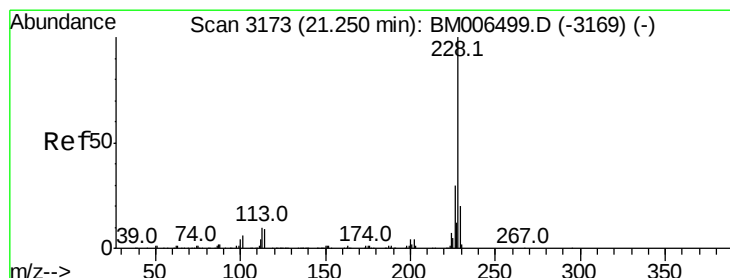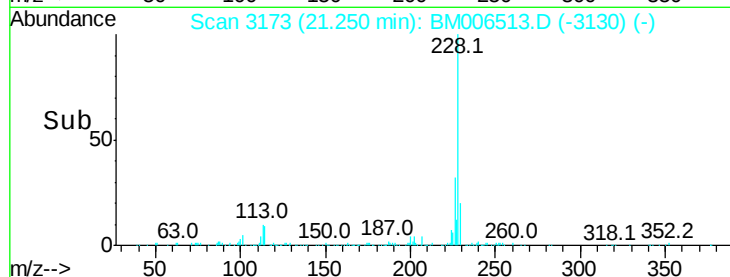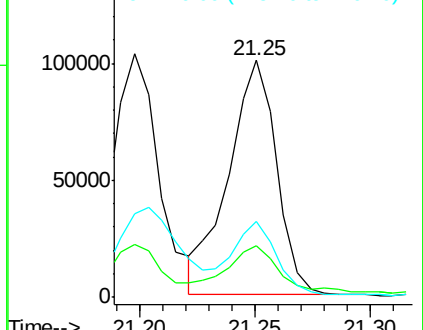

#82

Chrysene

Concen: 2.54 ng/ul

RT: 21.25 min Scan# 3173

Delta R.T. 0.00 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00


Tgt Ion:228 Resp: 145651

Ion Ratio Lower Upper

228 100

226 32.1 23.3 34.9



229 21.9 15.8 23.8

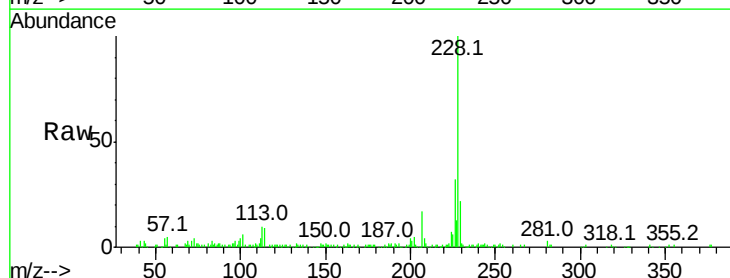


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



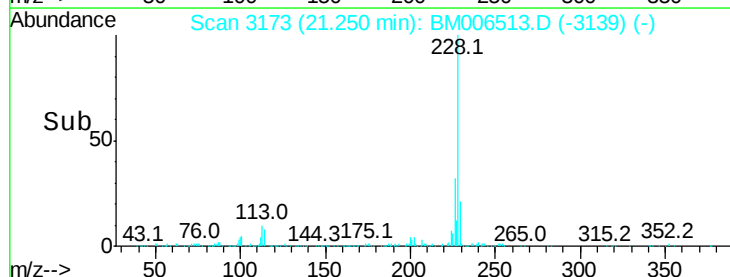
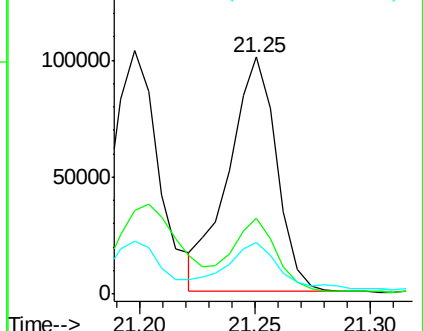


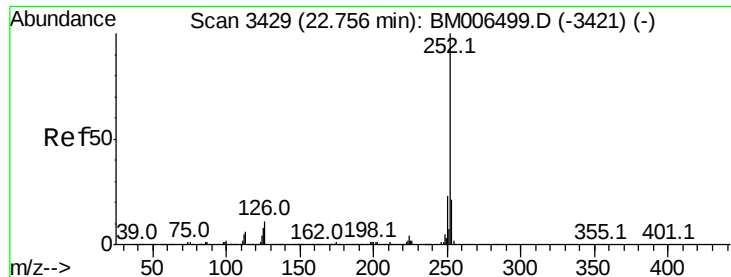

#85
Benzo(b)fluoranthene
Concen: 2.79 ng/ul
RT: 22.76 min Scan# 3429
Delta R.T. 0.00 min
Lab File: BM006513.D
Acq: 17 Jul 2016 13:00




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
252	100		
253	23.6	17.4	26.2
125	10.2	6.7	10.1

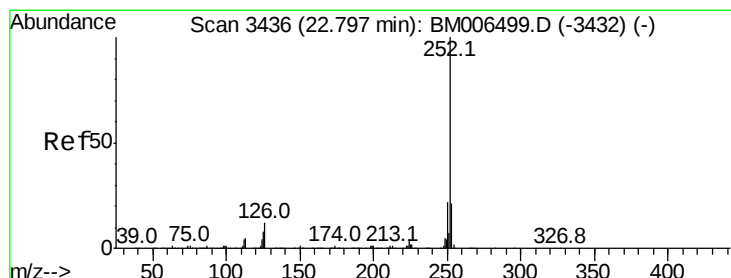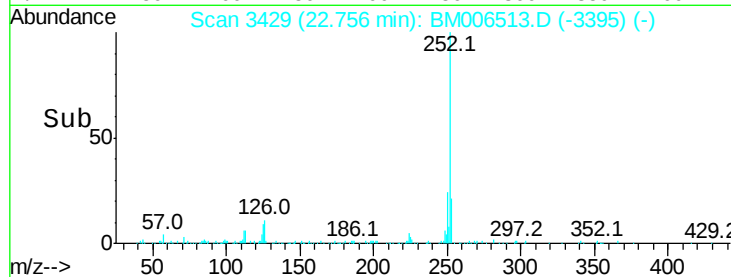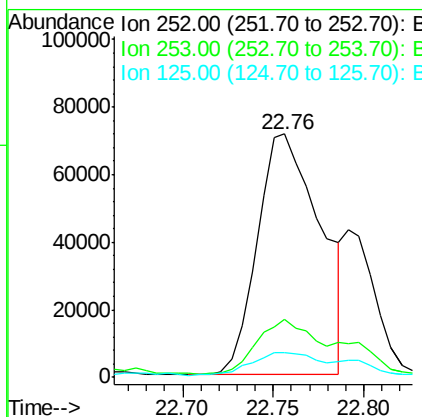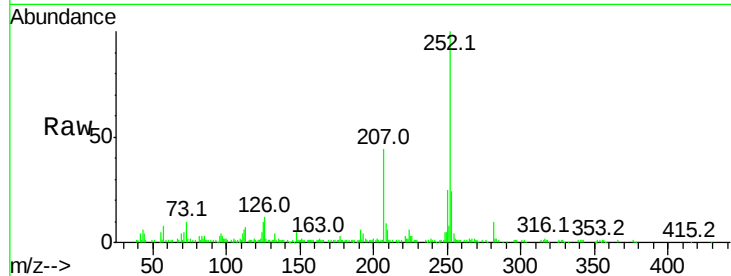

#86
Benzo(k)fluoranthene
Concen: 2.96 ng/ul
RT: 22.76 min Scan# 3429
Delta R.T. -0.04 min
Lab File: BM006513.D
Acq: 17 Jul 2016 13:00

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.6	17.3	25.9
125	10.2	7.0	10.4

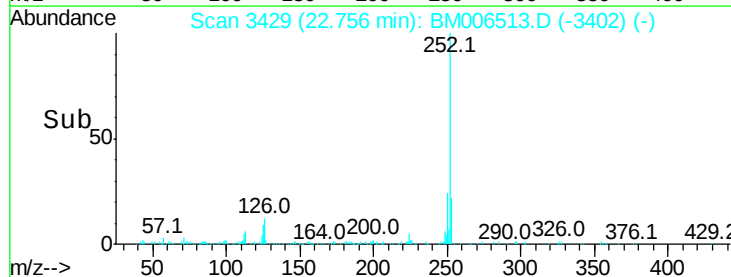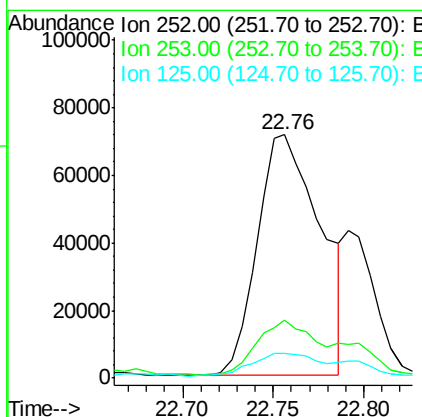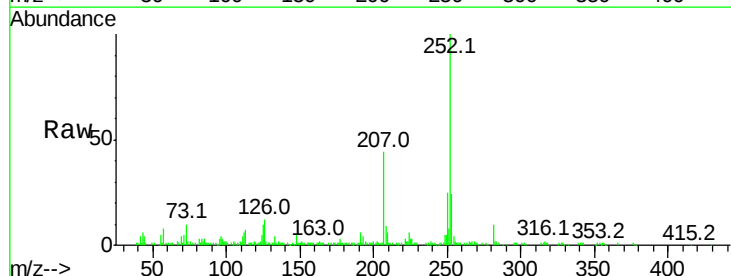

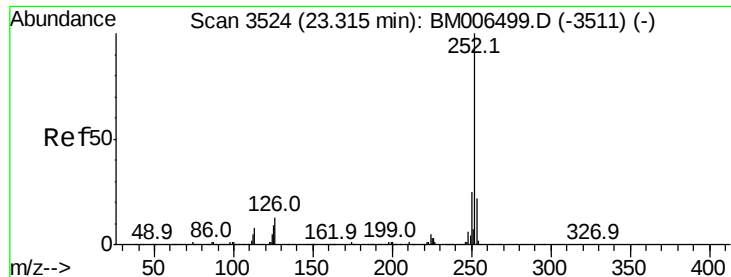

#88

Benzo(a)pyrene

Concen: 2.58 ng/ul

RT: 23.32 min Scan# 3524

Delta R.T. 0.00 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 153338

Ion Ratio Lower Upper

252 100

253 21.8 17.4 26.2




125 10.1 7.6 11.4

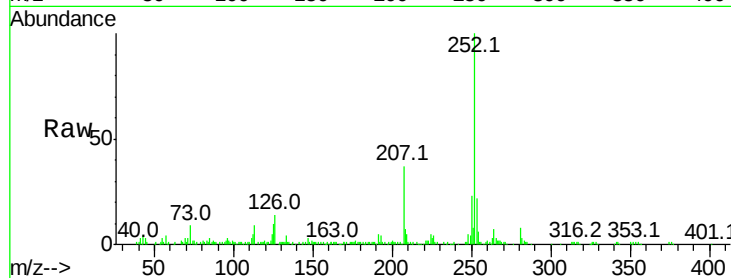

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

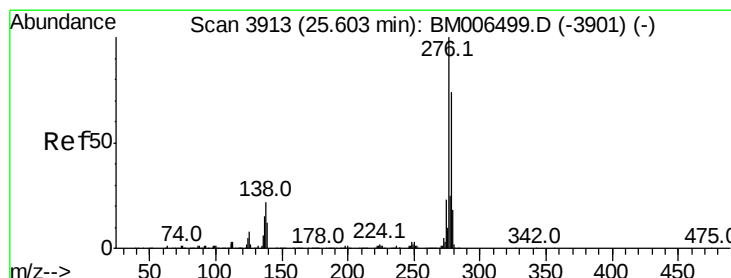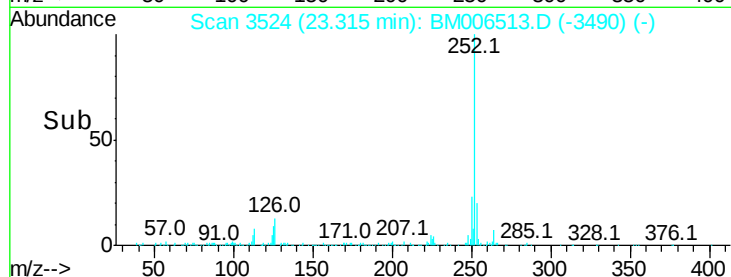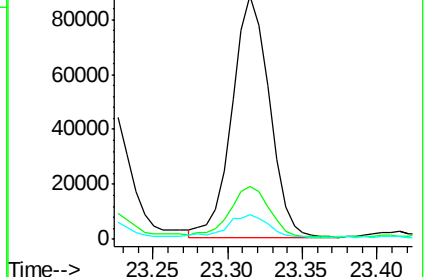

#89

Indeno(1,2,3-cd)pyrene

Concen: 1.26 ng/ul

RT: 25.60 min Scan# 3913

Delta R.T. 0.00 min

Lab File: BM006513.D

Acq: 17 Jul 2016 13:00


Tgt Ion:276 Resp: 86906

Ion Ratio Lower Upper

276 100

138 18.4 17.8 26.6



277 24.6 20.1 30.1

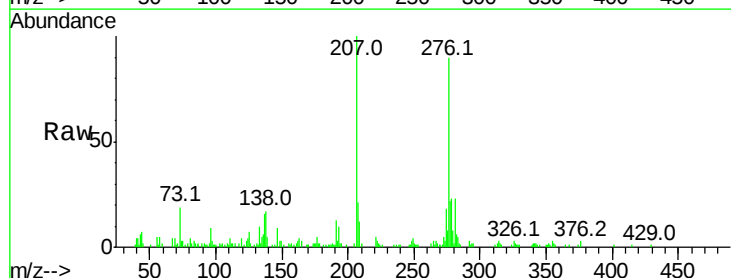


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

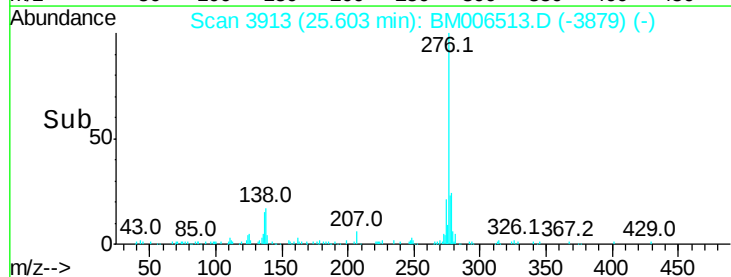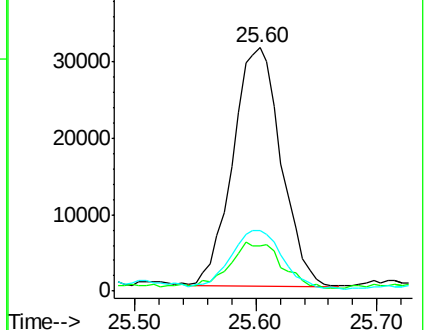


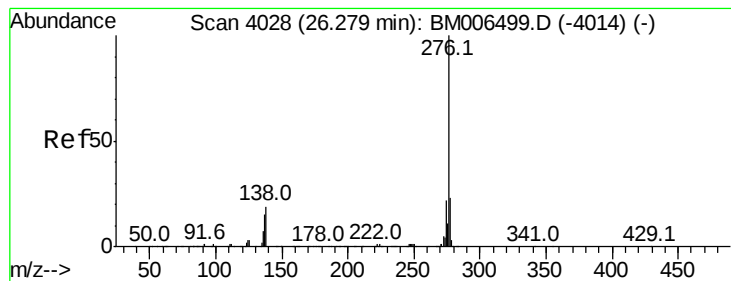

#91
 Benzo(a,h,i)perylene
 Concen: 1.26 ng/ul
 RT: 26.27 min Scan# 4027
 Delta R.T. -0.01 min
 Lab File: BM006513.D
 Acq: 17 Jul 2016 13:00

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
138	18.5	15.0	22.4
277	25.1	19.0	28.4

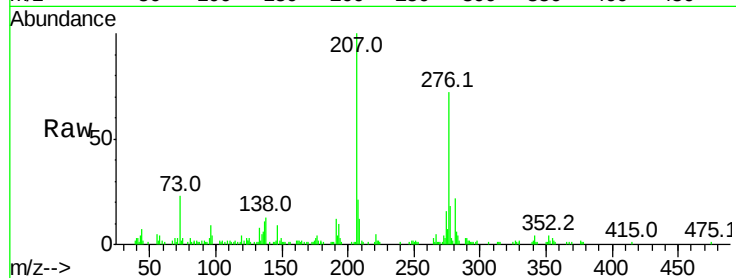

Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

