


Data Path : Z:\HPCHEM1\BNA M\DATA\BM071616\
 Data File : BM006470.D
 Acq On : 16 Jul 2016 09:40
 Operator : UM/SJ
 Sample : DFTPP52
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jul 15 23:20:22 2016

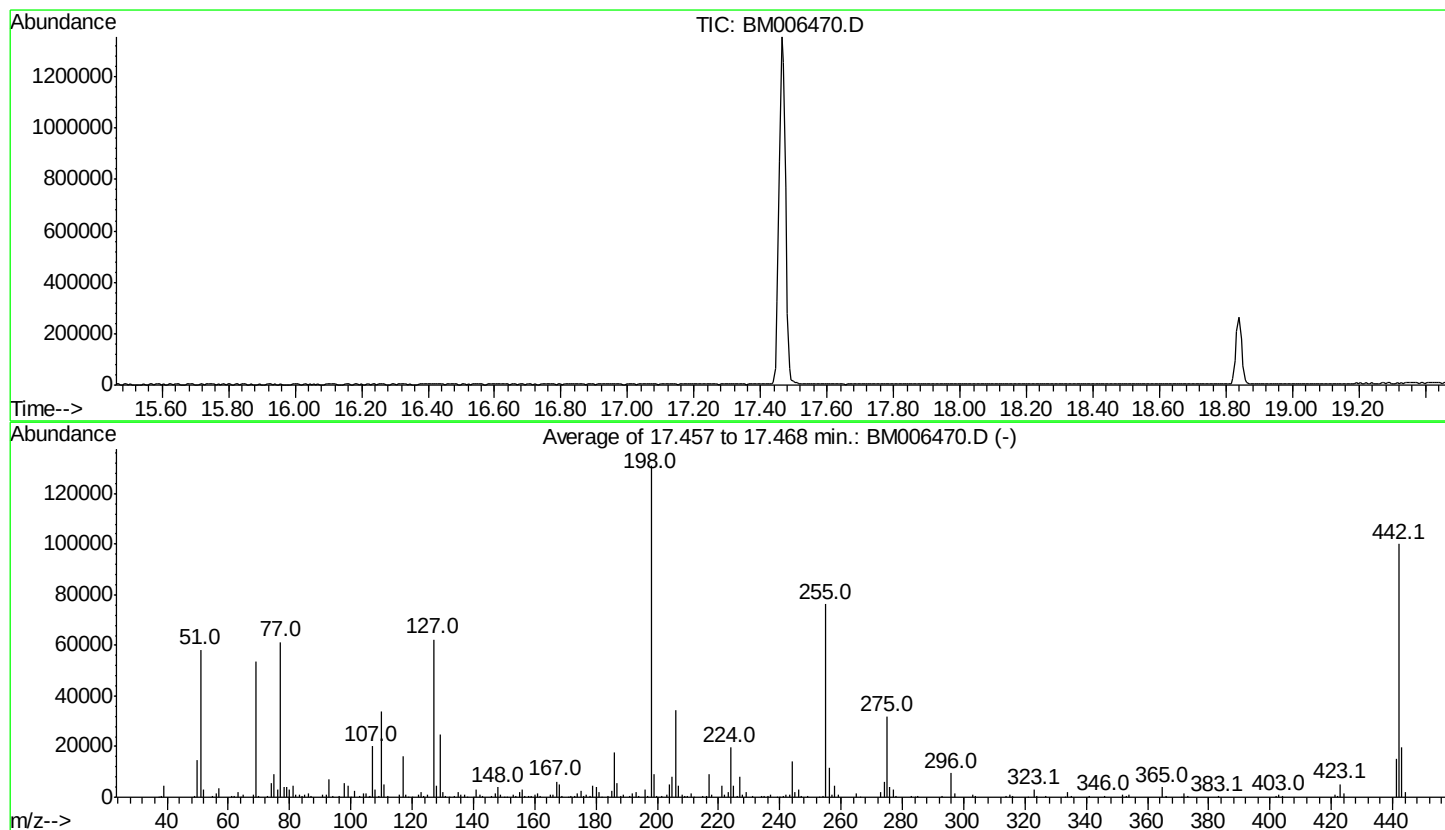

AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	58368	PASS
68	69	0.00	2	1.5	799	PASS
69	198	0.00	100	40.8	53458	PASS
70	69	0.00	2	0.5	276	PASS
127	198	10	80	47.7	62448	PASS
197	198	0.00	2	0.4	542	PASS
198	198	100	100	100.0	131042	PASS
199	198	5	9	7.0	9177	PASS
275	198	10	60	24.3	31845	PASS
365	198	1	100	3.0	3967	PASS
441	443	0.01	100	76.7	15257	PASS
442	198	50	100	76.3	100048	PASS
443	442	15	24	19.9	19892	PASS