

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
 Data File : BM006472.D
 Acq On : 16 Jul 2016 10:52
 Operator : UM/SJ
 Sample : H3959-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ20

Quant Time: Jul 18 06:32:09 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 23:20:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	176996	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	749942	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	414558	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	960514	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1111820	20.00	ng/ul	-0.01
83) Perylene-d12	23.41	264	1184288	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	6509	1.55	ng/uL	0.00
5) Phenol-d5	6.79	99	288557	19.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	182835	20.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	231609	19.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	230114	19.97	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	108663	19.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	121502	18.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	215229	17.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	299706	23.65	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	692541	20.41	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	848450	20.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	110411	18.73	ng/ul	0.00
57) Fluorene-d10	15.26	176	607001	20.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	86385	15.55	ng/ul	0.00
70) Anthracene-d10	17.12	188	973714	21.45	ng/ul	0.00
76) Pyrene-d10	19.42	212	1135909	22.53	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1232776	22.76	ng/ul	-0.01


Target Compounds					Qvalue
44) Dimethylphthalate	13.73	163	672474	19.54 ng/ul	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006472.D
Acq On : 16 Jul 2016 10:52
Operator : UM/SJ
Sample : H3959-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ20

Quant Time: Jul 18 06:32:09 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 23:20:22 2016
Response via : Initial Calibration

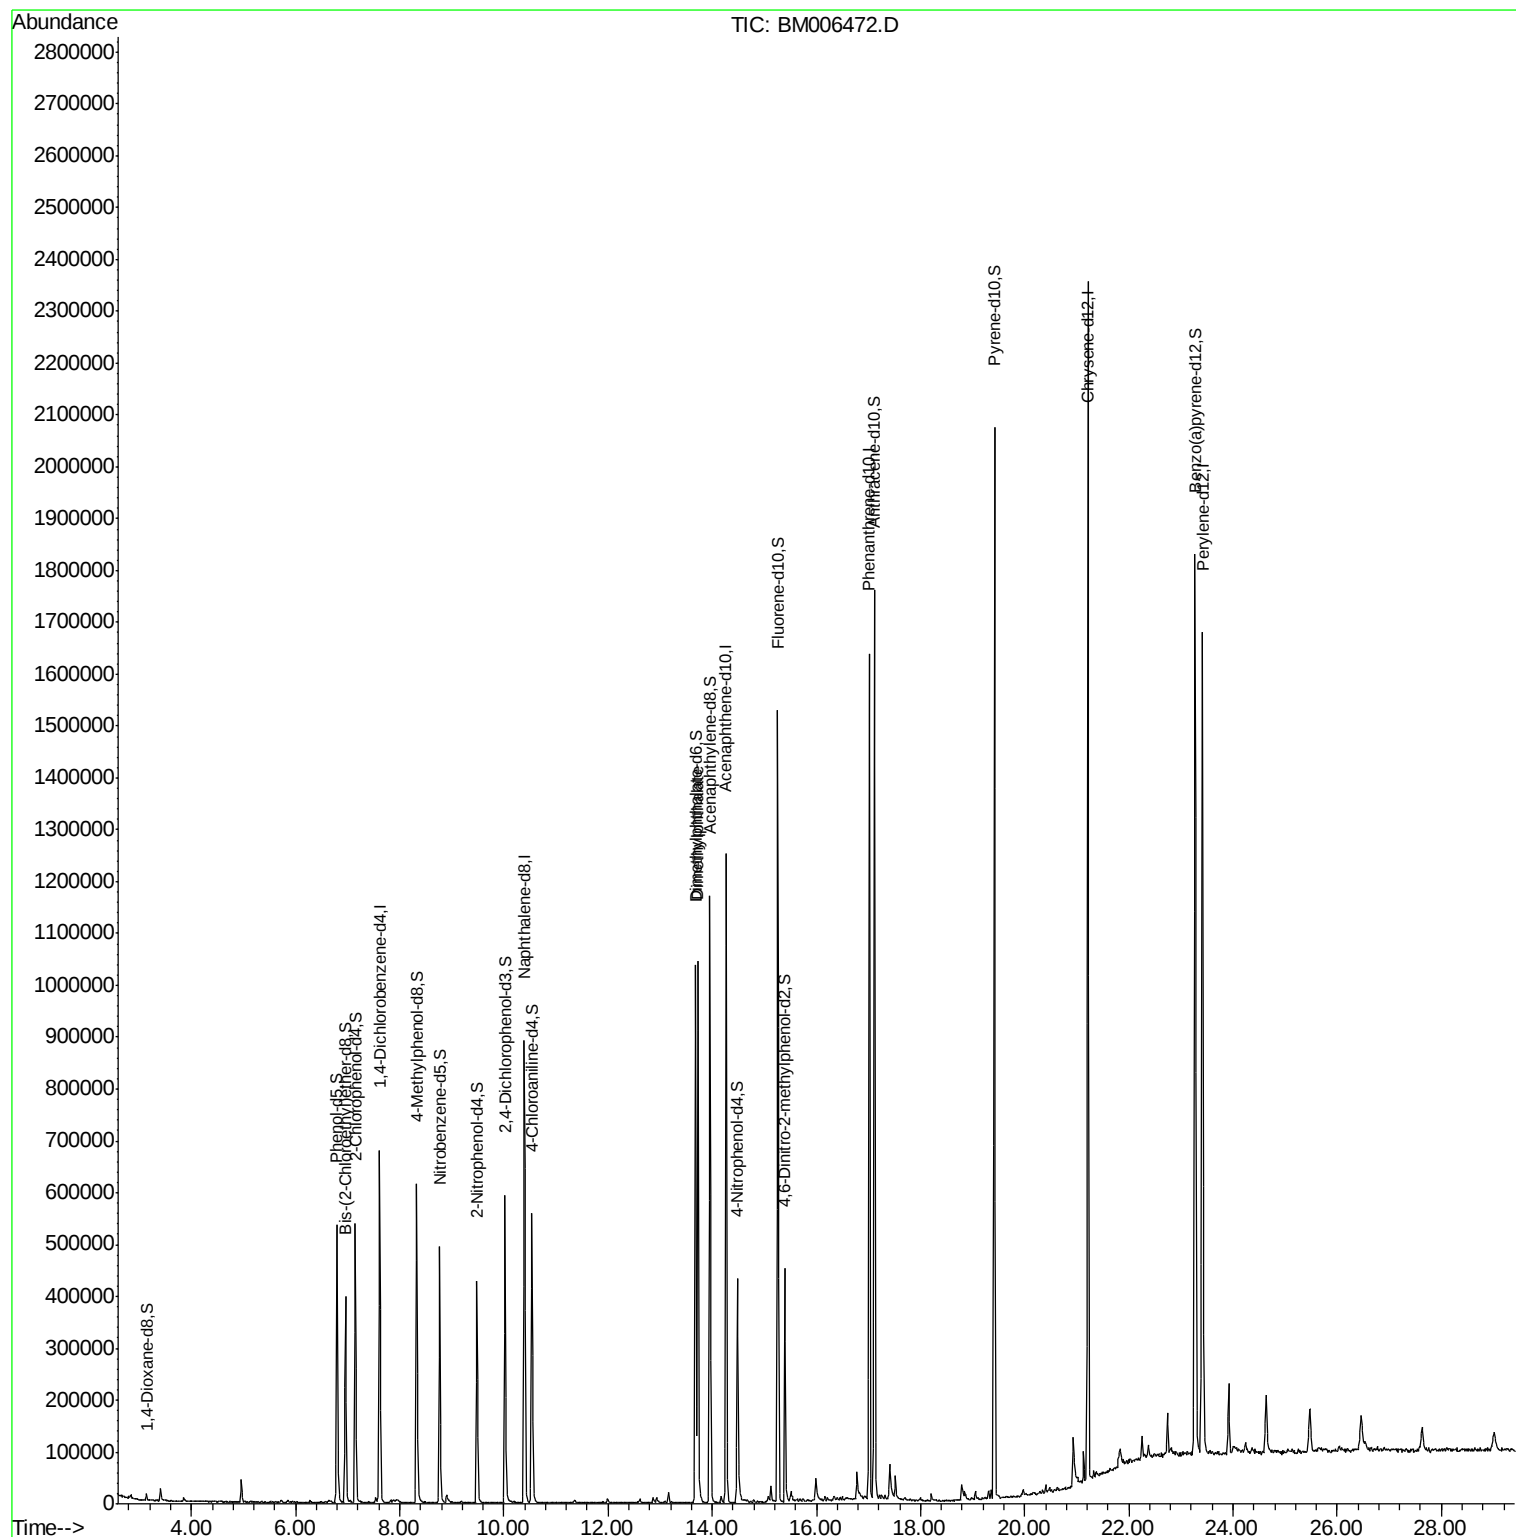

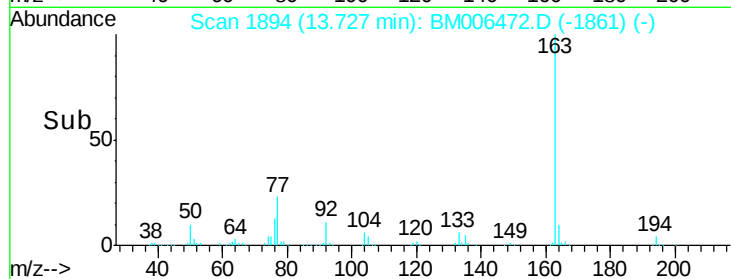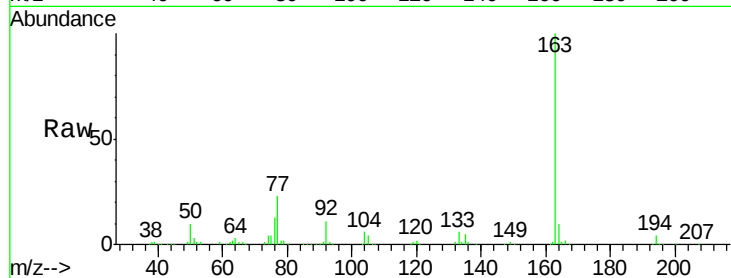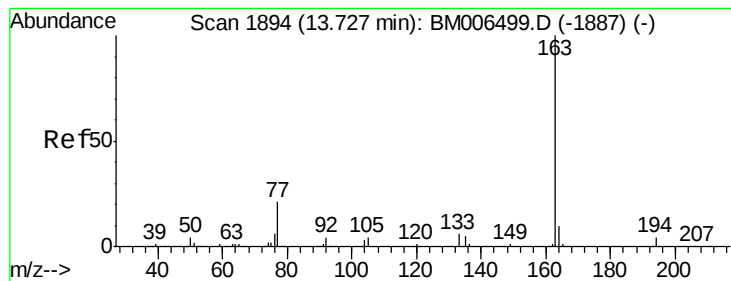

#44

Dimethylphthalate

Concen: 19.54 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BM006472.D

Acq: 16 Jul 2016 10:52

Instrument :

BNA_M

ClientSampleId :

BDJ20

Tgt Ion:163 Resp: 672474

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 9.9 7.8 11.8

