

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
 Data File : BM006495.D
 Acq On : 17 Jul 2016 01:30
 Operator : UM/SJ
 Sample : H3985-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ49

Quant Time: Jul 18 07:29:54 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 23:20:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	221285	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	896629	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	493704	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	1092905	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1307884	20.00	ng/ul	-0.01
83) Perylene-d12	23.41	264	1424724	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	13260	2.52	ng/uL	0.00
5) Phenol-d5	6.79	99	605591	33.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	378574	34.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	474692	32.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	474662	32.94	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	231835	34.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	256231	33.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	442844	30.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	594118	39.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	1346279	33.32	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1674875	33.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	240071	34.20	ng/ul	0.00
57) Fluorene-d10	15.26	176	1152764	32.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	162032	25.63	ng/ul	0.00
70) Anthracene-d10	17.12	188	1764039	34.15	ng/ul	0.00
76) Pyrene-d10	19.42	212	2037439	34.36	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	2272471	34.88	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.73	163	965043	23.54	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006495.D
Acq On : 17 Jul 2016 01:30
Operator : UM/SJ
Sample : H3985-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ49

Quant Time: Jul 18 07:29:54 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 23:20:22 2016
Response via : Initial Calibration

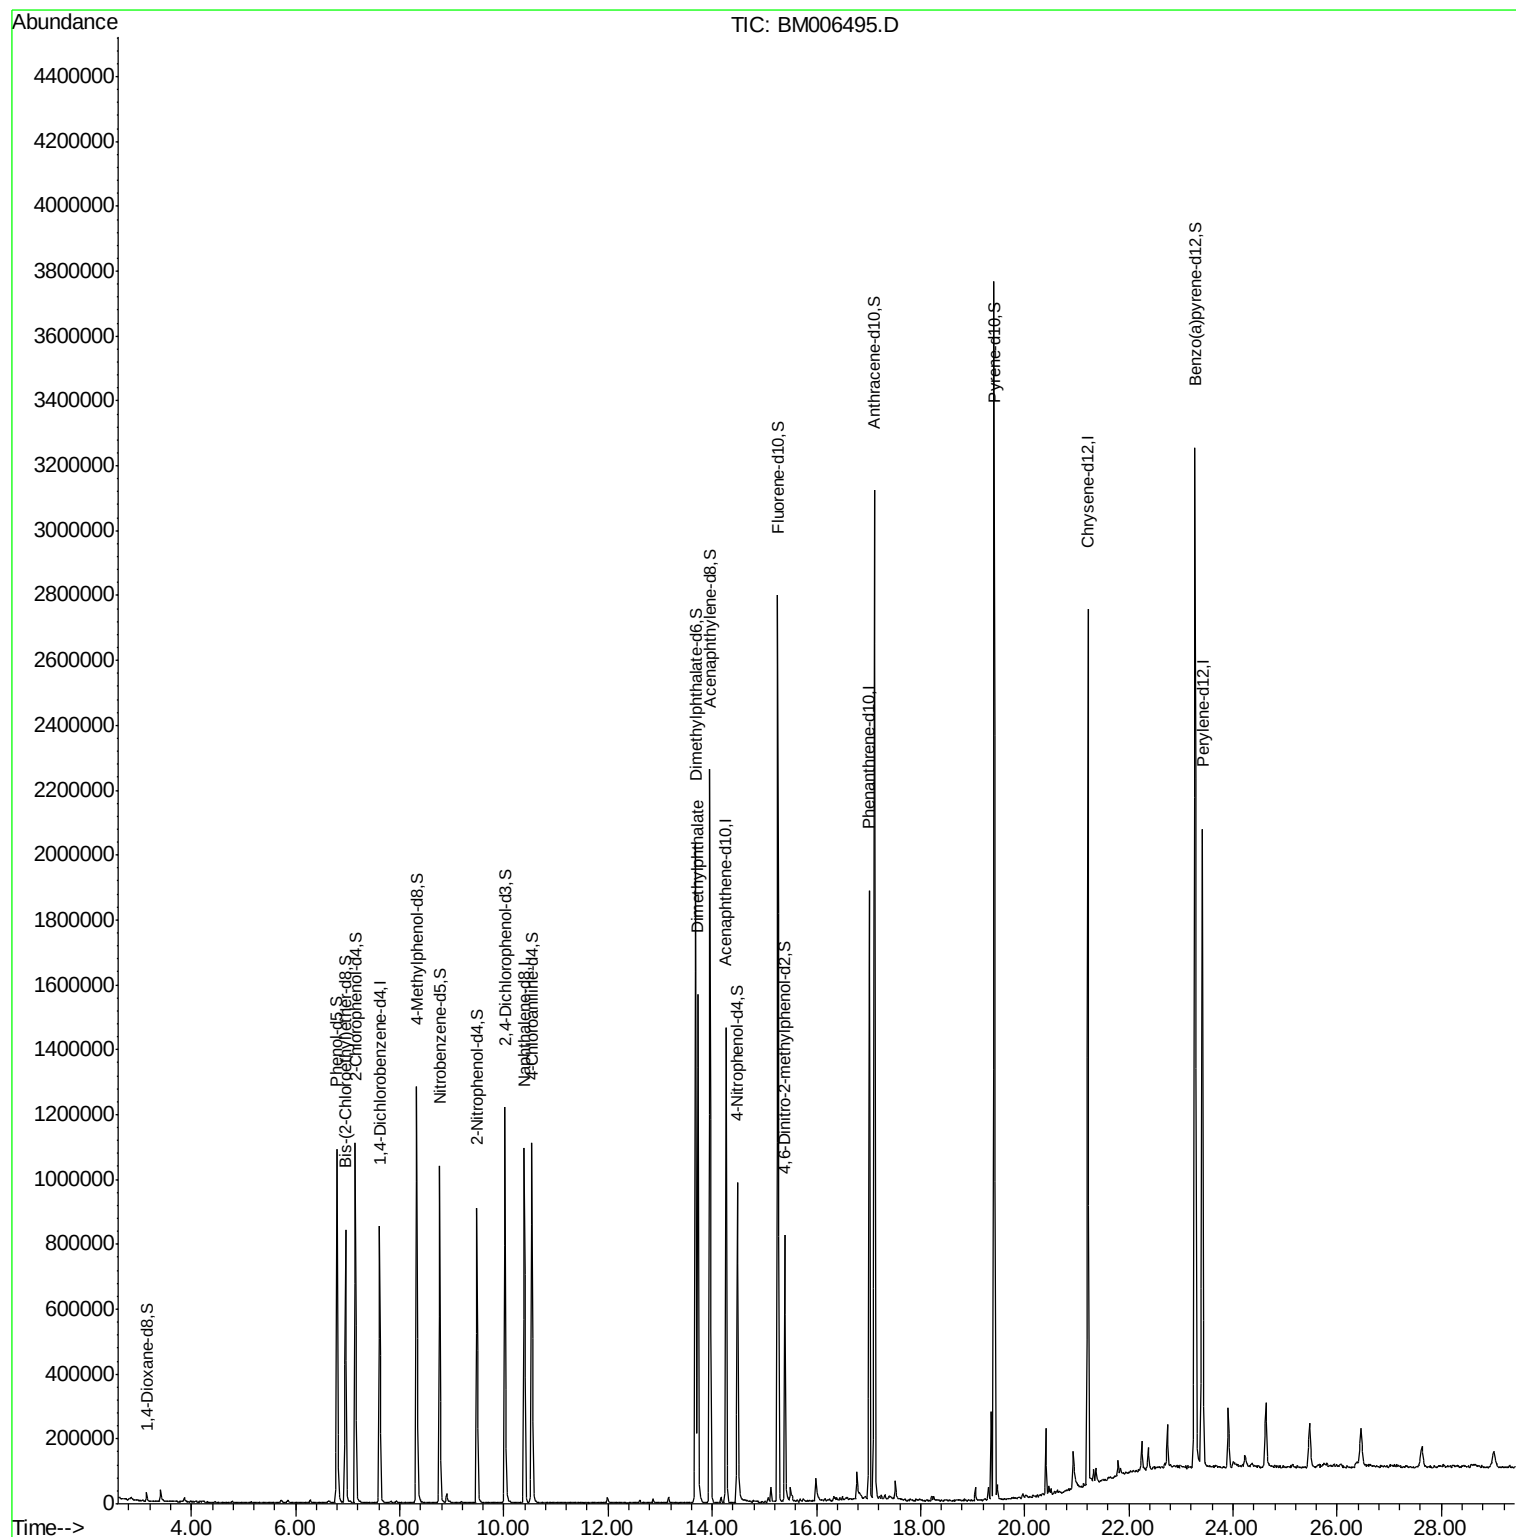

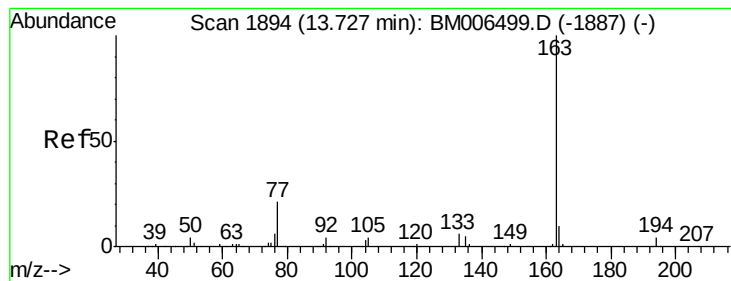

#44

Dimethylphthalate

Concen: 23.54 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BM006495.D


Acq: 17 Jul 2016 01:30

Instrument :

BNA_M

ClientSampleId :

BDJ49

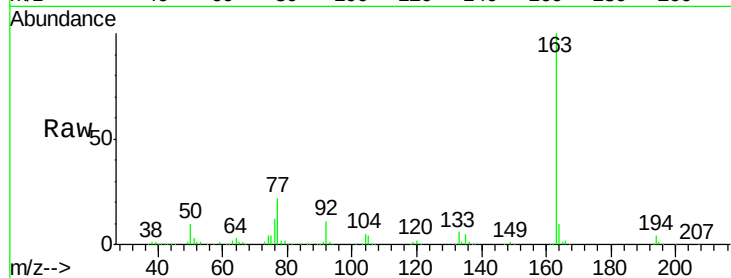


Tgt Ion:163 Resp: 965043

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.2 7.8 11.8

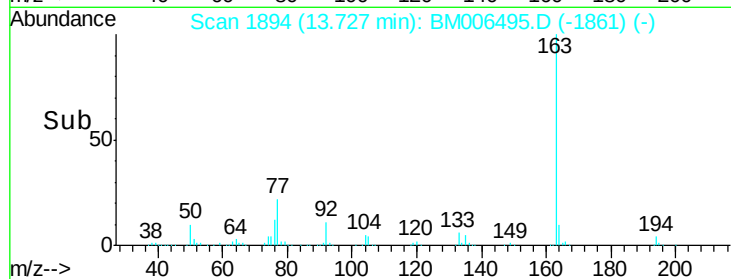

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

