

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
 Data File : BM006497.D
 Acq On : 17 Jul 2016 02:42
 Operator : UM/SJ
 Sample : H3985-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ55

Quant Time: Jul 18 06:20:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 15 23:20:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	216259	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	868468	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	471399	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.02	188	1068690	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1319477	20.00	ng/ul	-0.01
83) Perylene-d12	23.41	264	1431172	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	9658	1.88	ng/uL	0.00
5) Phenol-d5	6.79	99	416248	23.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	263679	24.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	325477	22.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	329735	23.42	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	155201	23.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	169065	22.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	297902	21.22	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	389138	26.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	959444	24.87	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1163627	24.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	155764	23.24	ng/ul	0.00
57) Fluorene-d10	15.26	176	822018	23.97	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	118443	19.16	ng/ul	0.00
70) Anthracene-d10	17.12	188	1307326	25.88	ng/ul	0.00
76) Pyrene-d10	19.42	212	1568240	26.21	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1809983	27.66	ng/ul	-0.01


Target Compounds					Qvalue
44) Dimethylphthalate	13.73	163	966598	24.70 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006497.D
Acq On : 17 Jul 2016 02:42
Operator : UM/SJ
Sample : H3985-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ55

Quant Time: Jul 18 06:20:11 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 15 23:20:22 2016
Response via : Initial Calibration

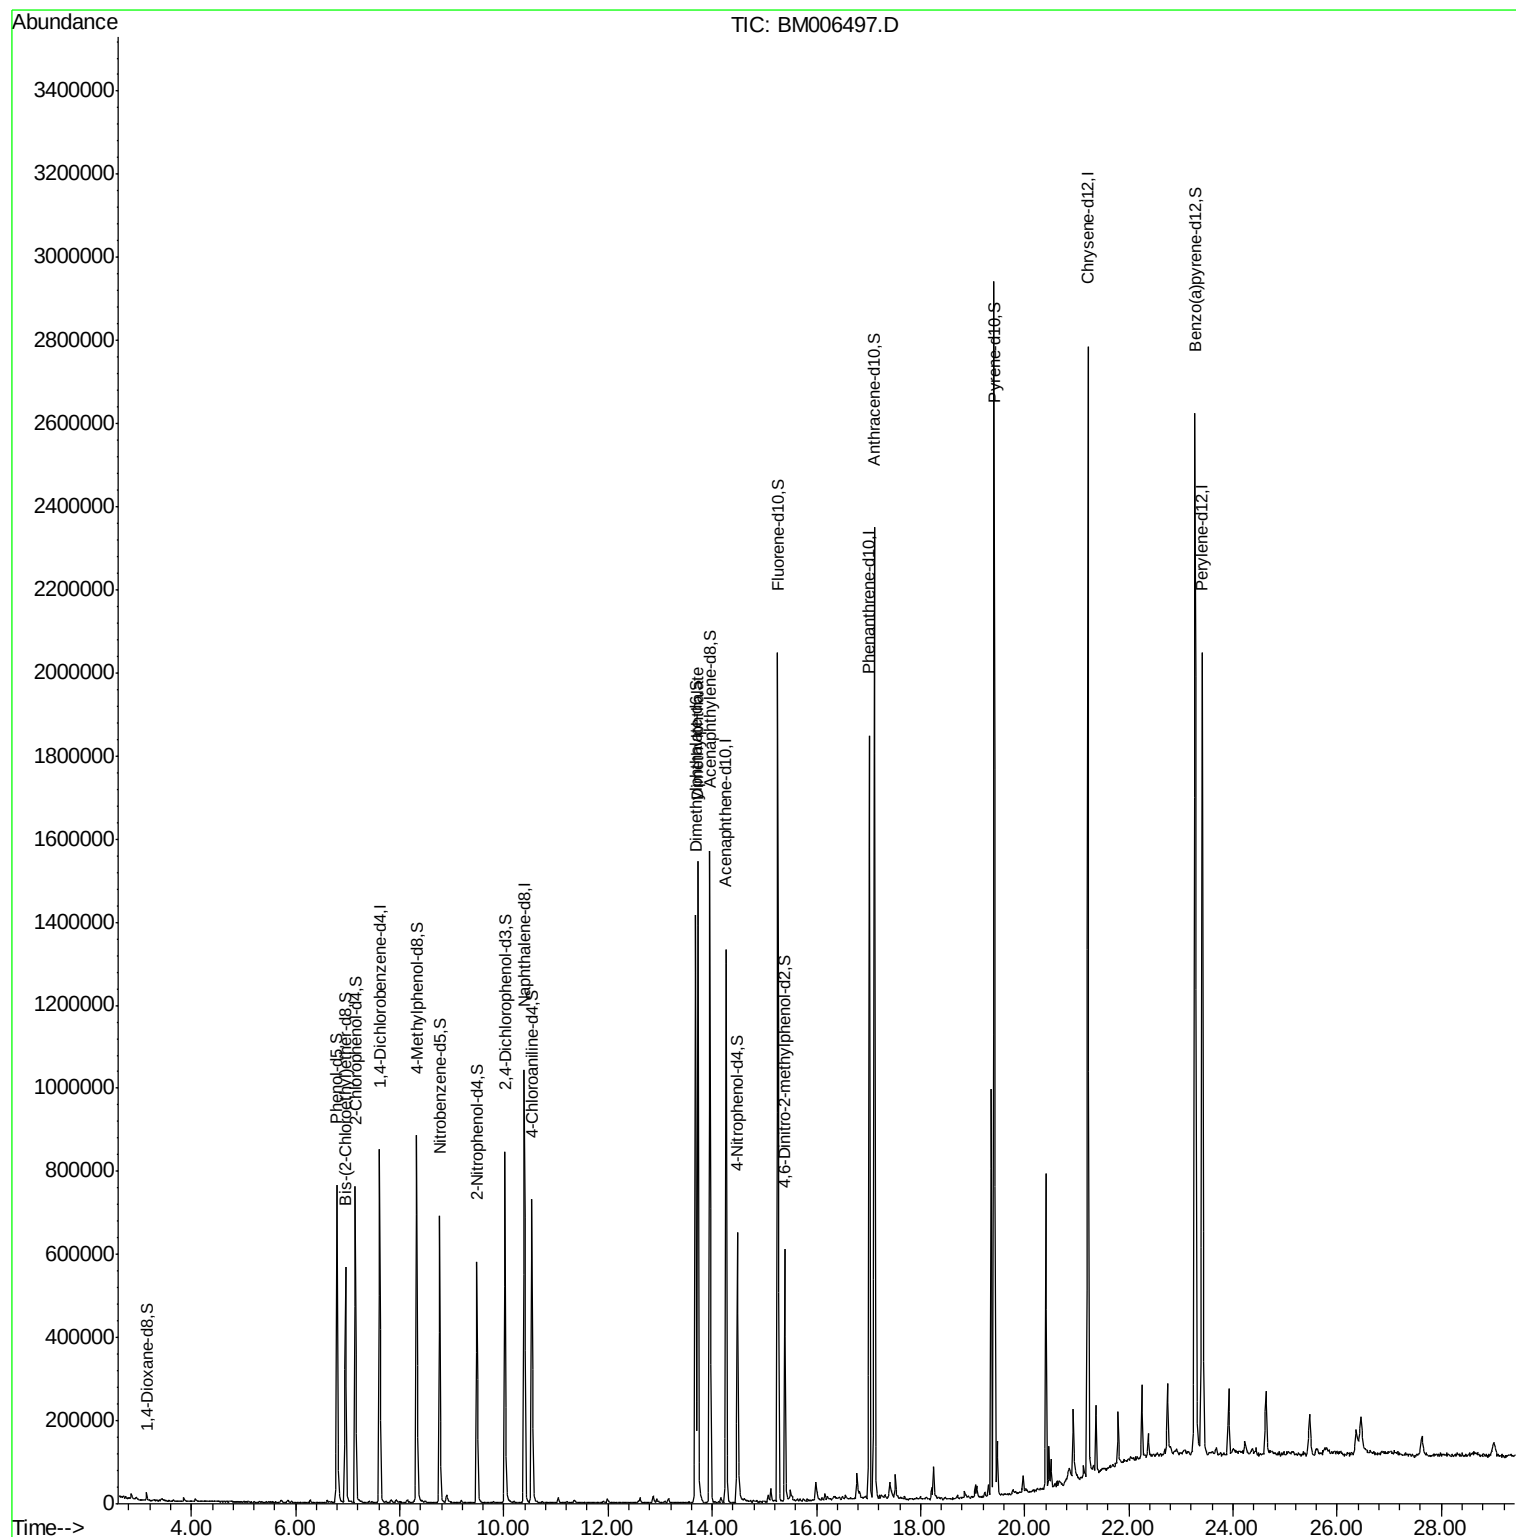

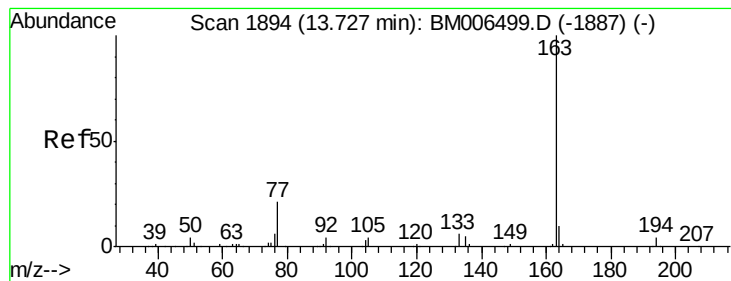

#44

Dimethylphthalate

Concen: 24.70 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BM006497.D


Acq: 17 Jul 2016 02:42

Instrument :

BNA_M

ClientSampleId :

BDJ55

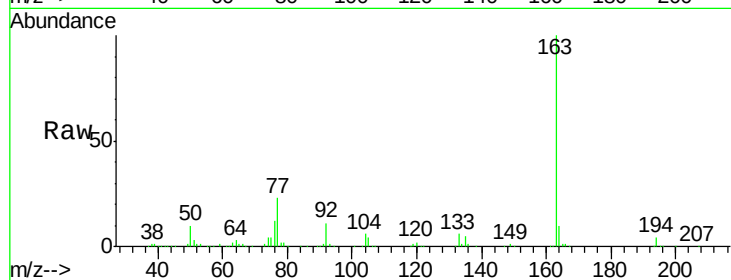

Tgt Ion:163 Resp: 966598

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.0 7.8 11.8

