

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
 Data File : BM006502.D
 Acq On : 17 Jul 2016 06:20
 Operator : UM/SJ
 Sample : H3985-19
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ56

Quant Time: Jul 18 07:42:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 18 07:39:41 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	251682	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1034290	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	574384	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	1295363	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1553775	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1672464	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	8687	1.45	ng/uL	0.00
5) Phenol-d5	6.79	99	382815	18.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	243855	19.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	304013	18.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	304644	18.59	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	143733	18.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	156708	17.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	281442	16.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	387772	22.18	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	926891	19.72	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1115106	19.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	124796	15.28	ng/ul	0.00
57) Fluorene-d10	15.26	176	795317	19.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	101296	13.52	ng/ul	0.00
70) Anthracene-d10	17.12	188	1251121	20.43	ng/ul	0.00
76) Pyrene-d10	19.42	212	1465711	20.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1592666	20.82	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.73	163	366087	7.68	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006502.D
Acq On : 17 Jul 2016 06:20
Operator : UM/SJ
Sample : H3985-19
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ56

Quant Time: Jul 18 07:42:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 18 07:39:41 2016
Response via : Initial Calibration

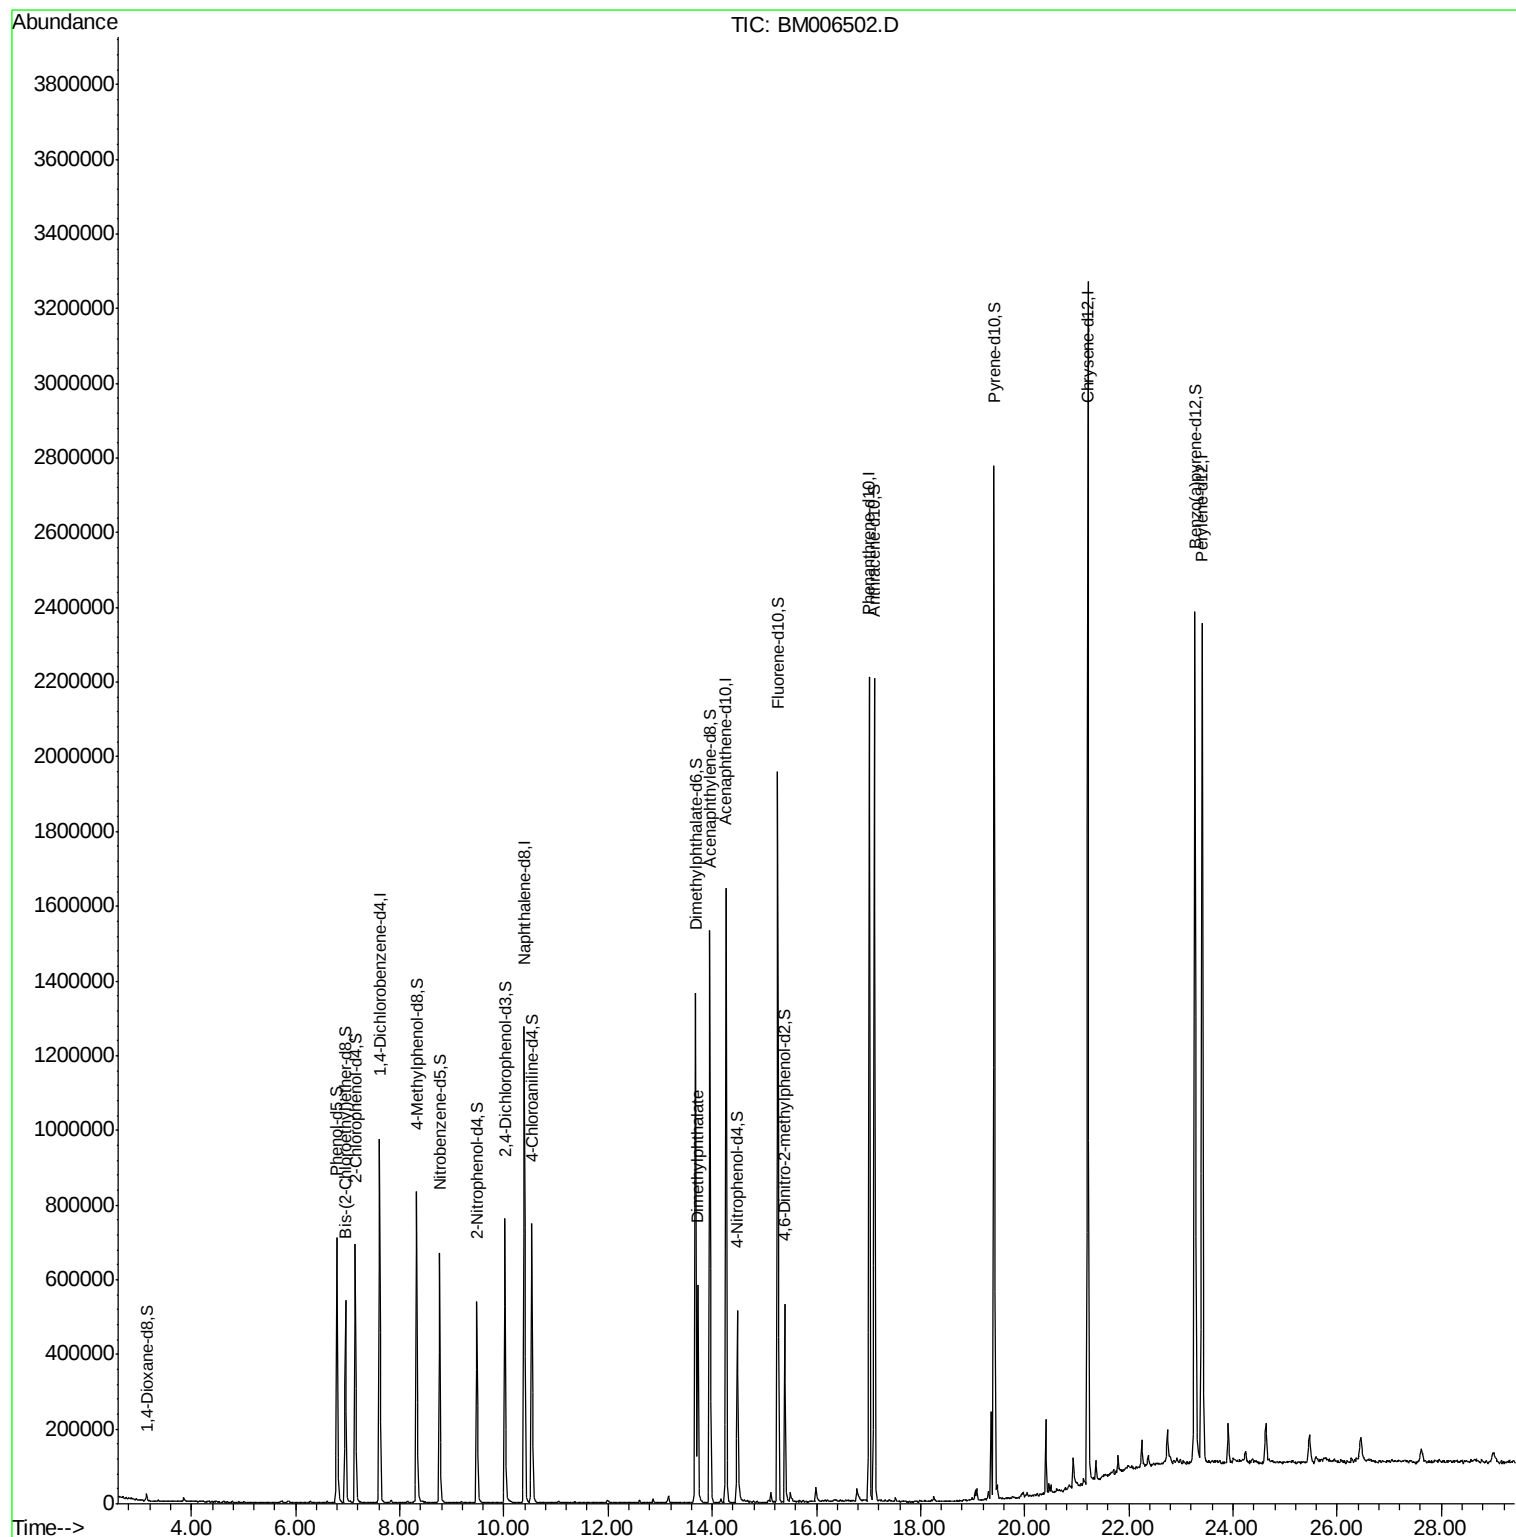

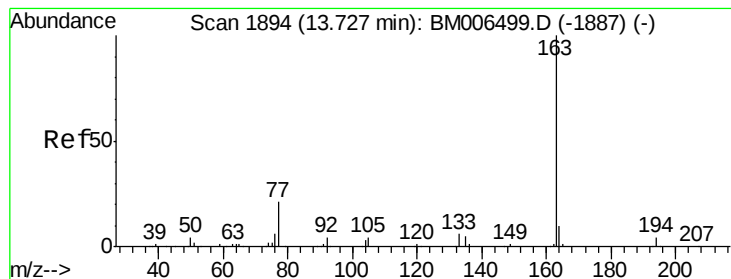

#44

Dimethylphthalate

Concen: 7.68 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. 0.00 min

Lab File: BM006502.D

Acq: 17 Jul 2016 06:20

Instrument :

BNA_M

ClientSampleId :

BDJ56



Tgt Ion:163 Resp: 366087

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 10.2 7.8 11.8

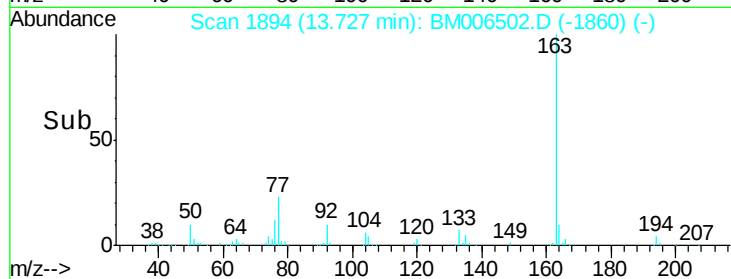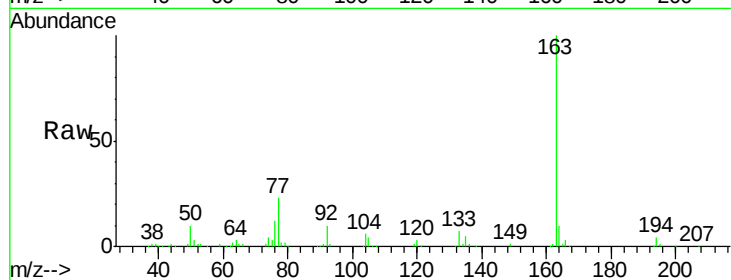

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

