

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
 Data File : BM006509.D
 Acq On : 17 Jul 2016 10:34
 Operator : UM/SJ
 Sample : H3959-20
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ37

Manual Integrations

sohil
 7/18/2016 7:40:14 PM

Quant Time: Jul 18 08:36:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 18 07:39:41 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	172310	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	742533	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	415714	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	958455	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1012645	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1149835	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	7230	1.77	ng/uL	0.00
5) Phenol-d5	6.79	99	319161	22.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	205925	24.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	258318	22.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	259759	23.15	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	126741	22.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	138202	21.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	242095	20.17	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	298006	23.75	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	775791	22.80	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	972073	23.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	97819	16.55	ng/ul	0.00
57) Fluorene-d10	15.26	176	687411	22.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	65286	11.77	ng/ul	0.00
70) Anthracene-d10	17.12	188	1063797	23.48	ng/ul	0.00
76) Pyrene-d10	19.42	212	1167459	25.43	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1252672	23.82	ng/ul	0.00

Target Compounds

					Qvalue
28) Naphthalene	10.45	128	41875	1.11 ng/ul	98
44) Dimethylphthalate	13.73	163	326843	9.47 ng/ul	99
47) Acenaphthylene	13.99	152	183543	4.19 ng/ul	99
49) Acenaphthene	14.33	153	52300	1.86 ng/ul	95
58) Fluorene	15.32	166	54518	1.66 ng/ul	96
69) Phenanthrene	17.06	178	692480	13.14 ng/ul	100
71) Anthracene	17.15	178	474688	8.76 ng/ul	100
74) Fluoranthene	19.08	202	2596119	42.39 ng/ul	98
77) Pyrene	19.44	202	2189969	36.22 ng/ul	99
80) Benzo(a)anthracene	21.20	228	1572329	25.44 ng/ul	96
82) Chrysene	21.25	228	1364672	23.45 ng/ul	98
85) Benzo(b)fluoranthene	22.76	252	1827019	26.59 ng/ul	98
86) Benzo(k)fluoranthene	22.80	252	616065m	9.53 ng/ul	
88) Benzo(a)pyrene	23.32	252	1397057	21.22 ng/ul	98
89) Indeno(1,2,3-cd)pyrene	25.60	276	818123	10.68 ng/ul	96
90) Dibenzo(a,h)anthracene	25.61	278	224359	3.52 ng/ul#	94
91) Benzo(g,h,i)perylene	26.28	276	630266	9.31 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006509.D
Acq On : 17 Jul 2016 10:34
Operator : UM/SJ
Sample : H3959-20
Misc :
ALS Vial : 37 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BDJ37

Manual Integrations

Quant Time: Jul 18 08:36:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 18 07:39:41 2016
Response via : Initial Calibration

sohil
7/18/2016 7:40:14 PM

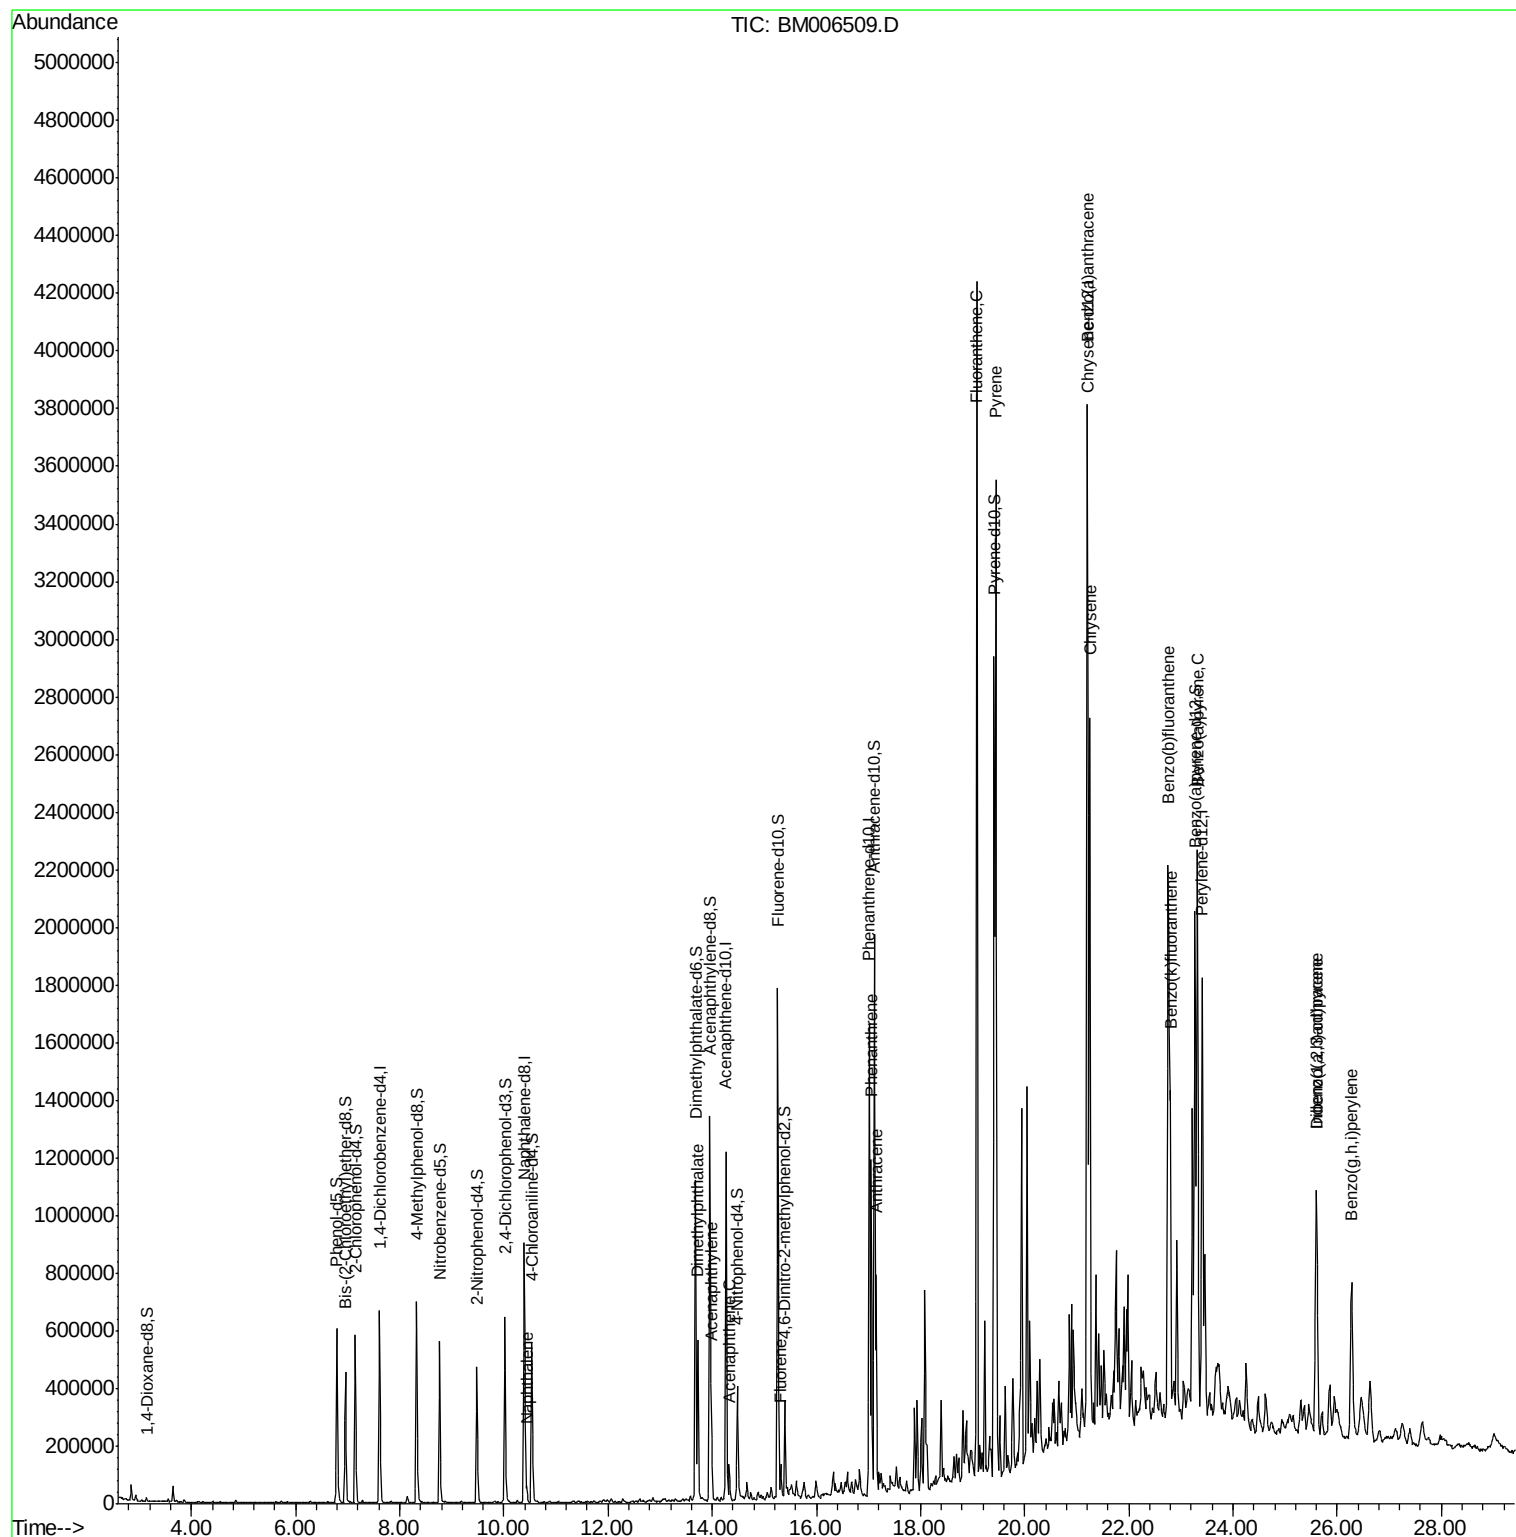

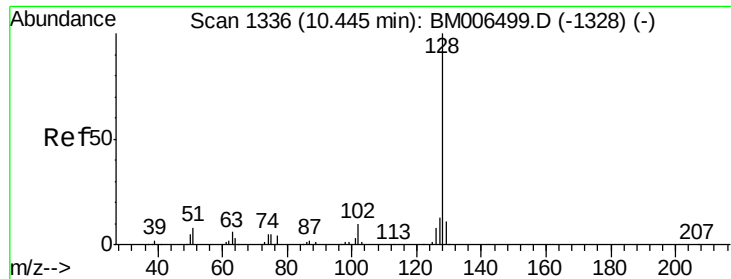





#28
Naphthalene
Concen: 1.11 ng/ul
RT: 10.45 min Scan# 1336
Delta R.T. 0.00 min
Lab File: BM006509.D
Acq: 17 Jul 2016 10:34

Instrument :
BNA_M
ClientSampleId :
BDJ37

Tgt Ion	Ratio	Lower	Upper
128	100		
129	9.4	8.6	13.0
127	13.3	10.9	16.3




Manual Integrations


sohil
7/18/2016 7:40:14 PM

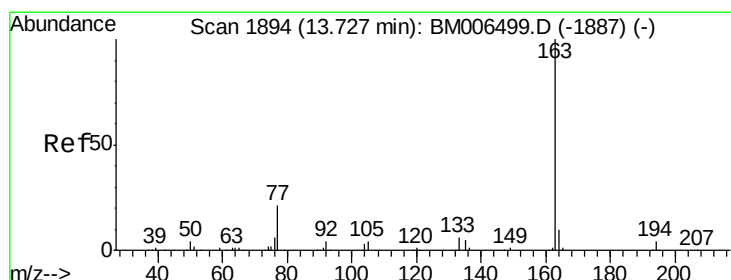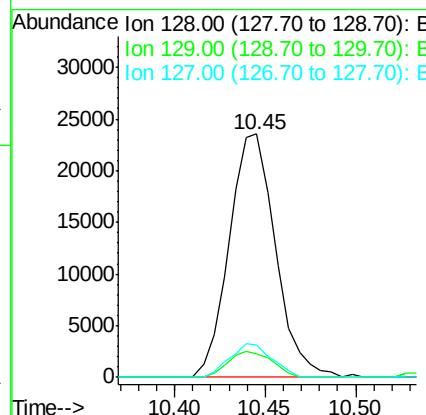

#44
Dimethylphthalate
Concen: 9.47 ng/ul
RT: 13.73 min Scan# 1894
Delta R.T. 0.00 min
Lab File: BM006509.D
Acq: 17 Jul 2016 10:34

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.4	5.0
164	10.2	7.8	11.8

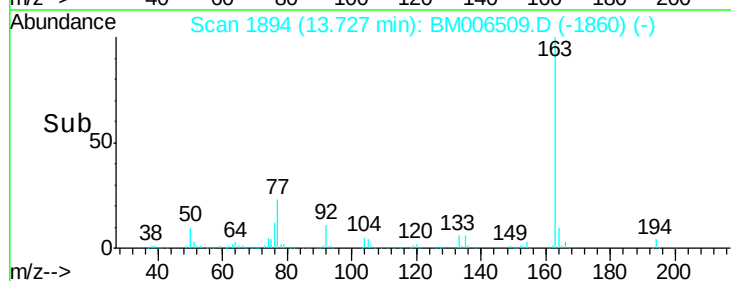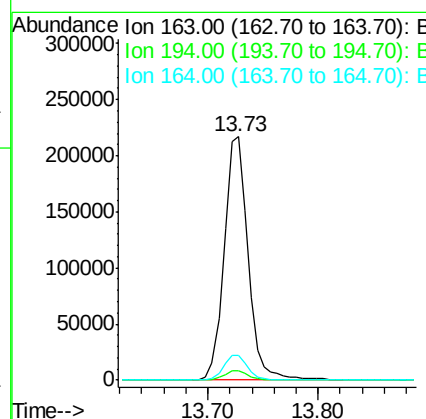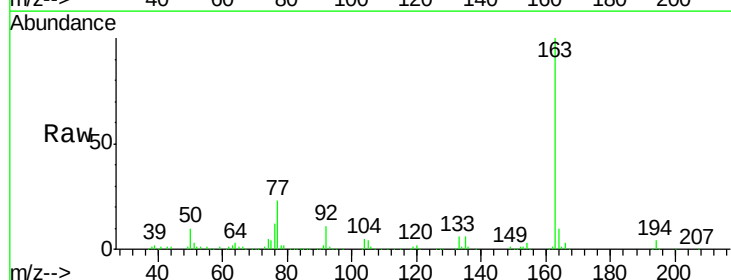

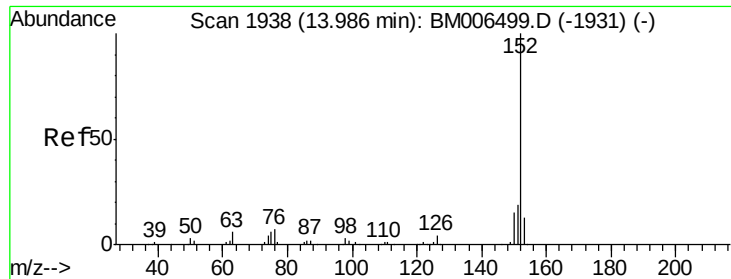





#47
Acenaphthylene
Concen: 4.19 ng/ul
RT: 13.99 min Scan# 1938
Delta R.T. 0.00 min
Lab File: BM006509.D
Acq: 17 Jul 2016 10:34

Instrument :
BNA_M
ClientSampleId :
BDJ37

Tgt Ion:	152	Resp:	183543
Ion Ratio	Lower	Upper	
152	100		
151	18.9	15.6	23.4
153	13.6	10.3	15.5




Manual Integrations


sohil
7/18/2016 7:40:14 PM

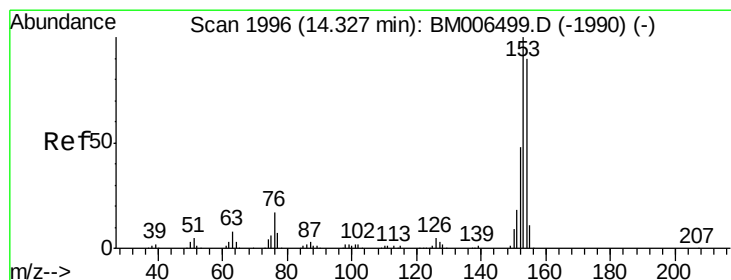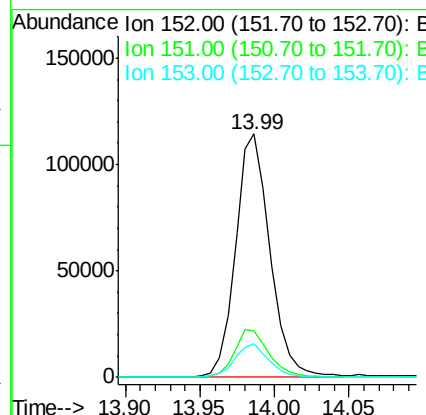

#49
Acenaphthene
Concen: 1.86 ng/ul
RT: 14.33 min Scan# 1997
Delta R.T. 0.01 min
Lab File: BM006509.D
Acq: 17 Jul 2016 10:34

Tgt Ion:	153	Resp:	52300
Ion Ratio	Lower	Upper	
153	100		
152	44.5	37.7	56.5
154	82.0	70.0	105.0

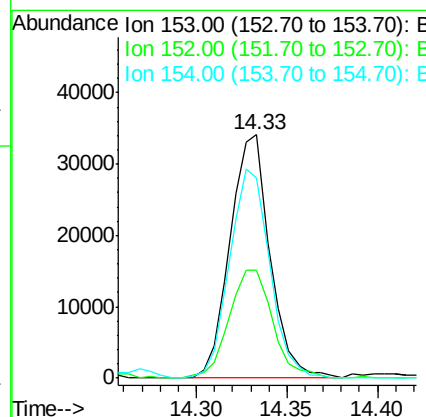

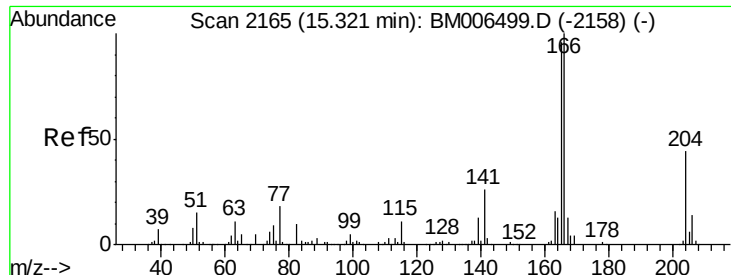





#58
 Fluorene
 Concen: 1.66 ng/ul
 RT: 15.32 min Scan# 2164
 Delta R.T. -0.01 min
 Lab File: BM006509.D
 Acq: 17 Jul 2016 10:34

Instrument :
 BNA_M
 ClientSampleId :
 BDJ37

Tgt Ion:166 Resp: 54518
 Ion Ratio Lower Upper
 166 100
 165 92.2 77.5 116.3
 167 14.1 10.8 16.2




Manual Integrations


sohil
 7/18/2016 7:40:14 PM

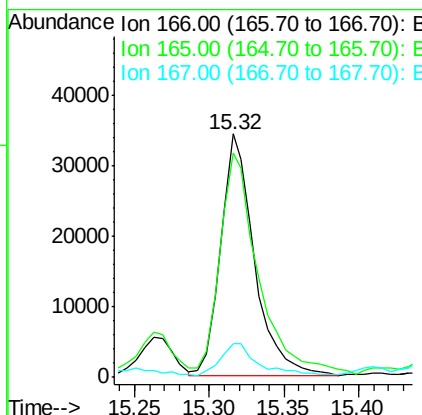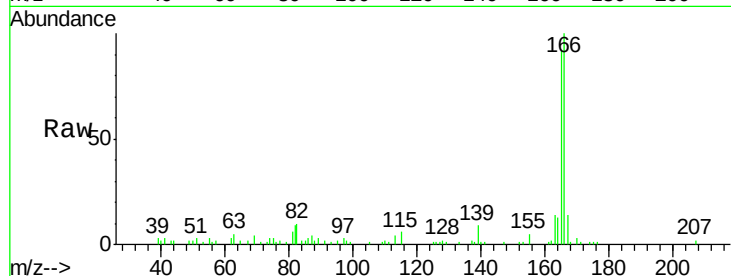

#69
 Phenanthrene
 Concen: 13.14 ng/ul
 RT: 17.06 min Scan# 2460
 Delta R.T. 0.00 min
 Lab File: BM006509.D
 Acq: 17 Jul 2016 10:34

Tgt Ion:178 Resp: 692480
 Ion Ratio Lower Upper
 178 100
 179 14.8 11.9 17.9
 176 18.7 15.2 22.8

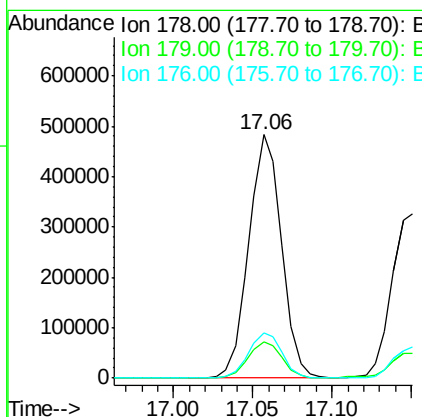

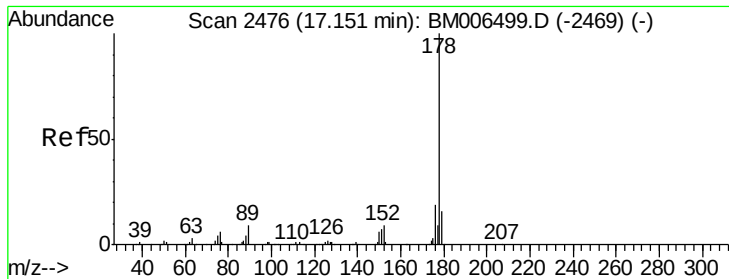





#71
 Anthracene
 Concen: 8.76 ng/ul
 RT: 17.15 min Scan# 2476
 Delta R.T. 0.00 min
 Lab File: BM006509.D
 Acq: 17 Jul 2016 10:34

Instrument :
 BNA_M
 ClientSampleId :
 BDJ37

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.3	12.0	18.0
176	18.9	15.0	22.6




Manual Integrations


sohil
 7/18/2016 7:40:14 PM

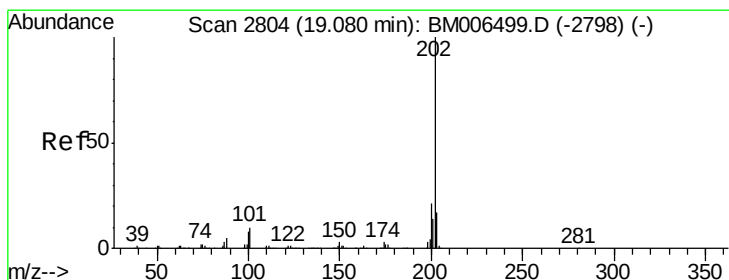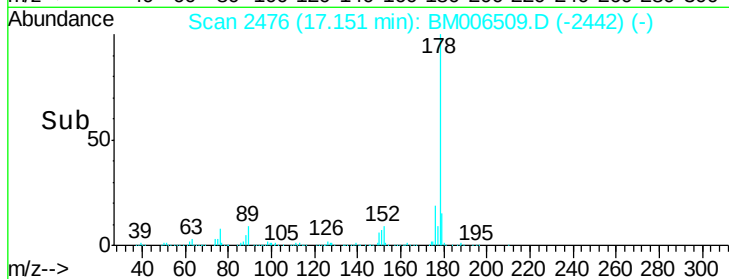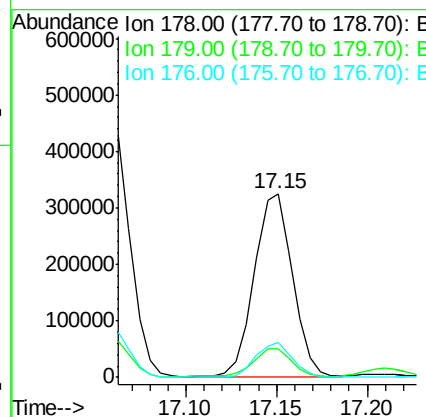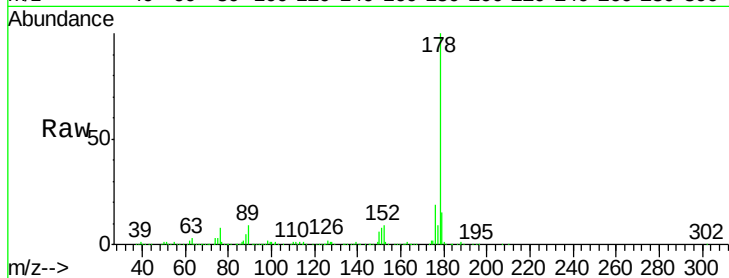

#74
 Fluoranthene
 Concen: 42.39 ng/ul
 RT: 19.08 min Scan# 2804
 Delta R.T. 0.00 min
 Lab File: BM006509.D
 Acq: 17 Jul 2016 10:34

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.9	8.6	12.8
100	7.4	6.4	9.6

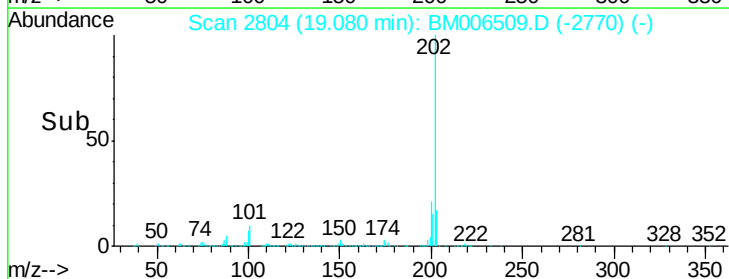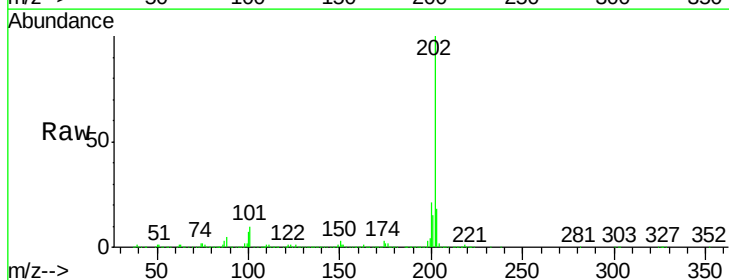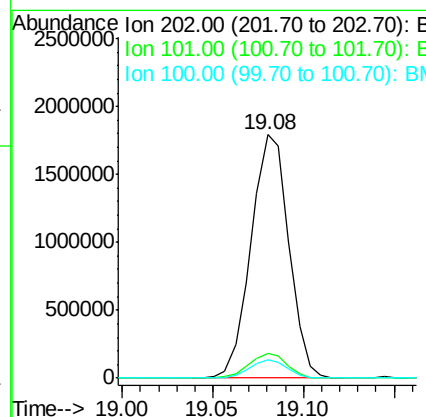

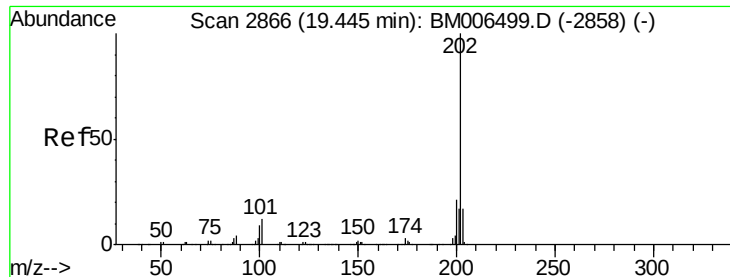

#77

Pyrene

Concen: 36.22 ng/ul

RT: 19.44 min Scan# 2866

Delta R.T. 0.00 min

Lab File: BM006509.D

Acq: 17 Jul 2016 10:34

Instrument :

BNA_M

ClientSampleId :

BDJ37

Tgt Ion:202 Resp: 2189969

Ion Ratio Lower Upper

202 100


101 11.8 10.0 15.0

100 9.6 7.9 11.9

Manual Integrations

sohil




7/18/2016 7:40:14 PM

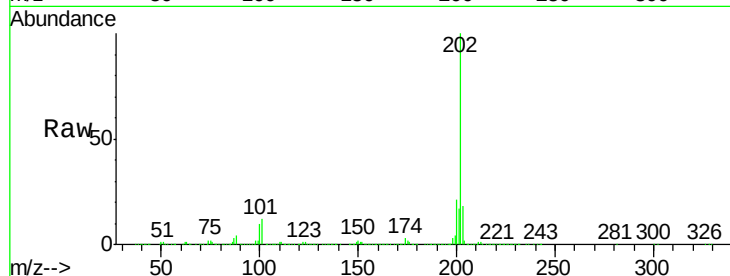

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

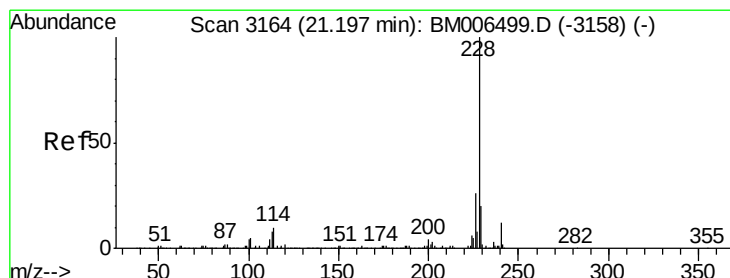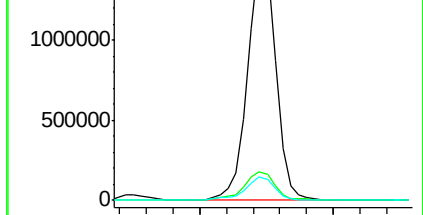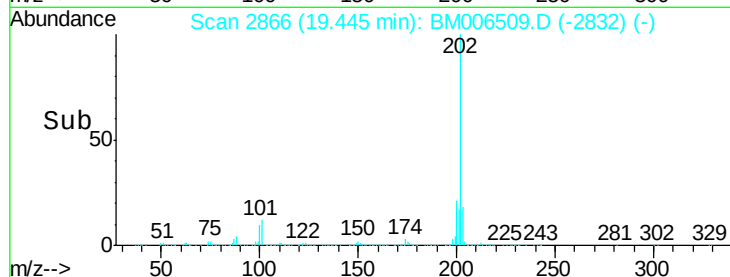

#80

Benzo(a)anthracene

Concen: 25.44 ng/ul

RT: 21.20 min Scan# 3164

Delta R.T. 0.00 min

Lab File: BM006509.D

Acq: 17 Jul 2016 10:34


Tgt Ion:228 Resp: 1572329

Ion Ratio Lower Upper

228 100

229 20.5 15.6 23.4



226 29.9 21.4 32.2

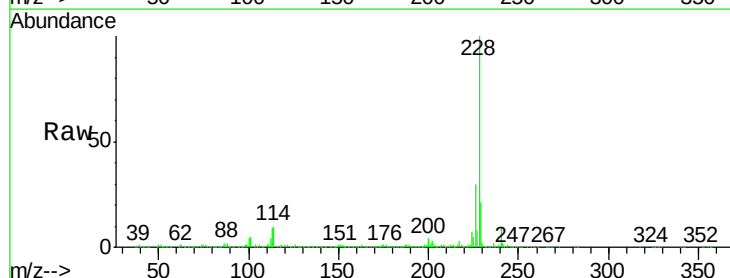


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

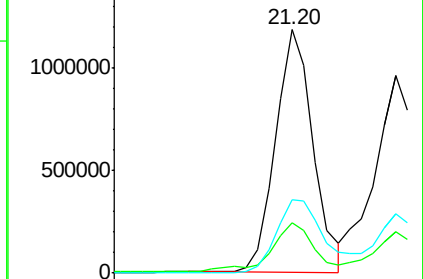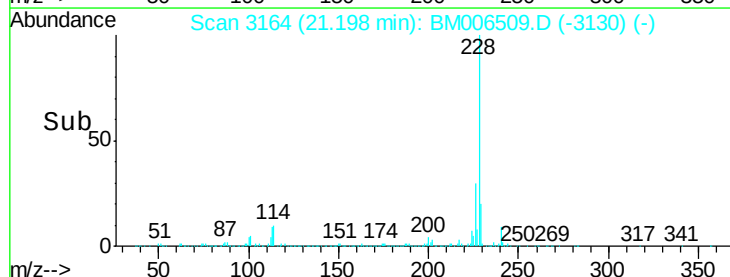

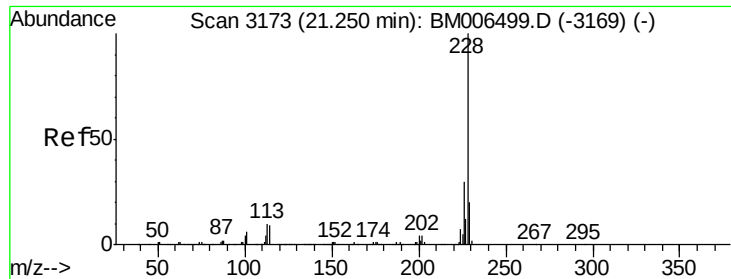

#82

Chrysene

Concen: 23.45 ng/ul

RT: 21.25 min Scan# 3173

Delta R.T. 0.00 min

Lab File: BM006509.D

Acq: 17 Jul 2016 10:34

Instrument :

BNA_M

ClientSampleId :

BDJ37

Tgt Ion:228 Resp: 1364672

Ion Ratio Lower Upper

228 100


226 29.7 23.3 34.9

229 20.9 15.8 23.8

Manual Integrations

sohil




7/18/2016 7:40:14 PM

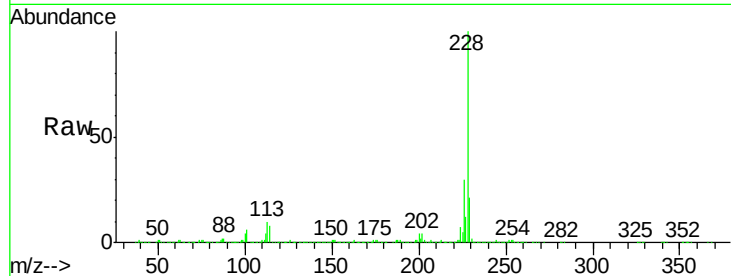

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

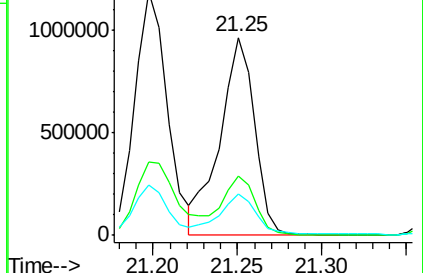

#85

Benzo(b)fluoranthene

Concen: 26.59 ng/ul

RT: 22.76 min Scan# 3429

Delta R.T. 0.00 min

Lab File: BM006509.D

Acq: 17 Jul 2016 10:34


Tgt Ion:252 Resp: 1827019

Ion Ratio Lower Upper

252 100

253 22.9 17.4 26.2



125 9.2 6.7 10.1




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

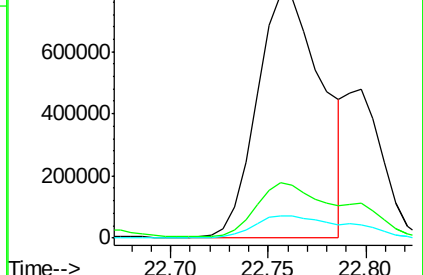

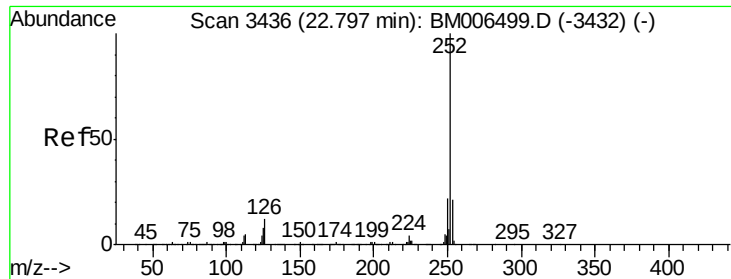

#86

Benzo(k)fluoranthene

Concen: 9.53 ng/ul m

RT: 22.80 min Scan# 3436

Delta R.T. 0.00 min

Lab File: BM006509.D

Acq: 17 Jul 2016 10:34

Instrument :

BNA_M

ClientSampled :


BDJ37

Tgt Ion:	252	Resp:	616065
Ion Ratio	Lower	Upper	
252	100		
253	23.3	17.3	25.9
125	9.0	7.0	10.4




Manual Integrations

sohil

7/18/2016 7:40:14 PM



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

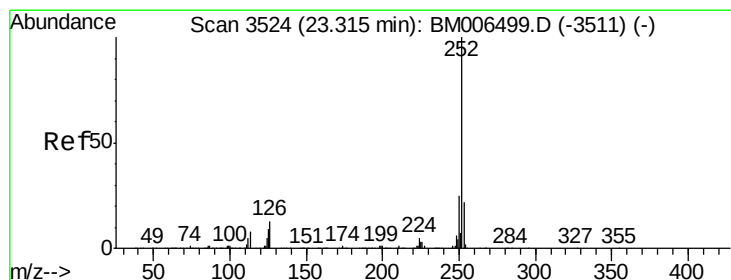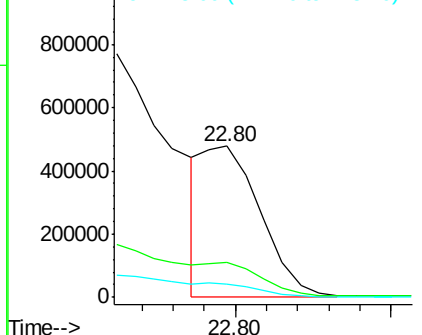

#88

Benzo(a)pyrene

Concen: 21.22 ng/ul

RT: 23.32 min Scan# 3525




Delta R.T. 0.01 min


Lab File: BM006509.D

Acq: 17 Jul 2016 10:34

Tgt Ion:	252	Resp:	1397057
Ion Ratio	Lower	Upper	
252	100		
253	22.9	17.4	26.2
125	9.3	7.6	11.4

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

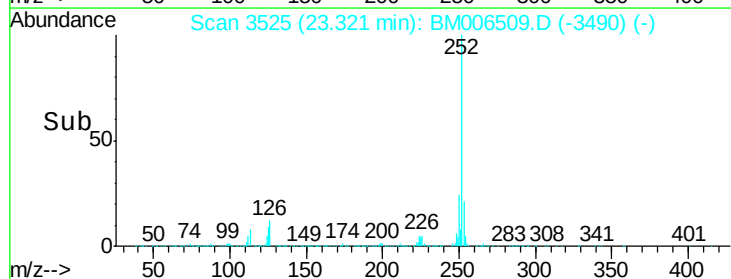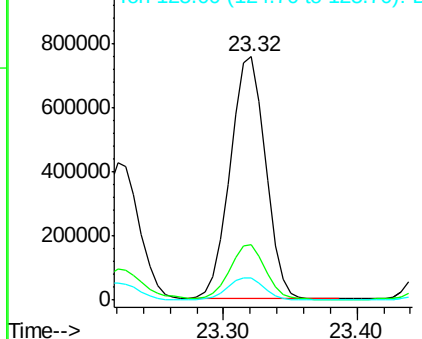

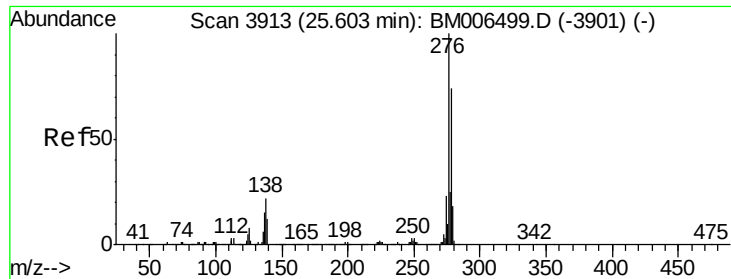





#89
 Indeno(1,2,3-cd)pyrene
 Concen: 10.68 ng/ul
 RT: 25.60 min Scan# 3913
 Delta R.T. 0.00 min
 Lab File: BM006509.D
 Acq: 17 Jul 2016 10:34

Instrument :
 BNA_M
 ClientSampleId :
 BDJ37

Tgt Ion	Ratio	Lower	Upper
276	100		
138	18.4	17.8	26.6
277	24.7	20.1	30.1




Manual Integrations


sohil
 7/18/2016 7:40:14 PM

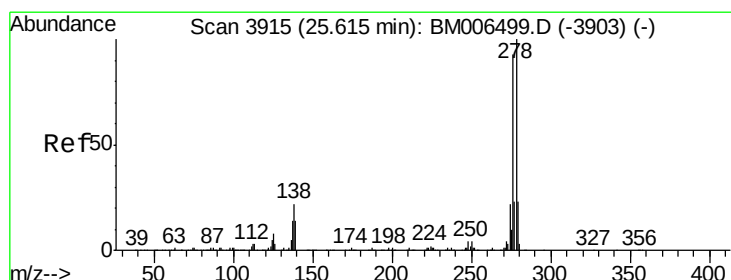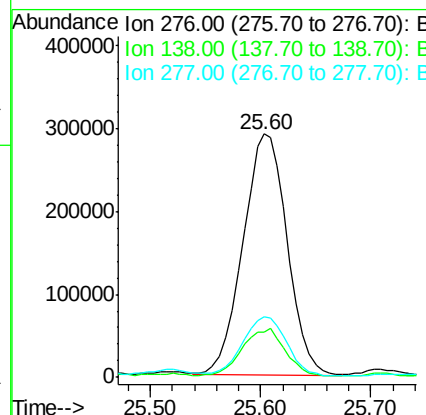

#90
 Dibenzo(a,h)anthracene
 Concen: 3.52 ng/ul
 RT: 25.61 min Scan# 3914
 Delta R.T. -0.01 min
 Lab File: BM006509.D
 Acq: 17 Jul 2016 10:34

Tgt Ion	Ratio	Lower	Upper
278	100		
139	18.6	11.7	17.5#
279	25.5	19.2	28.8

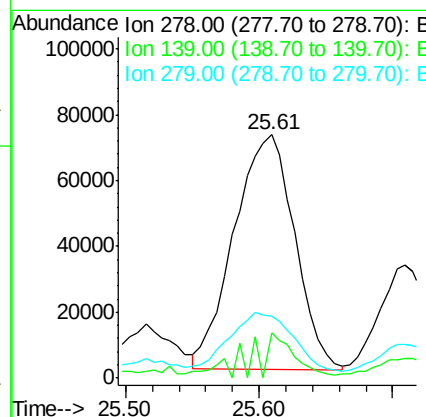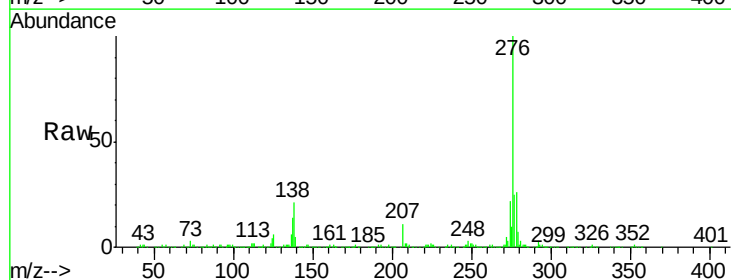

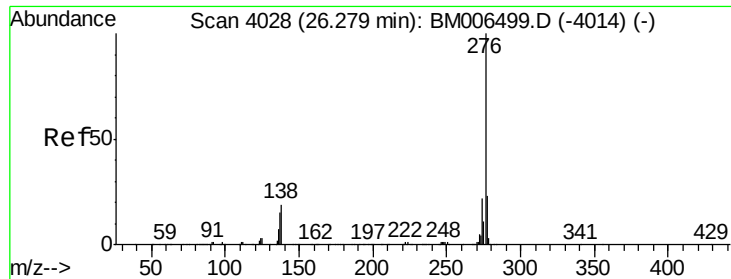

#91
 Benzo(g,h,i)perylene
 Concen: 9.31 ng/ul
 RT: 26.28 min Scan# 4028
 Delta R.T. 0.00 min
 Lab File: BM006509.D
 Acq: 17 Jul 2016 10:34

Instrument :
 BNA_M
 ClientSampleId :
 BDJ37

Tgt Ion:	276	Resp:	630266
Ion Ratio		Lower	Upper
276	100		
138	19.0	15.0	22.4
277	23.5	19.0	28.4

Manual Integrations

sohil
 7/18/2016 7:40:14 PM

