

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
 Data File : BM006511.D
 Acq On : 17 Jul 2016 11:47
 Operator : UM/SJ
 Sample : H3985-16
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ51

Manual Integrations

sohil
 7/18/2016 7:40:10 PM

Quant Time: Jul 18 08:45:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 18 07:39:41 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	149656	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	650560	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	363689	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	826308	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	928895	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	999760	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	5642	1.59	ng/uL	0.00
5) Phenol-d5	6.79	99	290323	23.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	189177	25.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	235417	23.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	236213	24.24	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	113977	23.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	127802	22.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	228030	21.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	254844	23.18	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	763973	25.67	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	944605	25.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	119191	23.05	ng/ul	0.00
57) Fluorene-d10	15.26	176	670802	25.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	88767	18.57	ng/ul	0.00
70) Anthracene-d10	17.12	188	1045572	26.77	ng/ul	0.00
76) Pyrene-d10	19.42	212	1194284	28.36	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1269416	27.77	ng/ul	0.00

Target Compounds

					Qvalue	
44) Dimethylphthalate	13.73	163	318059	10.53	ng/ul	99
47) Acenaphthylene	13.99	152	74715	1.95	ng/ul#	94
49) Acenaphthene	14.33	153	61415	2.49	ng/ul	98
58) Fluorene	15.32	166	66339	2.31	ng/ul	96
69) Phenanthrene	17.06	178	525136	11.56	ng/ul	98
71) Anthracene	17.15	178	239053	5.12	ng/ul	98
74) Fluoranthene	19.08	202	553899	10.49	ng/ul	99
77) Pyrene	19.44	202	685587	12.36	ng/ul	99
80) Benzo(a)anthracene	21.20	228	422076m	7.44	ng/ul	
82) Chrysene	21.25	228	422158	7.91	ng/ul	96
85) Benzo(b)fluoranthene	22.76	252	340367m	5.70	ng/ul	
86) Benzo(k)fluoranthene	22.78	252	168395m	3.00	ng/ul	
88) Benzo(a)pyrene	23.32	252	395489	6.91	ng/ul	100
89) Indeno(1,2,3-cd)pyrene	25.60	276	192609	2.89	ng/ul	96
90) Dibenzo(a,h)anthracene	25.60	278	65430	1.18	ng/ul#	88
91) Benzo(g,h,i)perylene	26.28	276	173968	2.96	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006511.D
Acq On : 17 Jul 2016 11:47
Operator : UM/SJ
Sample : H3985-16
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BDJ51

Manual Integrations

Quant Time: Jul 18 08:45:40 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 18 07:39:41 2016
Response via : Initial Calibration

sohil
7/18/2016 7:40:10 PM

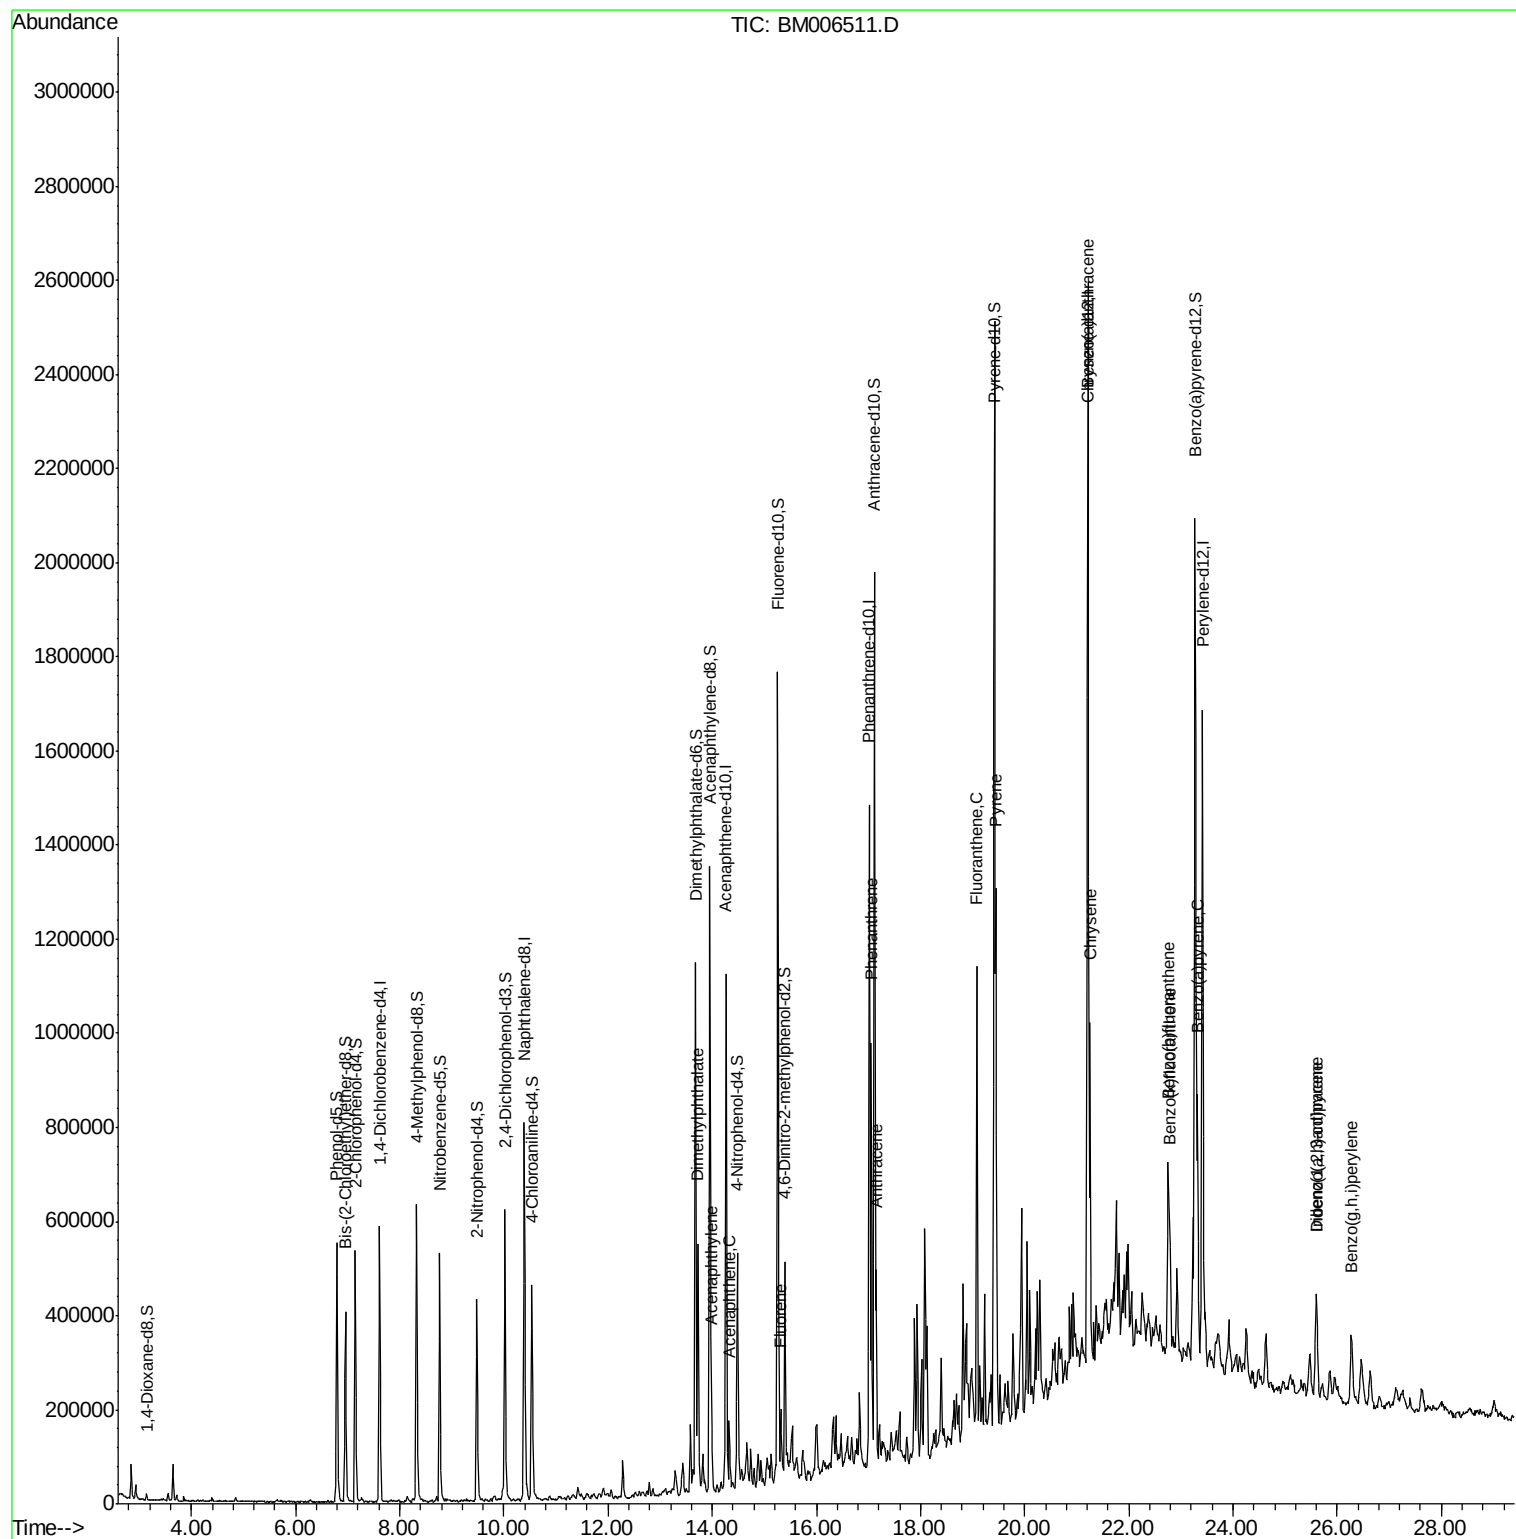

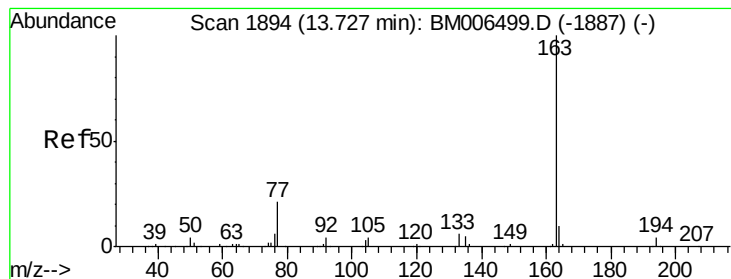

#44

Dimethylphthalate

Concen: 10.53 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. 0.00 min

Lab File: BM006511.D


Acq: 17 Jul 2016 11:47

Instrument :

BNA_M

ClientSampleId :

BDJ51

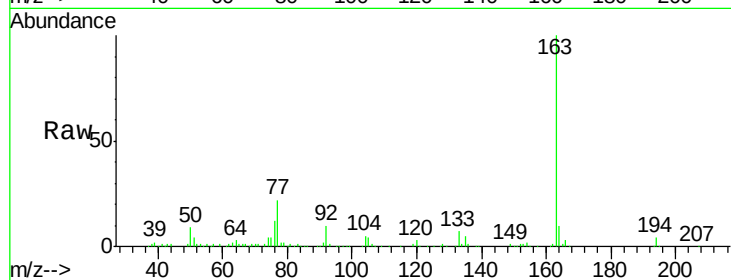

Tgt Ion:163 Resp: 318059

Ion Ratio Lower Upper

163 100



194 4.0 3.4 5.0

164 10.0 7.8 11.8

Manual Integrations

sohil

7/18/2016 7:40:10 PM

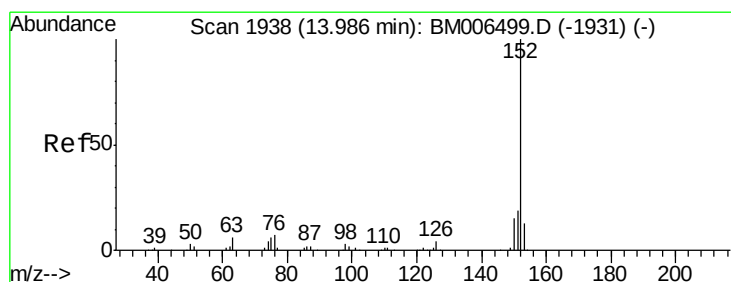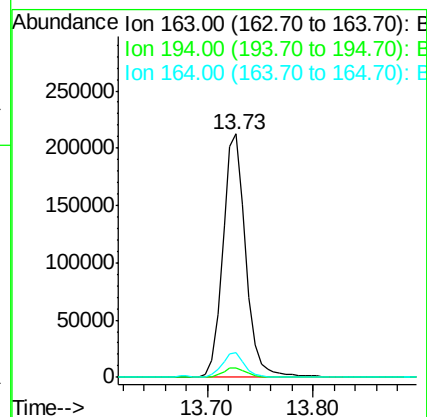

#47

Acenaphthylene

Concen: 1.95 ng/ul

RT: 13.99 min Scan# 1938

Delta R.T. 0.00 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47




Tgt Ion:152 Resp: 74715


Ion Ratio Lower Upper

152 100

151 21.8 15.6 23.4

153 16.0 10.3 15.5#

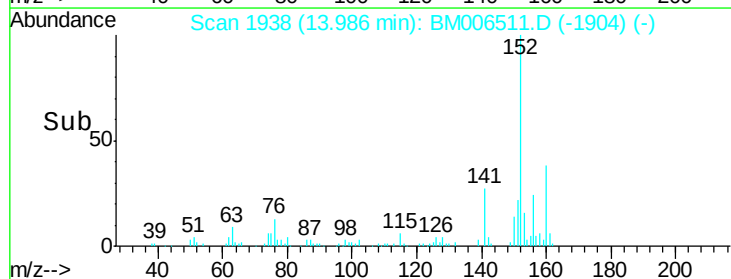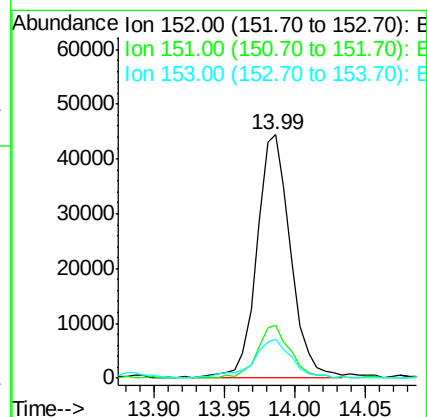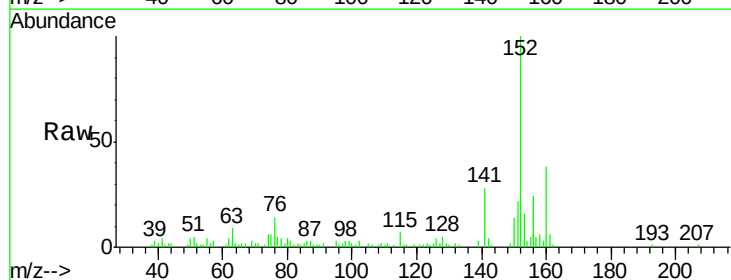



#49

Acenaphthene

Concen: 2.49 ng/ul

RT: 14.33 min Scan# 1996

Delta R.T. 0.00 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47

Instrument :

BNA_M

ClientSampleId :

BDJ51

Tgt Ion:153 Resp: 61415

Ion Ratio Lower Upper

153 100


152 46.1 37.7 56.5

154 85.4 70.0 105.0

Manual Integrations

sohil




7/18/2016 7:40:10 PM



Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

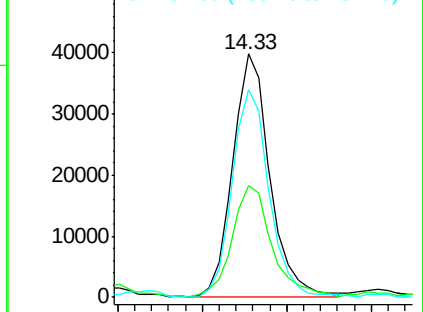

#58

Fluorene

Concen: 2.31 ng/ul

RT: 15.32 min Scan# 2164

Delta R.T. -0.01 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47


Tgt Ion:166 Resp: 66339

Ion Ratio Lower Upper

166 100

165 92.7 77.5 116.3



167 15.8 10.8 16.2




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

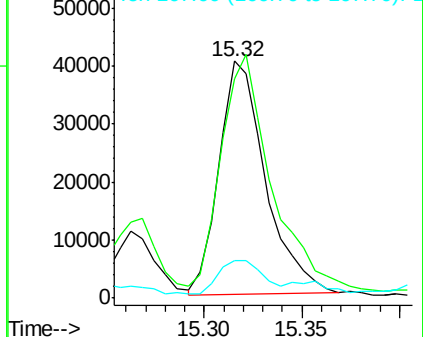



#69

Phenanthrene

Concen: 11.56 ng/ul

RT: 17.06 min Scan# 2460

Delta R.T. 0.00 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47

Instrument :

BNA_M

ClientSampleId :

BDJ51

Tgt Ion:178 Resp: 525136

Ion Ratio Lower Upper

178 100


179 15.7 11.9 17.9

176 20.0 15.2 22.8

Manual Integrations

sohil




7/18/2016 7:40:10 PM



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

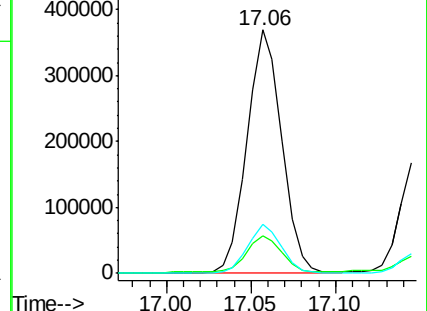

#71

Anthracene

Concen: 5.12 ng/ul

RT: 17.15 min Scan# 2476

Delta R.T. 0.00 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47


Tgt Ion:178 Resp: 239053

Ion Ratio Lower Upper

178 100

179 14.6 12.0 18.0



176 17.9 15.0 22.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

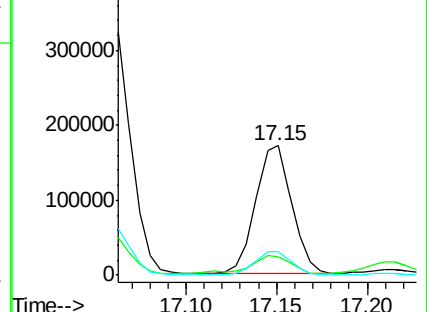

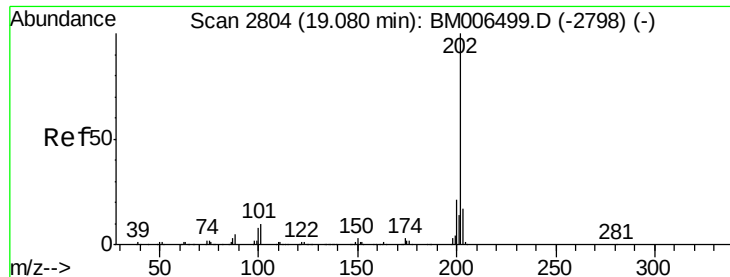

#74

Fluoranthene

Concen: 10.49 ng/ul

RT: 19.08 min Scan# 2804

Delta R.T. 0.00 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47

Instrument :

BNA_M

ClientSampled :


BDJ51

Tgt Ion:	202	Resp:	553899
Ion Ratio	Lower	Upper	
202	100		
101	10.2	8.6	12.8
100	7.7	6.4	9.6

Manual Integrations

sohil


7/18/2016 7:40:10 PM

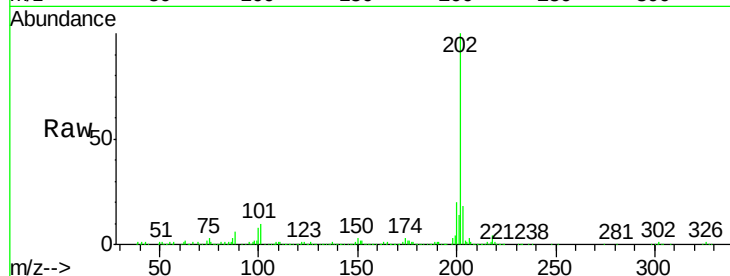



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

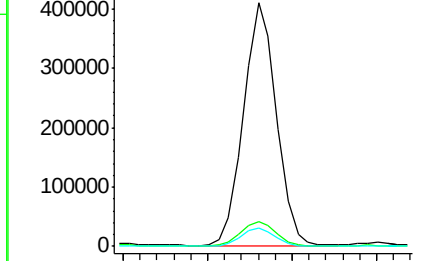

Time-->

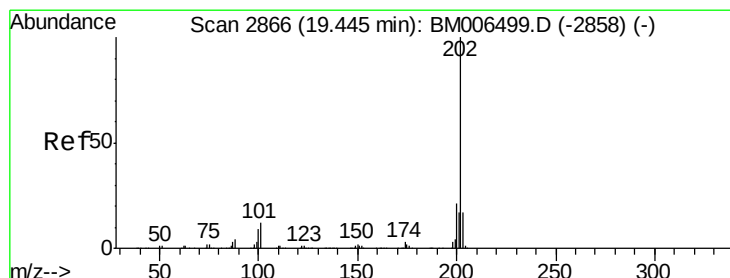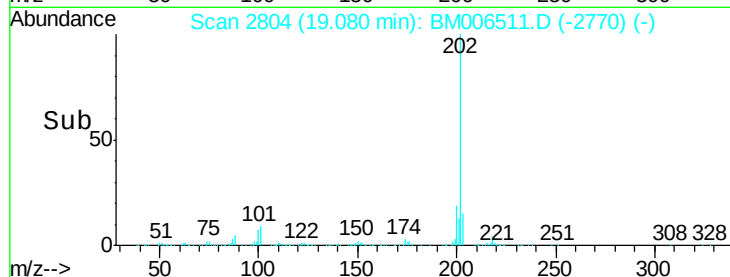

#77

Pyrene

Concen: 12.36 ng/ul


RT: 19.44 min Scan# 2866

Delta R.T. 0.00 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47


Tgt Ion:	202	Resp:	685587
Ion Ratio	Lower	Upper	
202	100		
101	13.3	10.0	15.0
100	10.1	7.9	11.9

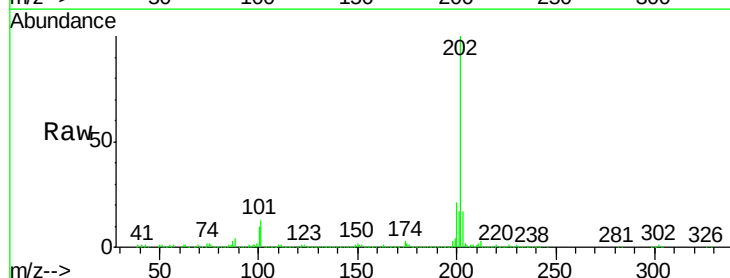


Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

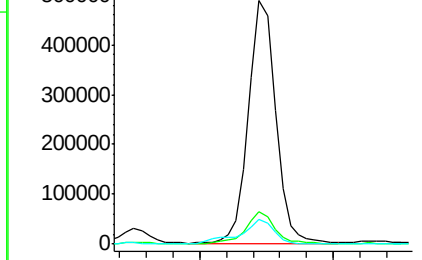

Time-->

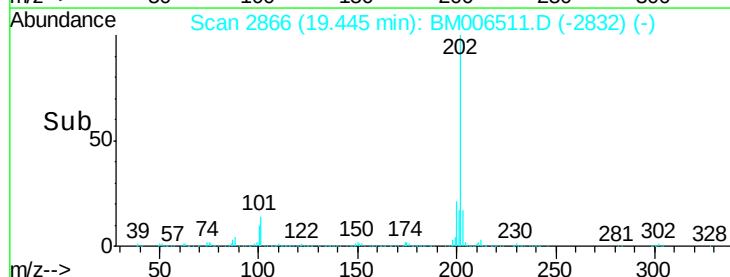

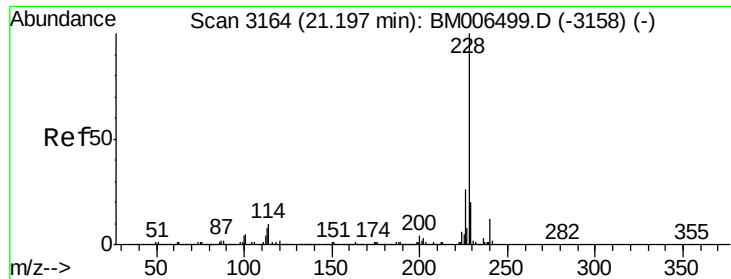





#80
Benzo(a)anthracene
Concen: 7.44 ng/ul m
RT: 21.20 min Scan# 3165
Delta R.T. 0.01 min
Lab File: BM006511.D
Acq: 17 Jul 2016 11:47

Instrument :
BNA_M
ClientSampleId :
BDJ51

Tgt Ion	Ratio	Lower	Upper
228	100		
229	22.0	15.6	23.4
226	36.5	21.4	32.2




Manual Integrations


sohil
7/18/2016 7:40:10 PM

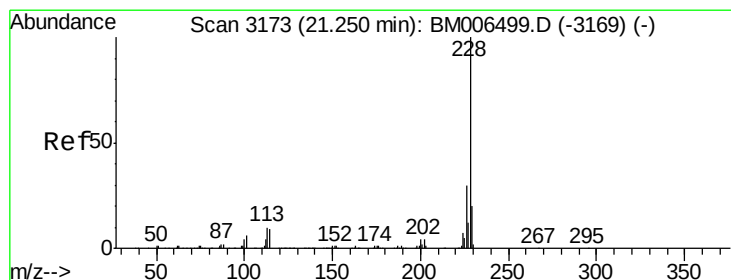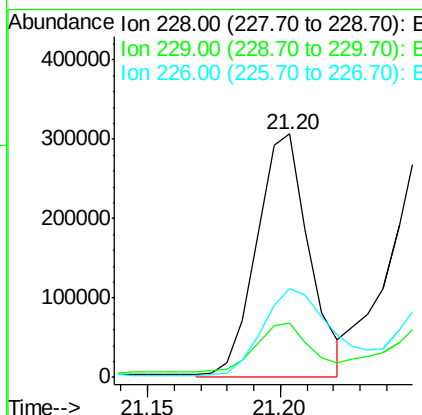

#82
Chrysene
Concen: 7.91 ng/ul
RT: 21.25 min Scan# 3173
Delta R.T. 0.00 min
Lab File: BM006511.D
Acq: 17 Jul 2016 11:47

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.8	23.3	34.9
229	22.4	15.8	23.8

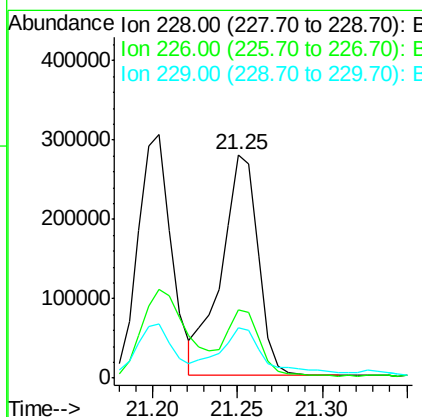

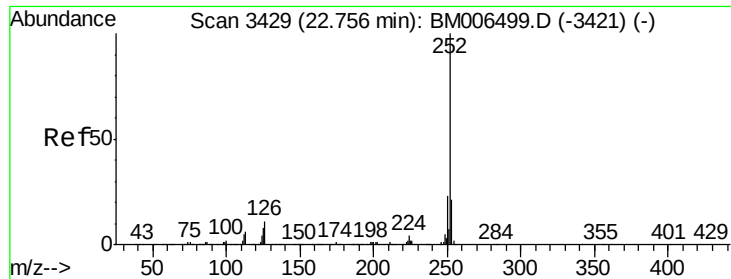

#85

Benzo(b)fluoranthene

Concen: 5.70 ng/ul m

RT: 22.76 min Scan# 3429

Delta R.T. 0.00 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47

Instrument :

BNA_M

ClientSampled :





BDJ51

Tgt Ion:	252	Resp:	340367
Ion Ratio	Lower	Upper	
252	100		
253	22.1	17.4	26.2
125	10.0	6.7	10.1

Manual Integrations

sohil

7/18/2016 7:40:10 PM

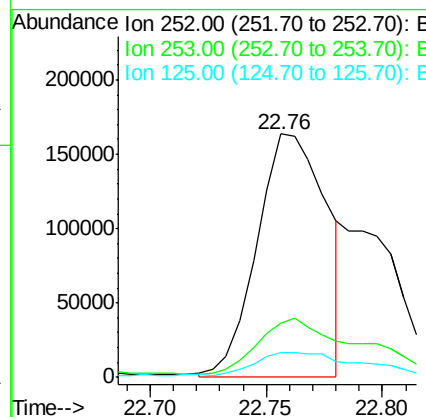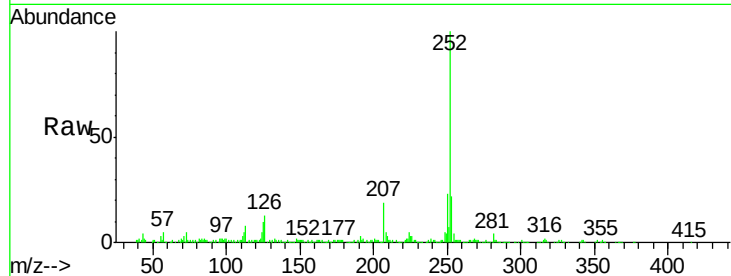

#86

Benzo(k)fluoranthene

Concen: 3.00 ng/ul m




RT: 22.78 min Scan# 3433


Delta R.T. -0.02 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47

Tgt Ion:	252	Resp:	168395
Ion Ratio	Lower	Upper	
252	100		
253	22.8	17.3	25.9
125	10.2	7.0	10.4

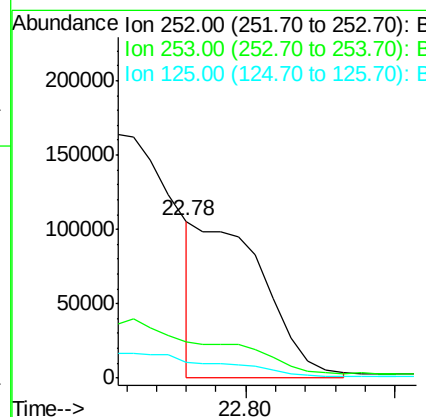

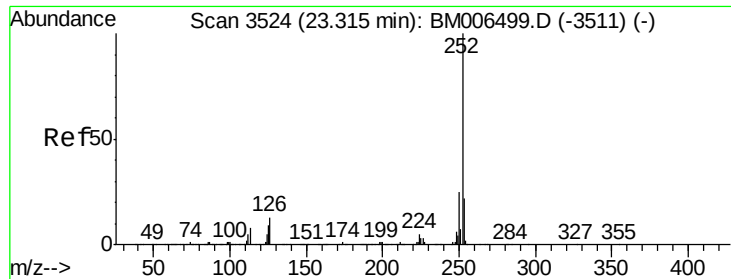

#88

Benzo(a)pyrene

Concen: 6.91 ng/ul

RT: 23.32 min Scan# 3524

Delta R.T. 0.00 min

Lab File: BM006511.D


Acq: 17 Jul 2016 11:47

Instrument :

BNA_M

ClientSampleId :




BDJ51



Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.9	17.4	26.2
125	9.9	7.6	11.4

Manual Integrations

sohil
7/18/2016 7:40:10 PM

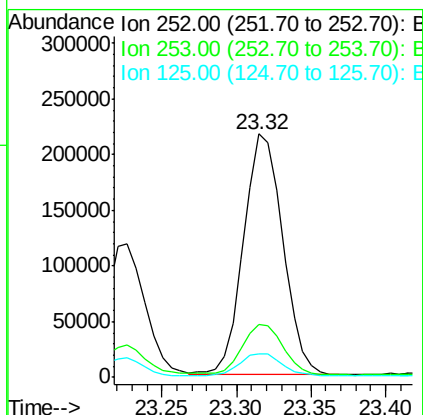

#89

Indeno(1,2,3-cd)pyrene


Concen: 2.89 ng/ul

RT: 25.60 min Scan# 3913



Delta R.T. 0.00 min


Lab File: BM006511.D

Acq: 17 Jul 2016 11:47



Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.4	17.8	26.6
277	23.7	20.1	30.1

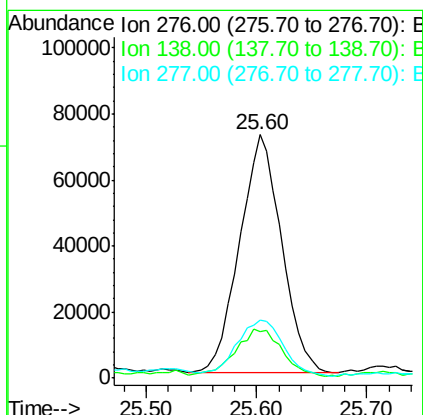

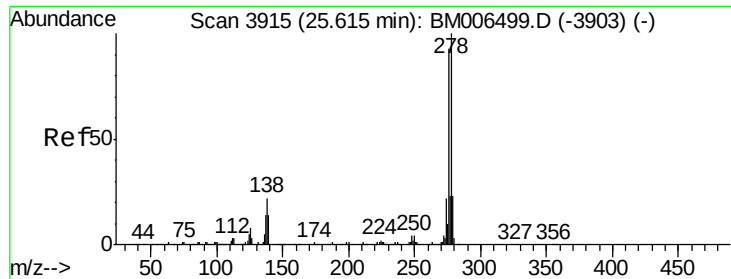

#90

Dibenzo(a,h)anthracene

Concen: 1.18 ng/ul

RT: 25.60 min Scan# 3913

Delta R.T. -0.01 min

Lab File: BM006511.D


Acq: 17 Jul 2016 11:47

Instrument :

BNA_M

ClientSampled :

BDJ51


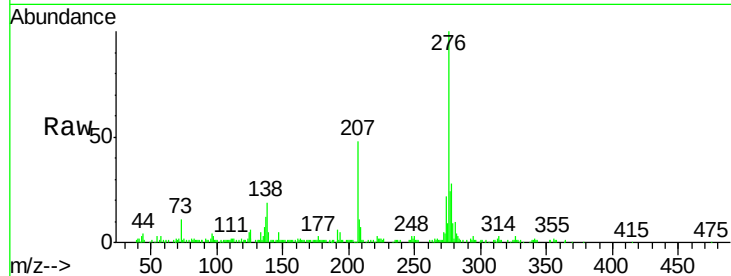


Tgt Ion:	278	Resp:	65430
Ion Ratio	Lower	Upper	
278	100		
139	18.5	11.7	17.5#
279	30.7	19.2	28.8#

Manual Integrations

sohil

7/18/2016 7:40:10 PM

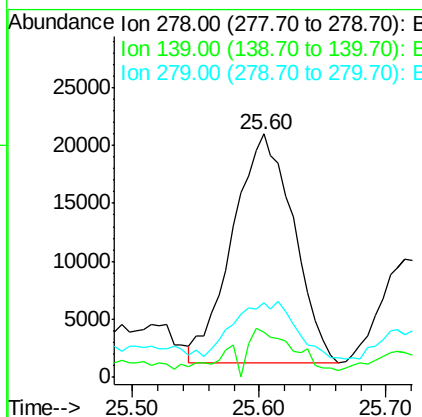

#91

Benzo(g,h,i)perylene

Concen: 2.96 ng/ul

RT: 26.28 min Scan# 4028

Delta R.T. 0.00 min

Lab File: BM006511.D

Acq: 17 Jul 2016 11:47

Tgt Ion:	276	Resp:	173968
Ion Ratio	Lower	Upper	
276	100		
138	22.2	15.0	22.4
277	24.9	19.0	28.4

