

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
 Data File : BM006473.D
 Acq On : 16 Jul 2016 11:29
 Operator : UM/SJ
 Sample : H3959-07
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	708	715	728	rBV	381212	670565	20.16%	2.002%
2	6.957	737	743	755	rBV	298033	475324	14.29%	1.419%
3	7.151	770	776	786	rBV	406953	643188	19.33%	1.921%
4	7.616	848	855	870	rVB	710137	1143822	34.38%	3.415%
5	8.322	969	975	989	rVB	373336	645989	19.42%	1.929%
6	8.769	1042	1051	1061	rBV	380123	630683	18.96%	1.883%
7	9.486	1165	1173	1183	rBV	297789	513081	15.42%	1.532%
8	10.022	1258	1264	1287	rBV	432301	764727	22.99%	2.283%
9	10.392	1320	1327	1340	rBV	913071	1643615	49.41%	4.908%
10	10.539	1345	1352	1363	rBV	383492	723729	21.76%	2.161%
11	13.163	1792	1798	1803	rBV	30963	48139	1.45%	0.144%
12	13.680	1880	1886	1890	rBV	781387	1152968	34.66%	3.443%
13	13.727	1890	1894	1909	rVB	565924	876982	26.36%	2.619%
14	13.957	1926	1933	1951	rVB	896236	1375232	41.34%	4.106%
15	14.269	1979	1986	2000	rVB2	1321919	2113999	63.55%	6.312%
16	14.486	2016	2023	2041	rBV	299301	555121	16.69%	1.658%
17	15.263	2149	2155	2163	rVB	1144063	1744419	52.44%	5.209%
18	15.398	2172	2178	2192	rBV	314678	467652	14.06%	1.396%
19	15.974	2270	2276	2287	rBV2	73665	167499	5.03%	0.500%
20	16.563	2372	2376	2384	rBV3	23853	37089	1.11%	0.111%
21	16.780	2408	2413	2420	rBV2	37840	69705	2.10%	0.208%
22	17.015	2447	2453	2463	rBV	1746799	2575332	77.41%	7.690%
23	17.115	2464	2470	2481	rVB	1313278	1904998	57.26%	5.688%
24	19.415	2855	2861	2869	rBV2	1607916	2321019	69.77%	6.931%
25	20.939	3115	3120	3124	rBV3	38653	64782	1.95%	0.193%
26	21.133	3150	3153	3158	rBV	30834	44817	1.35%	0.134%
27	21.215	3162	3167	3173	rBV	2477085	3254884	97.84%	9.719%
28	22.250	3340	3343	3347	rVB2	35968	45353	1.36%	0.135%
29	22.744	3423	3427	3433	rVB	61548	93272	2.80%	0.279%
30	23.274	3510	3517	3527	rBV2	1284604	2502394	75.22%	7.472%
31	23.415	3533	3541	3553	rVB	1769716	3326709	100.00%	9.934%
32	23.921	3620	3627	3633	rVB2	106784	221764	6.67%	0.662%
33	24.638	3743	3749	3756	rVB	110460	248899	7.48%	0.743%
34	25.480	3885	3892	3902	rVB3	94847	241960	7.27%	0.722%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006473.D
Acq On : 16 Jul 2016 11:29
Operator : UM/SJ
Sample : H3959-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ24

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION

35	26.462	4056	4059	4069	rVB2	75332	179582	5.40%	0.536%
----	--------	------	------	------	------	-------	--------	-------	--------


Sum of corrected areas: 33489293

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006473.D
Acq On : 16 Jul 2016 11:29
Operator : UM/SJ
Sample : H3959-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ24

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

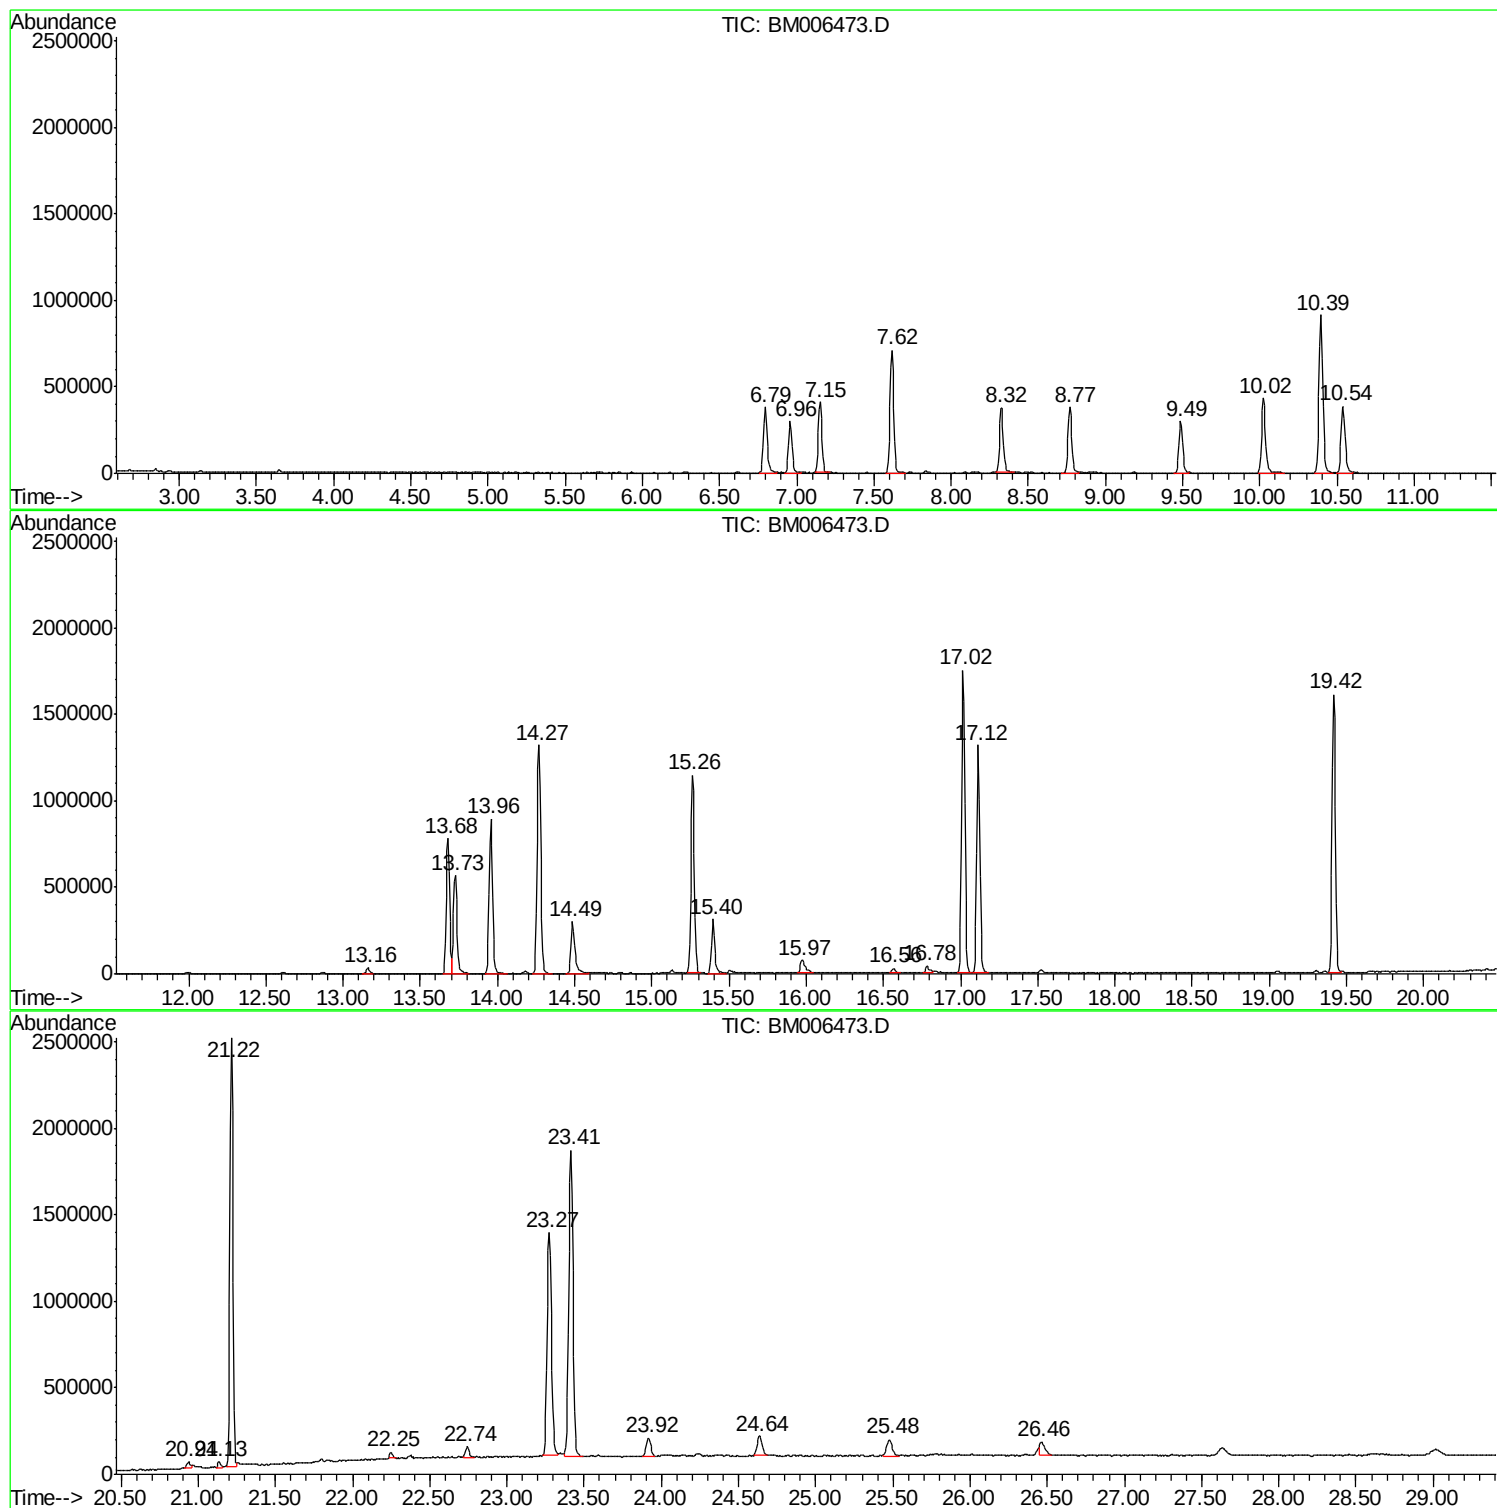

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006473.D
Acq On : 16 Jul 2016 11:29
Operator : UM/SJ
Sample : H3959-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ24

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006473.D
Acq On : 16 Jul 2016 11:29
Operator : UM/SJ
Sample : H3959-07
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ24

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc