

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
 Data File : BM006474.D
 Acq On : 16 Jul 2016 12:05
 Operator : UM/SJ
 Sample : H3959-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	135	139	153	rVB	28813	48903	1.17%	0.107%
2	6.793	708	715	730	rBV	654972	1129815	27.09%	2.479%
3	6.957	736	743	756	rBV	494487	788189	18.90%	1.729%
4	7.151	769	776	792	rBV	654041	1079150	25.88%	2.367%
5	7.616	848	855	864	rBV	711652	1142243	27.39%	2.506%
6	8.322	968	975	985	rBV	772029	1321538	31.69%	2.899%
7	8.769	1044	1051	1065	rBV	642069	1069622	25.65%	2.347%
8	9.486	1165	1173	1187	rBV	534853	898871	21.55%	1.972%
9	10.022	1257	1264	1283	rBV	753012	1322122	31.70%	2.900%
10	10.392	1320	1327	1341	rBV	882915	1610571	38.62%	3.533%
11	10.539	1345	1352	1369	rVB	675705	1251365	30.01%	2.745%
12	13.680	1880	1886	1890	rBV	1322704	1923302	46.12%	4.219%
13	13.727	1890	1894	1909	rVB	1024583	1549393	37.15%	3.399%
14	13.957	1925	1933	1948	rBV	1468700	2325235	55.76%	5.101%
15	14.269	1979	1986	1998	rVB2	1307373	2055045	49.28%	4.508%
16	14.486	2016	2023	2036	rBV	621728	1062289	25.47%	2.330%
17	15.127	2128	2132	2138	rVB	41322	55608	1.33%	0.122%
18	15.263	2149	2155	2165	rBV	1900445	2895746	69.44%	6.353%
19	15.398	2172	2178	2191	rBV	469849	700043	16.79%	1.536%
20	15.510	2191	2197	2200	rBV3	25843	43764	1.05%	0.096%
21	15.974	2268	2276	2277	rBV	76053	97921	2.35%	0.215%
22	16.786	2409	2414	2419	rBV2	75335	115329	2.77%	0.253%
23	17.015	2447	2453	2462	rBV2	1670177	2487743	59.65%	5.458%
24	17.115	2462	2470	2481	rVB2	2158005	3238682	77.66%	7.105%
25	17.521	2534	2539	2547	rBV	41654	57560	1.38%	0.126%
26	19.421	2855	2862	2869	rBV2	2648922	3873142	92.87%	8.497%
27	20.939	3115	3120	3131	rBV3	106154	248878	5.97%	0.546%
28	21.133	3150	3153	3157	rBV	47639	53347	1.28%	0.117%
29	21.215	3162	3167	3174	rBV2	2319378	3177441	76.19%	6.971%
30	21.333	3184	3187	3191	rVB3	38865	46422	1.11%	0.102%
31	22.250	3340	3343	3348	rBV3	34223	45162	1.08%	0.099%
32	22.374	3361	3364	3368	rBV	48793	60180	1.44%	0.132%
33	22.744	3424	3427	3433	rVB3	54125	76978	1.85%	0.169%
34	23.280	3510	3518	3528	rBV2	2146937	4170317	100.00%	9.149%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006474.D
Acq On : 16 Jul 2016 12:05
Operator : UM/SJ
Sample : H3959-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ25

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION

35	23.415	3534	3541	3553	rVB	1719614	3175075	76.14%	6.965%
36	23.921	3621	3627	3634	rVB	93452	181915	4.36%	0.399%
37	24.638	3745	3749	3765	rVB2	95430	204557	4.91%	0.449%


Sum of corrected areas: 45583463

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006474.D
Acq On : 16 Jul 2016 12:05
Operator : UM/SJ
Sample : H3959-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

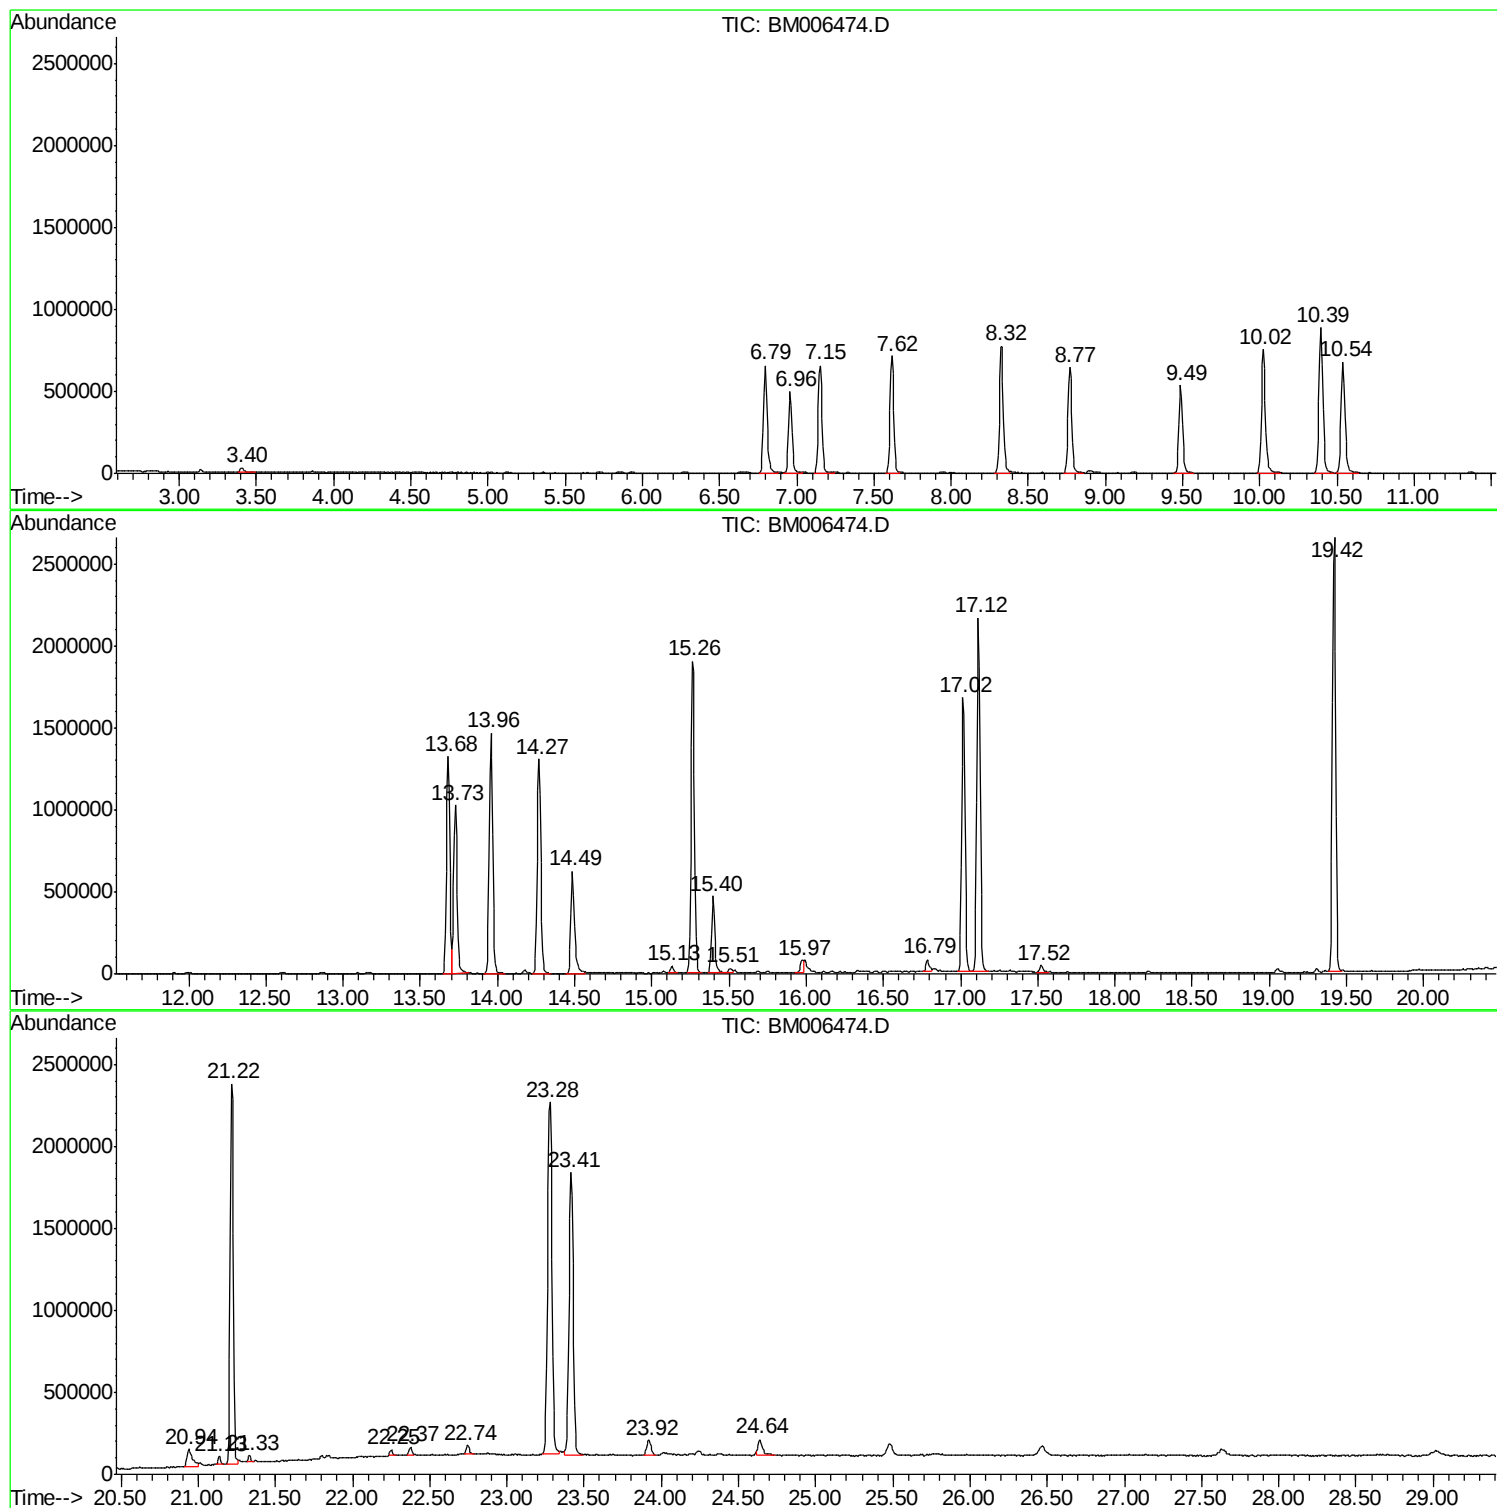

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006474.D
Acq On : 16 Jul 2016 12:05
Operator : UM/SJ
Sample : H3959-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006474.D
Acq On : 16 Jul 2016 12:05
Operator : UM/SJ
Sample : H3959-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc