

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
 Data File : BM006476.D
 Acq On : 16 Jul 2016 13:18
 Operator : UM/SJ
 Sample : H3959-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	709	715	730	rBV	574867	973827	25.74%	2.391%
2	6.957	735	743	755	rBV	438146	694543	18.36%	1.705%
3	7.151	769	776	787	rBV	590586	948046	25.06%	2.327%
4	7.616	848	855	866	rBV	580278	932788	24.65%	2.290%
5	8.322	969	975	987	rBV	674450	1163469	30.75%	2.856%
6	8.769	1044	1051	1065	rBV	550789	948419	25.07%	2.328%
7	9.487	1166	1173	1187	rVB	469630	797768	21.09%	1.959%
8	10.022	1257	1264	1290	rVB	654288	1189750	31.45%	2.921%
9	10.392	1320	1327	1341	rBV	771571	1354381	35.80%	3.325%
10	10.539	1345	1352	1368	rBV	623119	1152295	30.46%	2.829%
11	13.680	1880	1886	1890	rBV	1195079	1748810	46.22%	4.293%
12	13.727	1890	1894	1912	rVB	1077903	1607418	42.49%	3.946%
13	13.957	1925	1933	1945	rBV	1349949	2100543	55.52%	5.157%
14	14.269	1979	1986	1997	rVB3	1118046	1769899	46.78%	4.345%
15	14.486	2017	2023	2040	rBV	513820	914922	24.18%	2.246%
16	15.127	2128	2132	2140	rVB2	31463	41114	1.09%	0.101%
17	15.263	2148	2155	2165	rBV	1721789	2657192	70.23%	6.523%
18	15.398	2172	2178	2191	rBV	490953	703704	18.60%	1.728%
19	15.992	2275	2279	2288	rBV	48007	88434	2.34%	0.217%
20	16.786	2409	2414	2420	rBV2	60449	97814	2.59%	0.240%
21	17.015	2447	2453	2462	rBV2	1458635	2183095	57.70%	5.359%
22	17.115	2463	2470	2482	rVB2	1978479	2972242	78.56%	7.297%
23	17.521	2534	2539	2549	rVB	44950	62950	1.66%	0.155%
24	19.421	2855	2862	2873	rBV	2466873	3526830	93.22%	8.658%
25	20.939	3115	3120	3136	rBV2	85009	228232	6.03%	0.560%
26	21.215	3161	3167	3175	rBV	2148532	2820972	74.56%	6.925%
27	22.250	3338	3343	3349	rBV5	53893	90548	2.39%	0.222%
28	22.744	3423	3427	3431	rBV2	42596	63059	1.67%	0.155%
29	23.274	3510	3517	3533	rBV2	2003432	3783435	100.00%	9.288%
30	23.415	3533	3541	3552	rVB	1446125	2838366	75.02%	6.968%
31	23.915	3622	3626	3634	rVB	70867	132876	3.51%	0.326%
32	24.638	3744	3749	3756	rVB3	69065	145713	3.85%	0.358%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006476.D
Acq On : 16 Jul 2016 13:18
Operator : UM/SJ
Sample : H3959-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ27

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION


Sum of corrected areas: 40733454

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006476.D
Acq On : 16 Jul 2016 13:18
Operator : UM/SJ
Sample : H3959-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ27

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

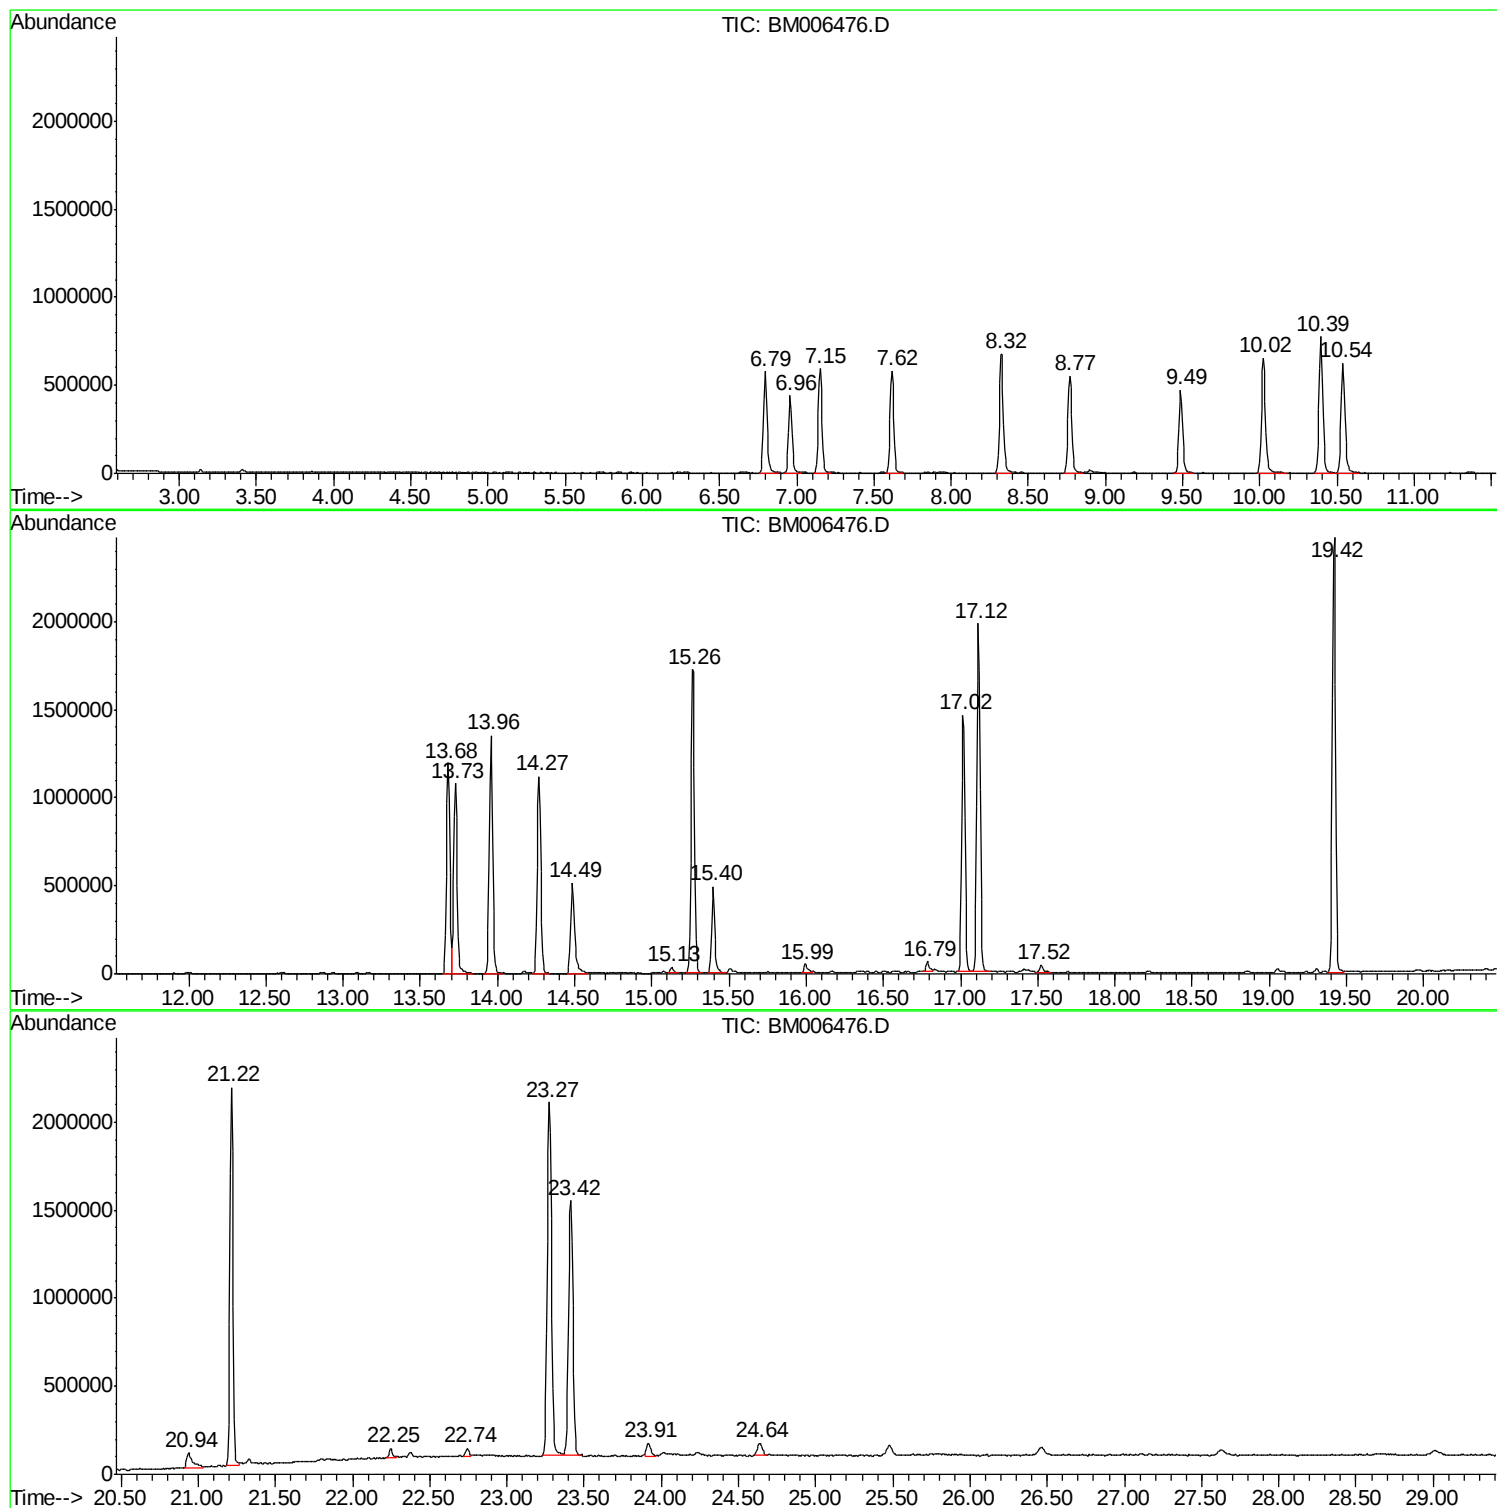

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006476.D
Acq On : 16 Jul 2016 13:18
Operator : UM/SJ
Sample : H3959-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ27

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006476.D
Acq On : 16 Jul 2016 13:18
Operator : UM/SJ
Sample : H3959-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ27

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc