

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
 Data File : BM006481.D
 Acq On : 16 Jul 2016 16:22
 Operator : UM/SJ
 Sample : H3959-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	709	715	732	rVB	490951	810426	24.79%	2.268%
2	6.957	736	743	755	rBV	385013	606084	18.54%	1.696%
3	7.151	768	776	788	rBV	510383	830727	25.41%	2.325%
4	7.616	848	855	865	rBV	579933	947861	28.99%	2.653%
5	8.322	969	975	991	rBV	579251	997308	30.50%	2.791%
6	8.769	1044	1051	1068	rBV	476660	806143	24.65%	2.256%
7	9.487	1165	1173	1186	rBV	391389	673850	20.61%	1.886%
8	10.022	1258	1264	1283	rBV	567443	991365	30.32%	2.775%
9	10.392	1320	1327	1340	rBV	751224	1356141	41.47%	3.796%
10	10.539	1344	1352	1367	rBV	529733	970633	29.68%	2.717%
11	13.680	1880	1886	1890	rBV	1016102	1473385	45.06%	4.124%
12	13.727	1890	1894	1915	rVB	617189	933994	28.56%	2.614%
13	13.957	1926	1933	1944	rBV	1144217	1783959	54.56%	4.993%
14	14.269	1978	1986	1998	rVB2	1105247	1741089	53.25%	4.873%
15	14.486	2017	2023	2040	rBV	365531	653981	20.00%	1.830%
16	15.127	2128	2132	2138	rBV	25081	32955	1.01%	0.092%
17	15.263	2149	2155	2164	rBV	1444673	2243583	68.61%	6.279%
18	15.398	2171	2178	2192	rBV	346558	540541	16.53%	1.513%
19	15.992	2274	2279	2288	rBV	35370	67634	2.07%	0.189%
20	16.786	2408	2414	2419	rBV2	45759	72390	2.21%	0.203%
21	17.015	2447	2453	2463	rBV	1424539	2108488	64.48%	5.901%
22	17.115	2463	2470	2481	rVB2	1663569	2499098	76.43%	6.995%
23	17.521	2535	2539	2544	rBV	31702	41783	1.28%	0.117%
24	19.415	2855	2861	2873	rBV	2018143	2934019	89.73%	8.212%
25	20.933	3115	3119	3135	rBV4	69467	178784	5.47%	0.500%
26	21.215	3161	3167	3174	rBV	2068948	2697211	82.49%	7.549%
27	22.245	3340	3342	3350	rVB5	31598	41872	1.28%	0.117%
28	22.739	3423	3426	3431	rVB	54912	69238	2.12%	0.194%
29	23.274	3509	3517	3528	rBV2	1668553	3269821	100.00%	9.152%
30	23.409	3533	3540	3552	rVB	1453760	2747082	84.01%	7.689%
31	23.915	3622	3626	3633	rVB2	103963	188145	5.75%	0.527%
32	24.633	3743	3748	3759	rVB2	101180	225999	6.91%	0.633%
33	25.474	3886	3891	3902	rVB2	76121	193637	5.92%	0.542%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006481.D
Acq On : 16 Jul 2016 16:22
Operator : UM/SJ
Sample : H3959-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ32

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION


Sum of corrected areas: 35729226

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006481.D
Acq On : 16 Jul 2016 16:22
Operator : UM/SJ
Sample : H3959-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BDJ32

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

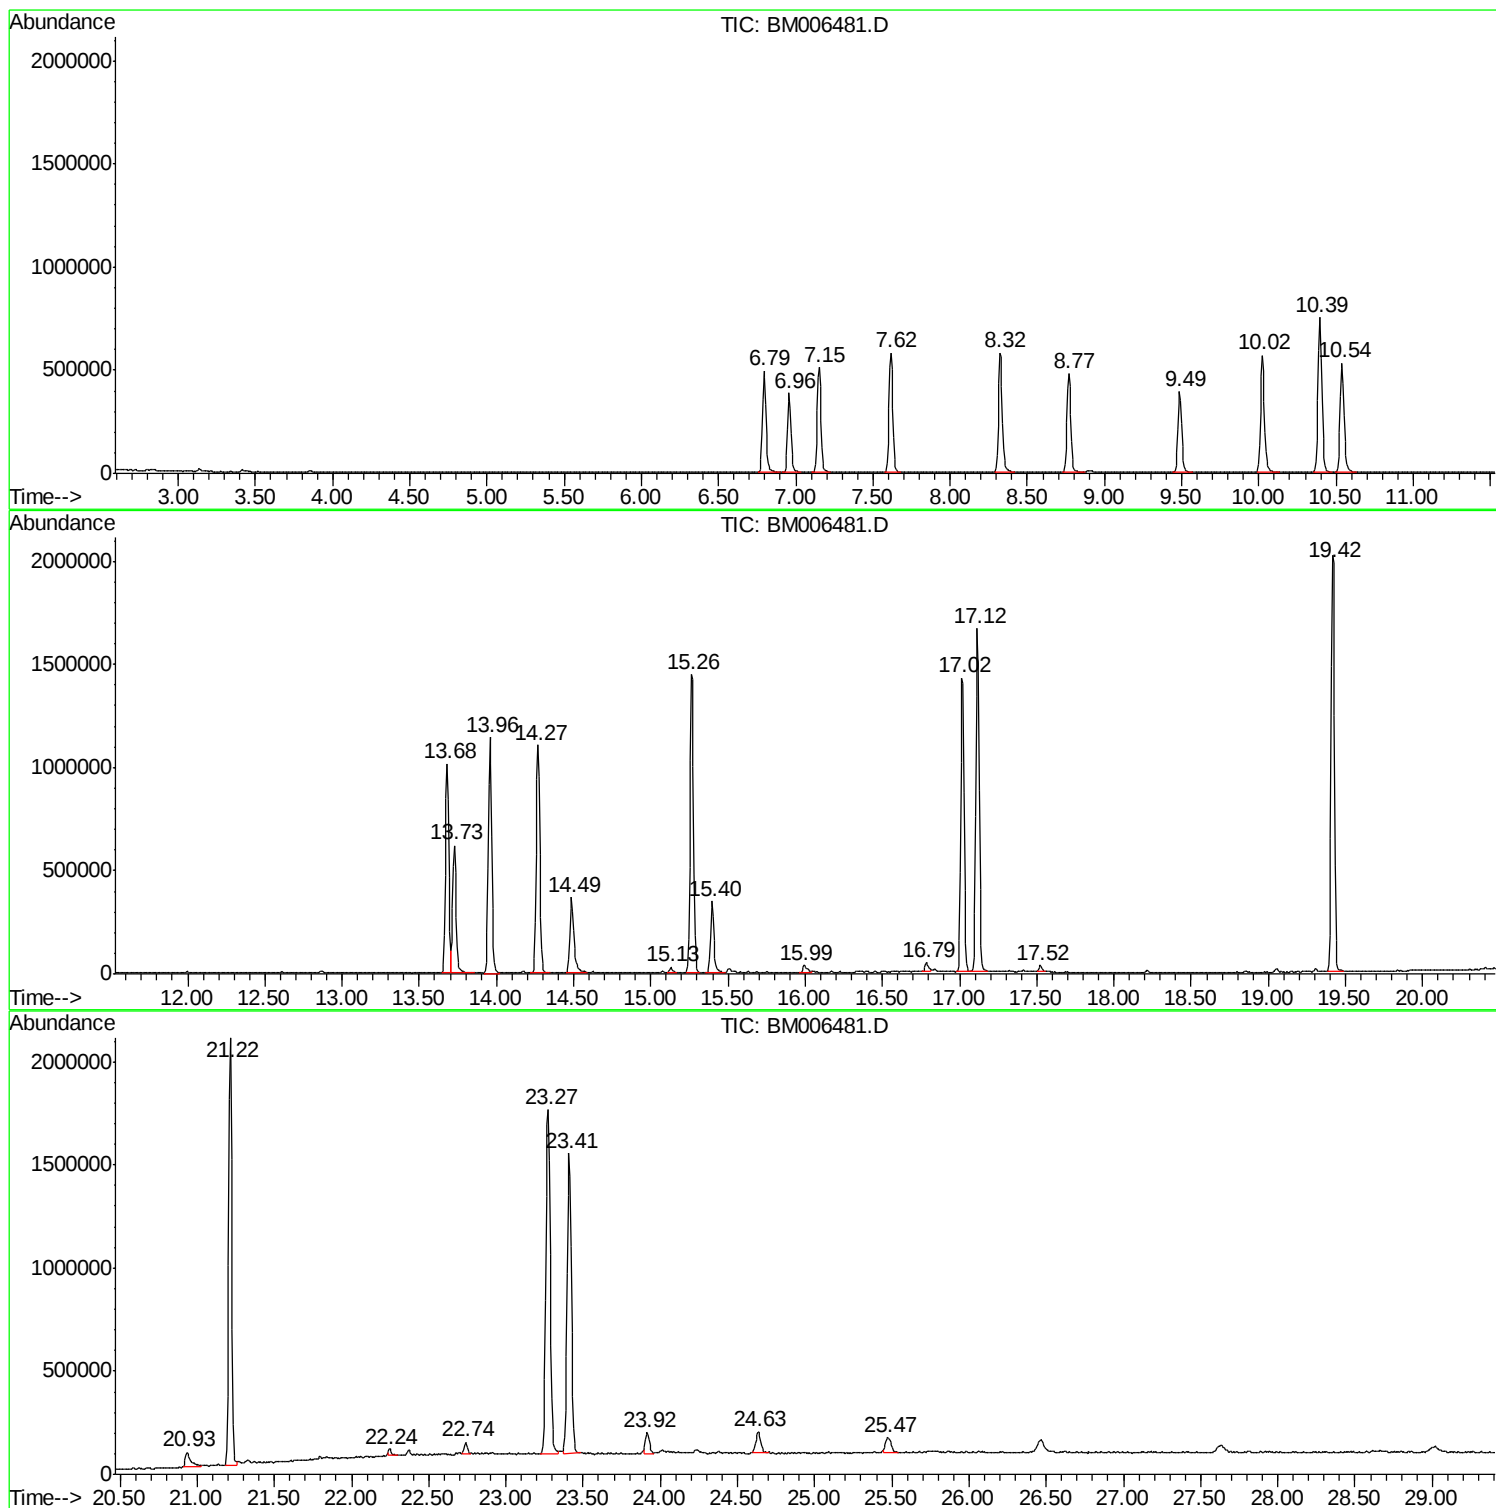

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006481.D
Acq On : 16 Jul 2016 16:22
Operator : UM/SJ
Sample : H3959-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ32

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM071616\
Data File : BM006481.D
Acq On : 16 Jul 2016 16:22
Operator : UM/SJ
Sample : H3959-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ32

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc