

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
 Data File : BM006504.D
 Acq On : 17 Jul 2016 07:32
 Operator : UM/SJ
 Sample : H3985-21
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.792	709	715	731	rVB	401134	667534	17.74%	1.742%
2	6.957	736	743	756	rBV	303673	489207	13.00%	1.277%
3	7.151	769	776	788	rBV	377119	628941	16.72%	1.641%
4	7.616	848	855	870	rBV	793300	1306728	34.73%	3.410%
5	8.322	969	975	987	rBV	484499	807736	21.47%	2.108%
6	8.769	1044	1051	1064	rBV	392810	659077	17.52%	1.720%
7	9.486	1166	1173	1189	rVB	306137	538133	14.30%	1.404%
8	10.022	1257	1264	1277	rBV	462318	819797	21.79%	2.140%
9	10.392	1319	1327	1342	rBV	976137	1736744	46.16%	4.533%
10	10.533	1344	1351	1364	rBV	456935	846929	22.51%	2.210%
11	13.680	1879	1886	1890	rBV	950616	1426809	37.93%	3.724%
12	13.721	1890	1893	1912	rVB	429513	655986	17.44%	1.712%
13	13.957	1926	1933	1945	rBV	1017890	1607653	42.73%	4.196%
14	14.262	1979	1985	1996	rBV2	1289737	2138812	56.85%	5.582%
15	14.480	2017	2022	2036	rBV	411292	748643	19.90%	1.954%
16	15.262	2149	2155	2166	rBV	1479501	2134514	56.74%	5.571%
17	15.392	2172	2177	2192	rBV	418514	630619	16.76%	1.646%
18	15.992	2274	2279	2286	rBV2	22849	40986	1.09%	0.107%
19	16.780	2410	2413	2421	rBV3	20621	40386	1.07%	0.105%
20	17.015	2447	2453	2463	rBV	1770047	2569278	68.29%	6.705%
21	17.115	2463	2470	2482	rVB2	1585788	2453772	65.22%	6.404%
22	19.080	2801	2804	2809	rVB	39271	48146	1.28%	0.126%
23	19.415	2855	2861	2875	rVB	2237563	3165361	84.14%	8.261%
24	20.939	3117	3120	3129	rBV9	23007	51493	1.37%	0.134%
25	21.215	3161	3167	3172	rBV	2722836	3641161	96.78%	9.503%
26	22.244	3339	3342	3346	rBV5	37117	52751	1.40%	0.138%
27	22.374	3360	3364	3369	rBV	101358	132707	3.53%	0.346%
28	22.744	3422	3427	3434	rBV4	72580	162936	4.33%	0.425%
29	23.274	3510	3517	3530	rVB2	1925877	3700773	98.37%	9.658%
30	23.415	3533	3541	3550	rVB2	1948805	3762151	100.00%	9.819%
31	23.915	3621	3626	3634	rVB	104936	210024	5.58%	0.548%
32	24.632	3743	3748	3757	rVB	109689	232879	6.19%	0.608%
33	25.479	3886	3892	3900	rVB5	77076	207915	5.53%	0.543%

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006504.D
Acq On : 17 Jul 2016 07:32
Operator : UM/SJ
Sample : H3985-21
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ58

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION


Sum of corrected areas: 38316581

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006504.D
Acq On : 17 Jul 2016 07:32
Operator : UM/SJ
Sample : H3985-21
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ58

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

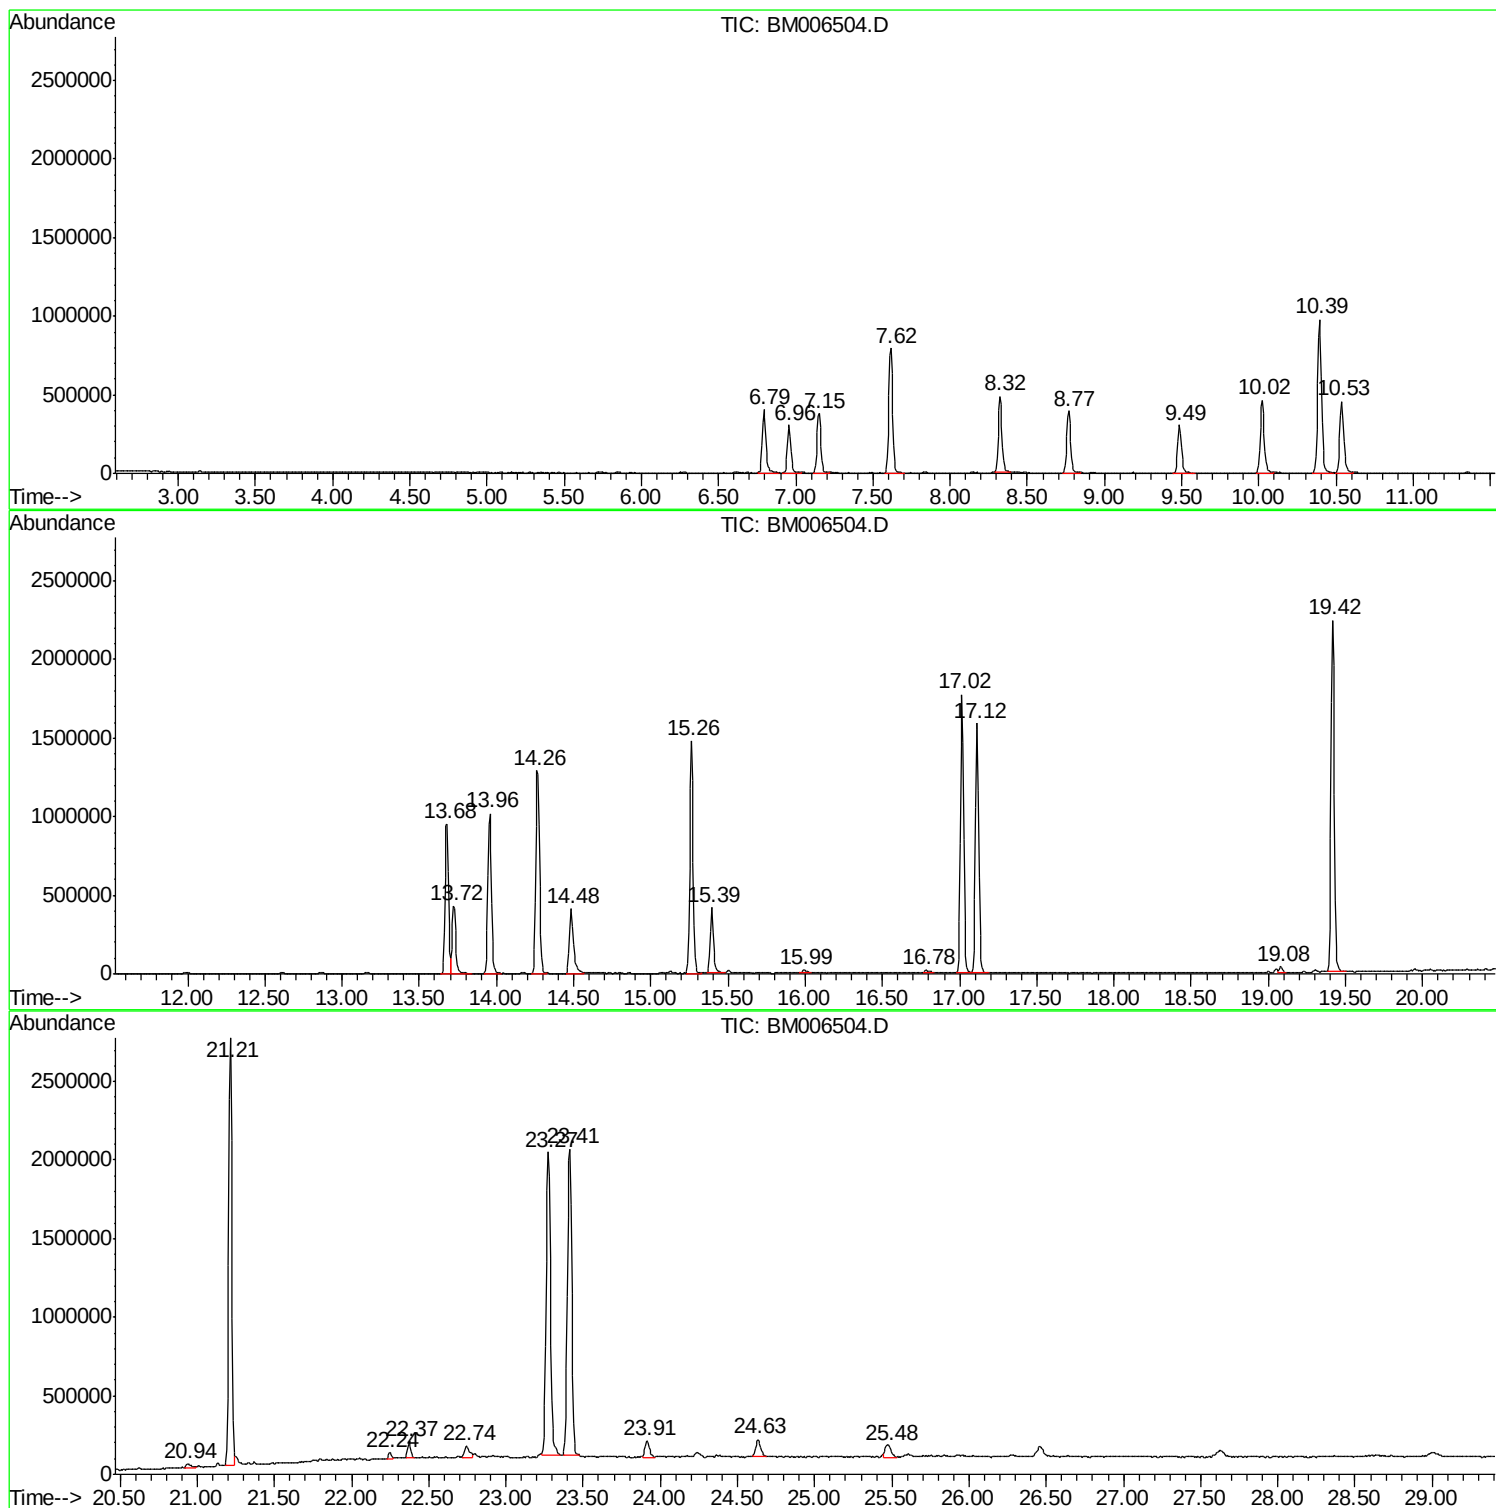

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006504.D
Acq On : 17 Jul 2016 07:32
Operator : UM/SJ
Sample : H3985-21
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ58

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006504.D
Acq On : 17 Jul 2016 07:32
Operator : UM/SJ
Sample : H3985-21
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ58

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc