

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
 Data File : BM006513.D
 Acq On : 17 Jul 2016 13:00
 Operator : UM/SJ
 Sample : H3985-22
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	706	715	732	rBV	912020	1542277	29.12%	2.746%
2	6.957	736	743	756	rBV	677555	1084672	20.48%	1.931%
3	7.151	769	776	787	rBV	879187	1469523	27.75%	2.616%
4	7.616	847	855	863	rBV	614333	1005397	18.98%	1.790%
5	8.322	963	975	990	rBV	1095631	1852224	34.97%	3.298%
6	8.769	1044	1051	1065	rBV	853651	1461242	27.59%	2.602%
7	9.487	1164	1173	1187	rBV	723138	1262700	23.84%	2.248%
8	10.022	1256	1264	1277	rBV	1006747	1792754	33.85%	3.192%
9	10.392	1318	1327	1334	rBV	828923	1441289	27.21%	2.566%
10	10.534	1344	1351	1364	rBV	923120	1706350	32.22%	3.038%
11	13.680	1878	1886	1890	rBV	1715940	2569804	48.52%	4.575%
12	13.727	1890	1894	1907	rVB	783503	1212852	22.90%	2.159%
13	13.957	1925	1933	1943	rBV	2005316	3191364	60.25%	5.682%
14	14.269	1979	1986	1993	rBV2	1112119	1805489	34.09%	3.215%
15	14.480	2016	2022	2033	rBV	773416	1375087	25.96%	2.448%
16	15.127	2128	2132	2139	rBV2	46238	66348	1.25%	0.118%
17	15.263	2149	2155	2162	rBV	2555112	3772034	71.22%	6.716%
18	15.398	2172	2178	2190	rBV	767482	1165167	22.00%	2.074%
19	15.992	2275	2279	2282	rBV2	74865	130836	2.47%	0.233%
20	16.780	2409	2413	2418	rBV2	56727	87720	1.66%	0.156%
21	16.833	2419	2422	2428	rVB2	38120	54440	1.03%	0.097%
22	17.015	2447	2453	2458	rBV	1485133	2187965	41.31%	3.896%
23	17.057	2458	2460	2464	rVV	152915	196928	3.72%	0.351%
24	17.115	2464	2470	2481	rVB	2768693	4200985	79.32%	7.480%
25	17.892	2598	2602	2606	rBV2	36318	54865	1.04%	0.098%
26	17.939	2606	2610	2616	rVB	45726	68606	1.30%	0.122%
27	18.021	2620	2624	2629	rVV	36392	61109	1.15%	0.109%
28	18.086	2629	2635	2639	rVV3	85490	171350	3.24%	0.305%
29	18.398	2684	2688	2693	rVB	34792	53615	1.01%	0.095%
30	18.815	2755	2759	2763	rBV2	50035	79424	1.50%	0.141%
31	19.080	2800	2804	2810	rVV	319062	424495	8.01%	0.756%
32	19.233	2826	2830	2835	rBV	56685	72478	1.37%	0.129%
33	19.304	2838	2842	2846	rVV2	40378	68603	1.30%	0.122%
34	19.356	2848	2851	2855	rVB3	43691	56174	1.06%	0.100%

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006513.D
Acq On : 17 Jul 2016 13:00
Operator : UM/SJ
Sample : H3985-22
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ59

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Title : SVOA CALIBRATION

35	19.415	2855	2861	2875	rBV2	3277719	5181948	97.84%	9.226%
36	19.768	2917	2921	2931	rBV4	49628	103481	1.95%	0.184%
37	19.945	2947	2951	2955	rVB2	118696	160853	3.04%	0.286%
38	20.045	2964	2968	2972	rVB	117736	143356	2.71%	0.255%
39	20.104	2975	2978	2983	rVB	54825	64279	1.21%	0.114%
40	20.933	3116	3119	3130	rVV4	115845	240124	4.53%	0.428%
41	21.215	3160	3167	3171	rBV	2156963	3163086	59.72%	5.632%
42	21.250	3171	3173	3180	rVB	260848	306700	5.79%	0.546%
43	21.368	3190	3193	3195	rBV2	51490	58084	1.10%	0.103%
44	22.750	3423	3428	3433	rBV2	180792	412725	7.79%	0.735%
45	23.221	3504	3508	3510	rBV	109659	169056	3.19%	0.301%
46	23.274	3510	3517	3530	rVB2	2537691	5296478	100.00%	9.430%
47	23.409	3533	3540	3547	rBV	1377573	2663598	50.29%	4.742%
48	23.909	3622	3625	3635	rVB2	107897	202862	3.83%	0.361%
49	24.633	3743	3748	3755	rVB	118244	253378	4.78%	0.451%


Sum of corrected areas: 56166174

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006513.D
Acq On : 17 Jul 2016 13:00
Operator : UM/SJ
Sample : H3985-22
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ59

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

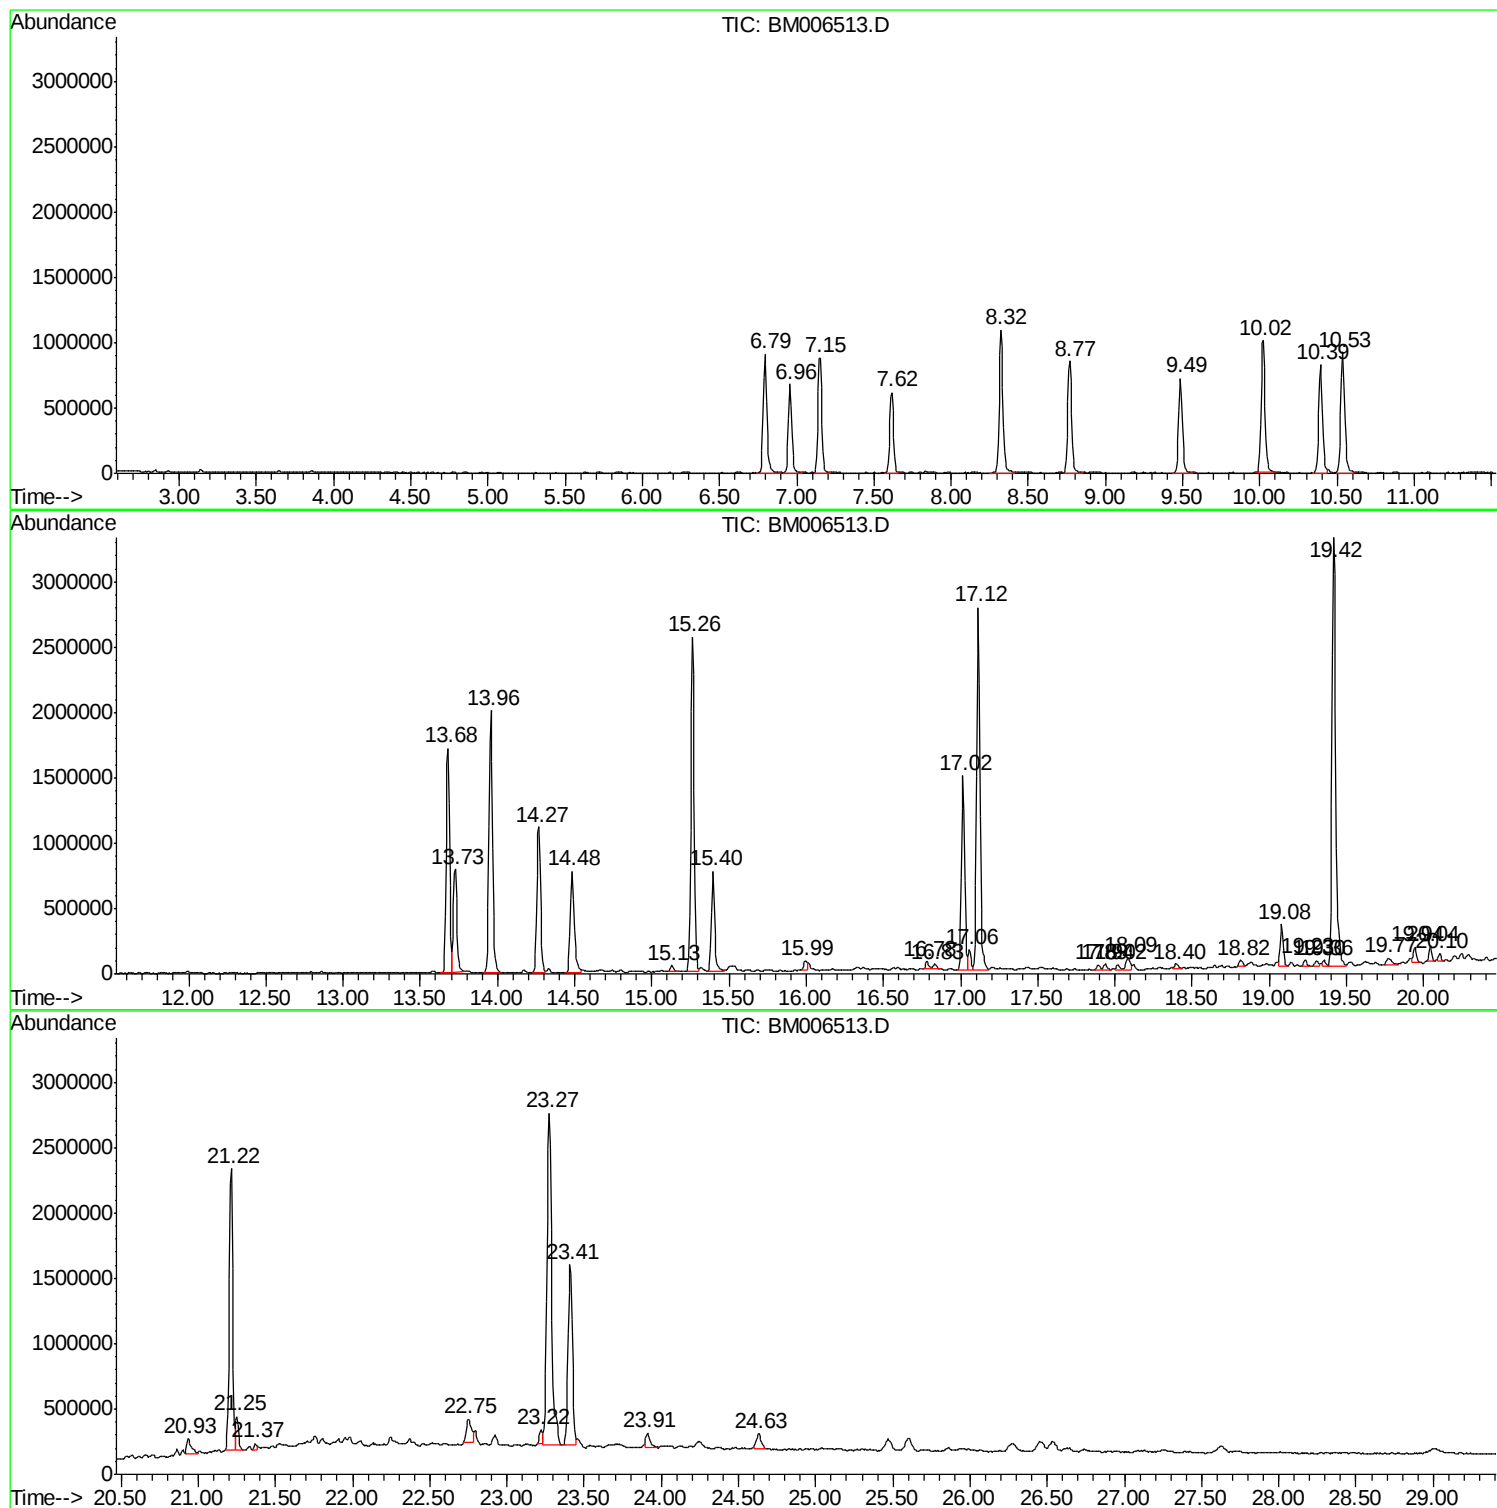

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006513.D
Acq On : 17 Jul 2016 13:00
Operator : UM/SJ
Sample : H3985-22
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ59

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM071616\
Data File : BM006513.D
Acq On : 17 Jul 2016 13:00
Operator : UM/SJ
Sample : H3985-22
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ59

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc