

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071717\
 Data File : BM010850.D
 Acq On : 18 Jul 2017 00:33
 Operator : SJ/JU
 Sample : I4203-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 NB-SB01B

Quant Time: Jul 18 05:42:55 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 14:21:16 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	197666	20.00	ng	-0.01
21) Naphthalene-d8	10.20	136	752115	20.00	ng	0.00
38) Acenaphthene-d10	14.09	164	505725	20.00	ng	0.00
63) Phenanthrene-d10	16.84	188	1268075	20.00	ng	0.00
75) Chrysene-d12	21.06	240	1475386	20.00	ng	0.00
86) Perylene-d12	23.19	264	1287919	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.08	112	1324632	111.01	ng	0.00
7) Phenol-d6	6.63	99	1788982	108.75	ng	0.00
23) Nitrobenzene-d5	8.59	82	1438392	73.51	ng	0.00
41) 2,4,6-Tribromophenol	15.59	330	867500	112.25	ng	0.00
44) 2-Fluorobiphenyl	12.70	172	2913258	71.66	ng	0.00
78) Terphenyl-d14	19.51	244	4885861	64.05	ng	0.00
Target Compounds						
10) Phenol	6.66	94	69707	4.008	ng	82
49) Dimethylphthalate	13.56	163	273981	6.368	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071717\
Data File : BM010850.D
Acq On : 18 Jul 2017 00:33
Operator : SJ/JU
Sample : I4203-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NB-SB01B

Quant Time: Jul 18 05:42:55 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

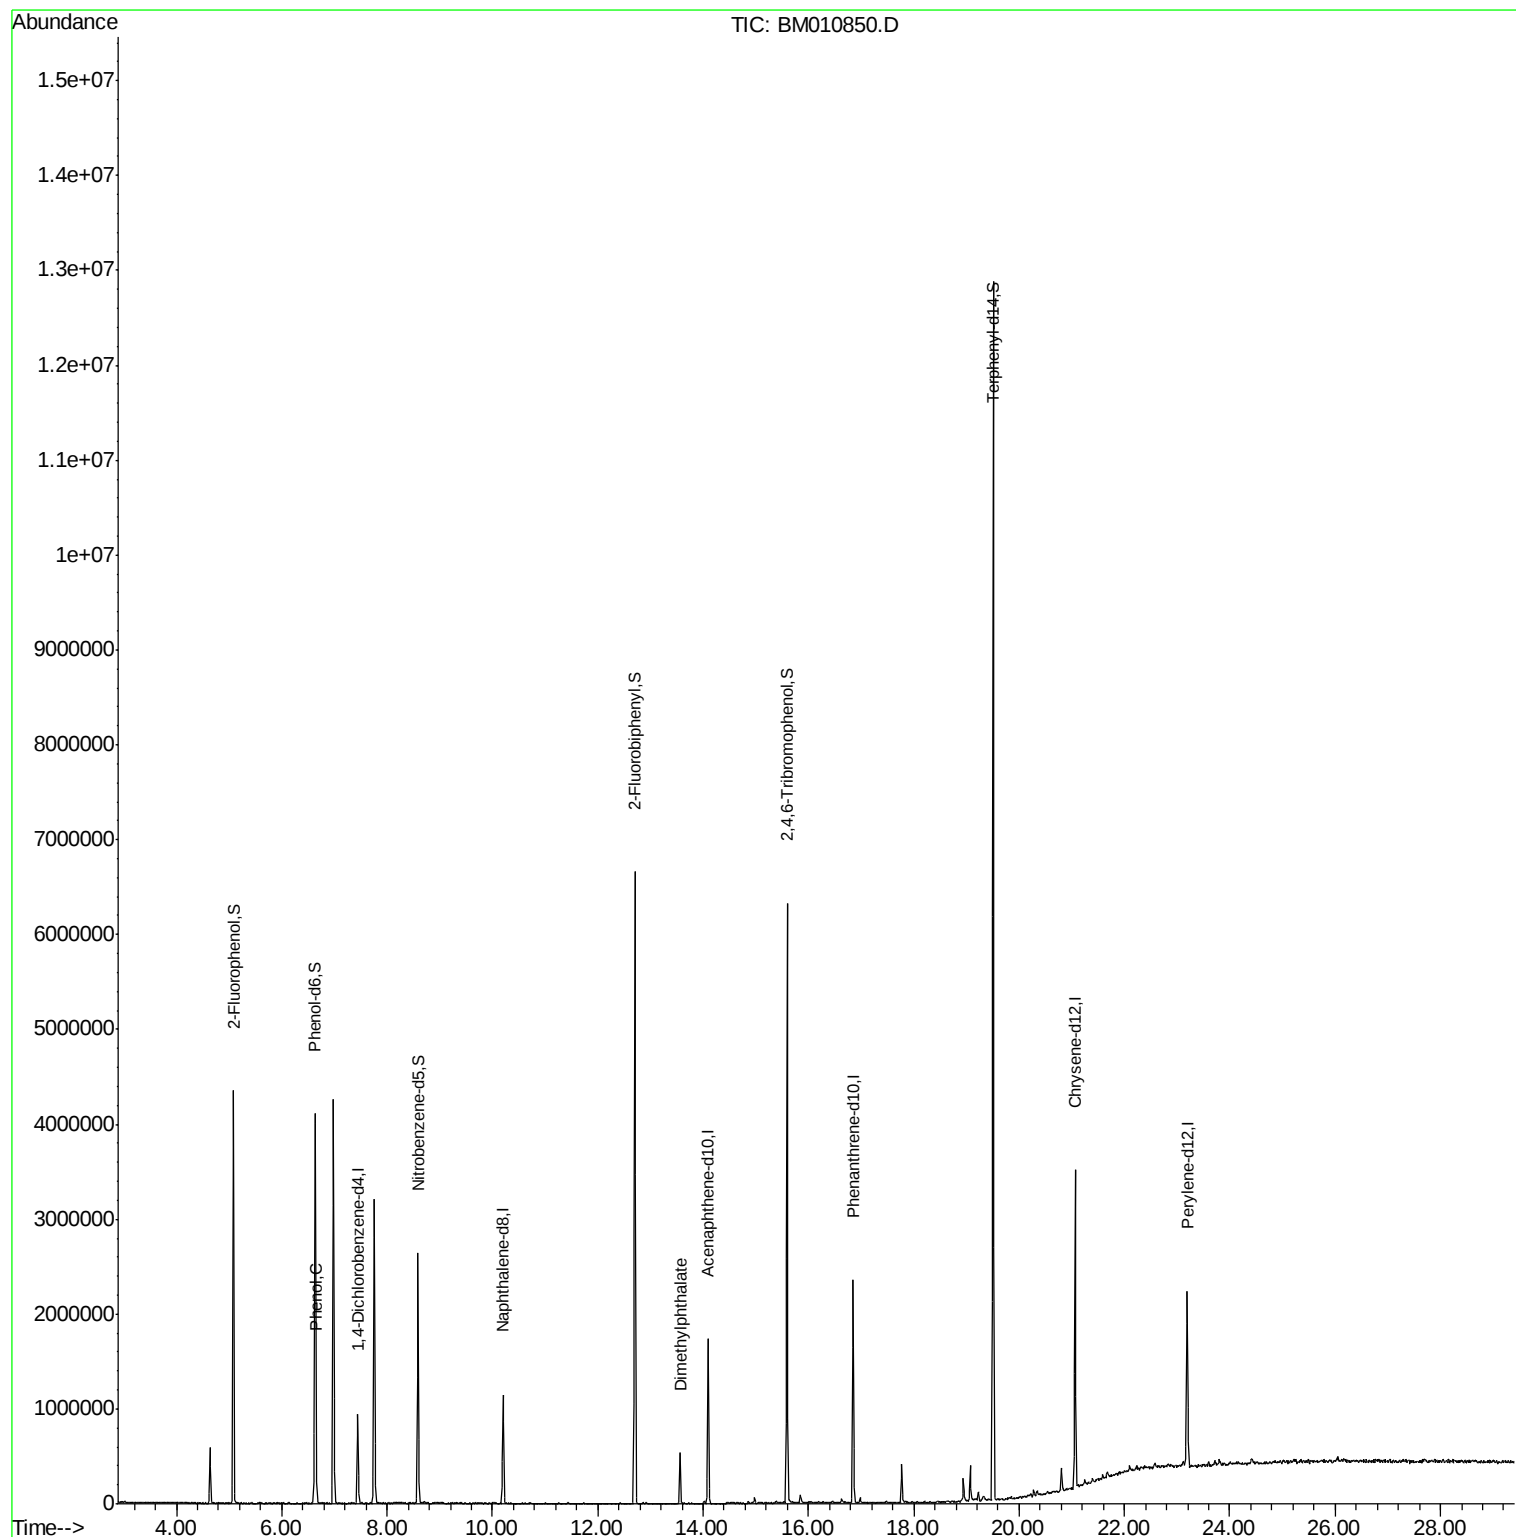







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.44 min Scan# 774
Delta R.T. -0.01 min
Lab File: BM010850.D
Acq: 18 Jul 2017 00:33

Instrument :
BNA_M
ClientSampleId :
NB-SB01B




Tot Ion:152 Resp: 197666
Ion Ratio Lower Upper
152 100
150 143.9 119.5 179.3
115 70.1 43.0 64.4#

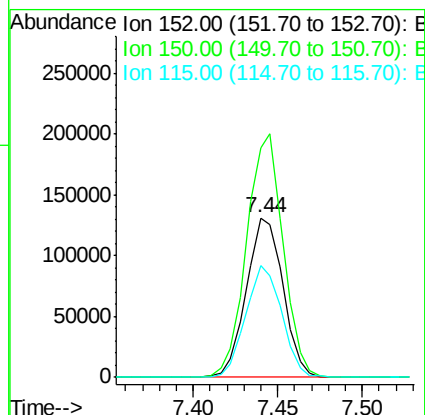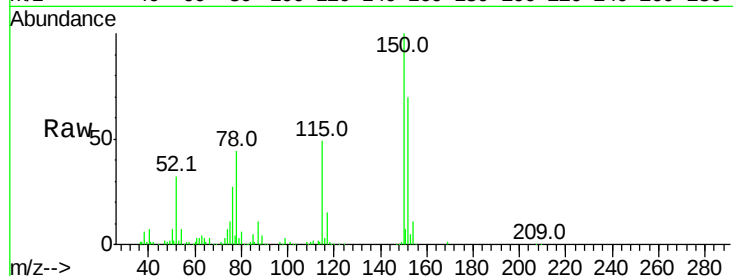


#5

2-Fluorophenol
Concen: 111.007 ng
RT: 5.08 min Scan# 373
Delta R.T. 0.00 min
Lab File: BM010850.D
Acq: 18 Jul 2017 00:33

Tgt Ion:112 Resp: 1324632
Ion Ratio Lower Upper
112 100
64 65.3 38.6 57.8#
63 43.9 19.3 28.9#

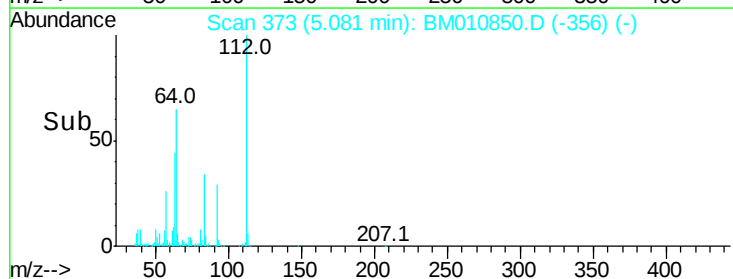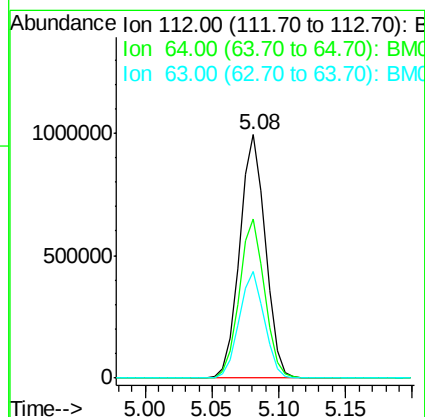



#7

Phenol-d6

Concen: 108.750 ng

RT: 6.63 min Scan# 637

Delta R.T. -0.01 min

Lab File: BM010850.D

Acq: 18 Jul 2017 00:33

Instrument :

BNA_M

ClientSampleId :

NB-SB01B





Tot Ion: 99 Resp: 1788982

Ion Ratio Lower Upper

99 100

42 25.5 11.0 16.4#

71 60.2 23.4 35.2#

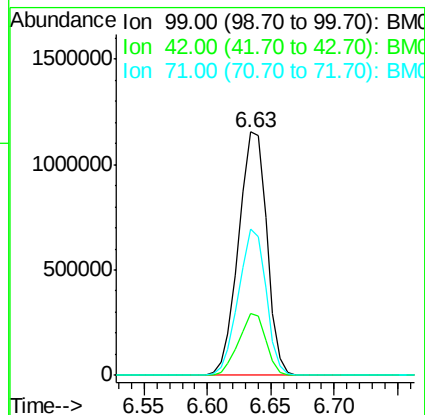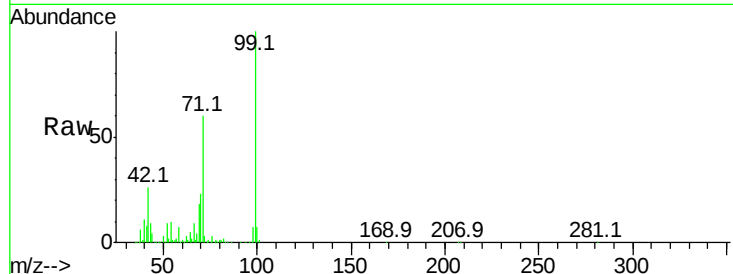

#10

Phenol

Concen: 4.008 ng

RT: 6.66 min Scan# 641

Delta R.T. -0.01 min

Lab File: BM010850.D

Acq: 18 Jul 2017 00:33




Tgt Ion: 94 Resp: 69707


Ion Ratio Lower Upper

94 100

65 45.1 18.8 58.8

66 77.6 39.9 79.9

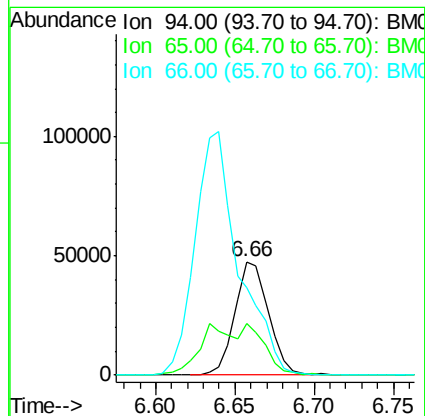


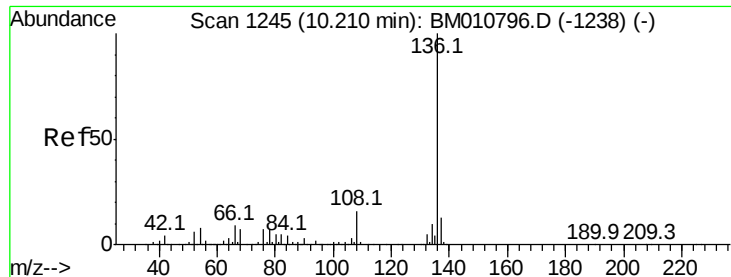




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.20 min Scan# 1244
Delta R.T. -0.01 min
Lab File: BM010850.D
Acq: 18 Jul 2017 00:33

Instrument :
BNA_M
ClientSampleId :
NB-SB01B

Tot Ion:136	Resp:	752115
Ion Ratio	Lower	Upper
136 100		
137 11.0	8.7	13.1
54 8.7	4.6	6.8#
68 5.6	3.7	5.5#

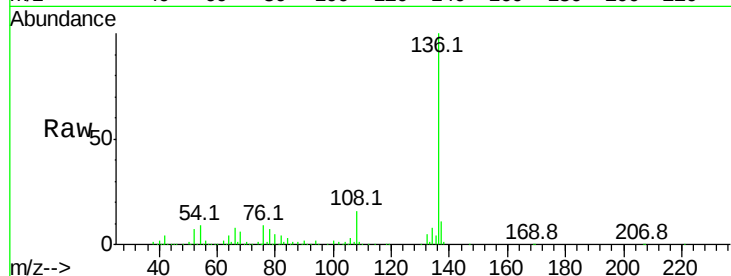


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

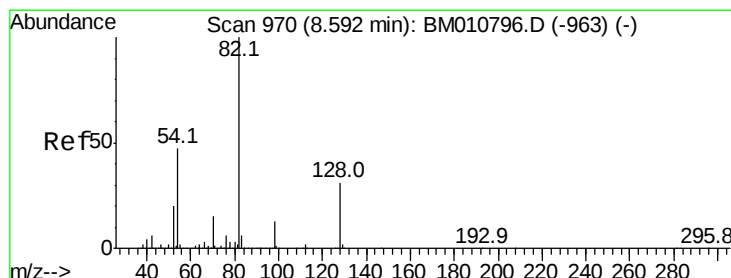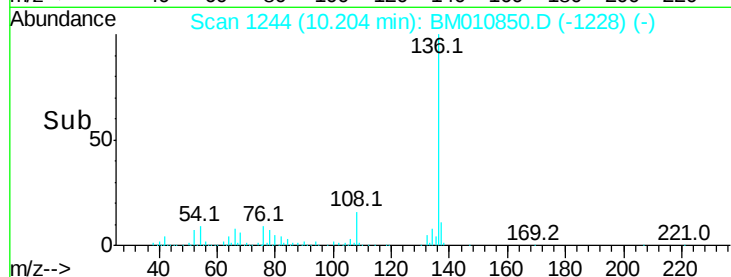
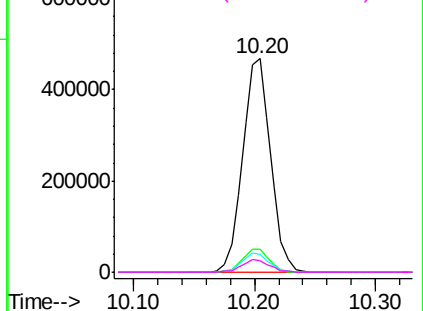



#23
Nitrobenzene-d5
Concen: 73.510 ng
RT: 8.59 min Scan# 969
Delta R.T. -0.01 min
Lab File: BM010850.D
Acq: 18 Jul 2017 00:33

Tgt Ion: 82	Resp: 1438392
Ion Ratio	Lower Upper
82 100	
128 29.4	32.8 49.2#
54 50.1	40.6 60.8

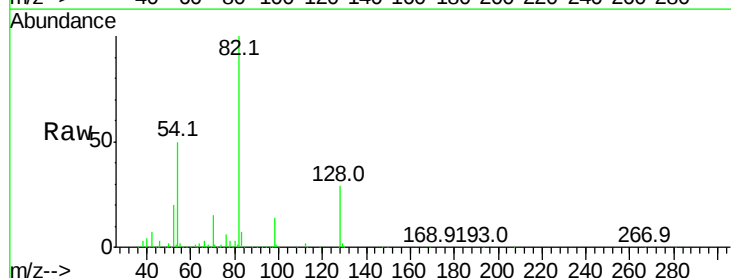

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

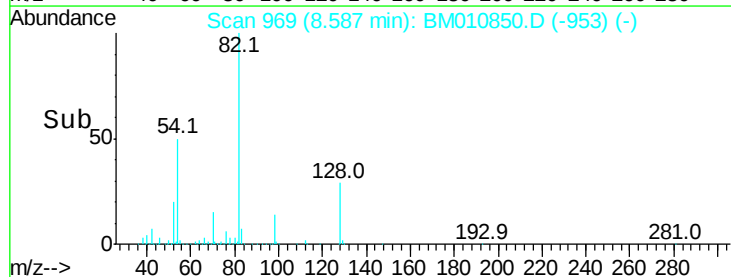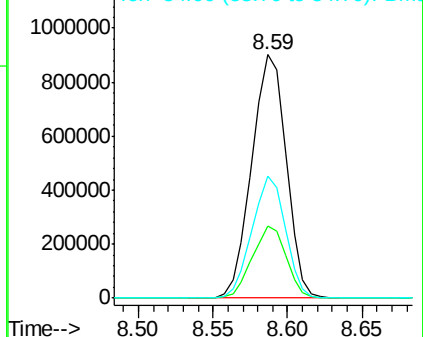

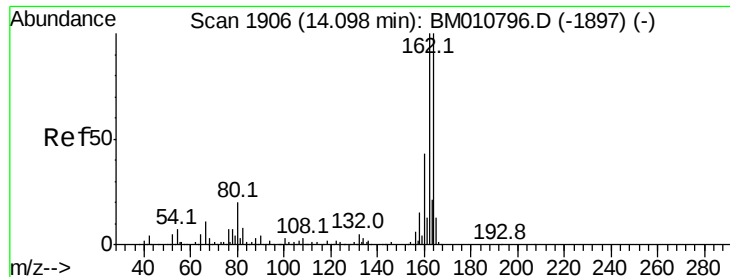

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.09 min Scan# 1905

Delta R.T. -0.01 min

Lab File: BM010850.D

Acq: 18 Jul 2017 00:33

Instrument :

BNA_M

ClientSampleId :

NB-SB01B


Tot Ion:164 Resp: 505725

Ion Ratio Lower Upper

164 100

162 105.7 82.4 123.6




160 40.2 35.8 53.6

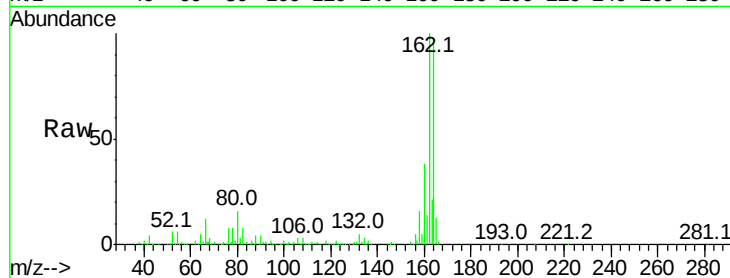

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

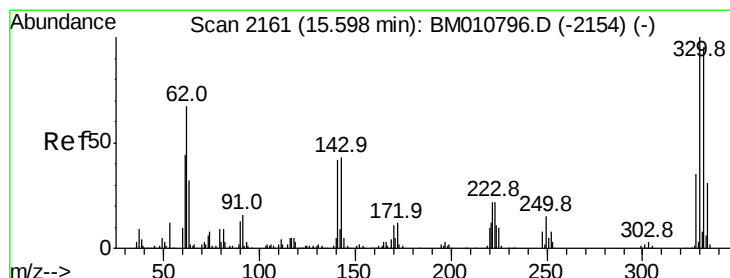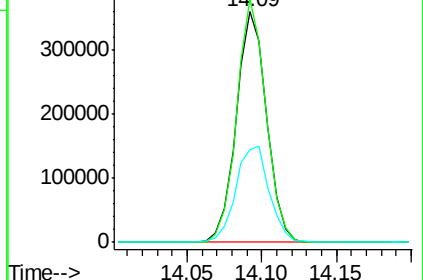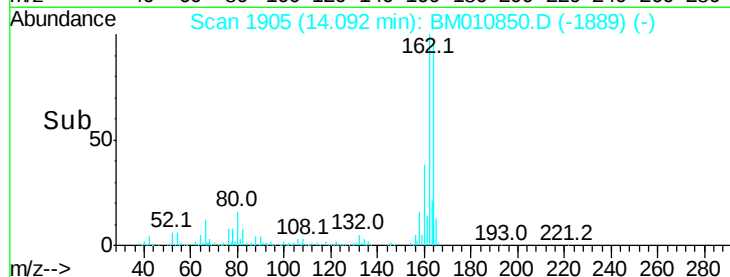

#41

2,4,6-Tribromophenol

Concen: 112.248 ng

RT: 15.59 min Scan# 2160

Delta R.T. -0.01 min

Lab File: BM010850.D

Acq: 18 Jul 2017 00:33


Tgt Ion:330 Resp: 867500

Ion Ratio Lower Upper

330 100

332 95.3 0.0 0.0#



141 44.8 0.0 0.0#

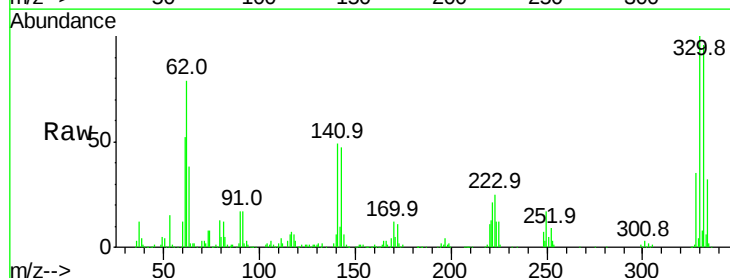


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



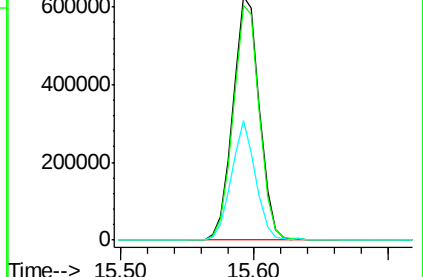
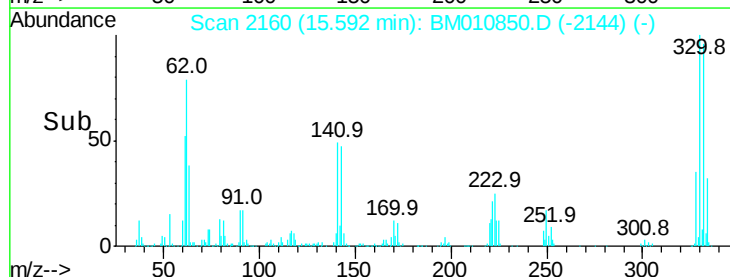




#44
2-Fluorobiphenyl
Concen: 71.663 ng
RT: 12.70 min Scan# 1669
Delta R.T. -0.01 min
Lab File: BM010850.D
Acq: 18 Jul 2017 00:33




Instrument :
BNA_M
ClientSampleId :
NB-SB01B


Tot Ion:172 Resp: 2913258
Ion Ratio Lower Upper
172 100
171 34.3 28.5 42.7
170 22.7 18.8 28.2

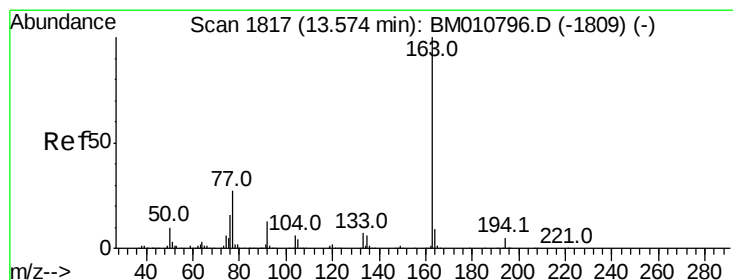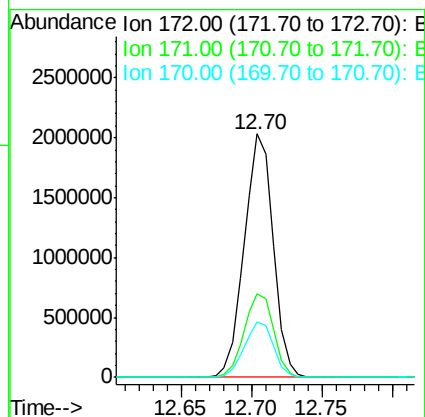

#49
Dimethylphthalate
Concen: 6.368 ng
RT: 13.56 min Scan# 1815
Delta R.T. -0.01 min
Lab File: BM010850.D
Acq: 18 Jul 2017 00:33

Tgt Ion:163 Resp: 273981
Ion Ratio Lower Upper
163 100
194 4.6 2.7 4.1#
164 9.8 8.2 12.2

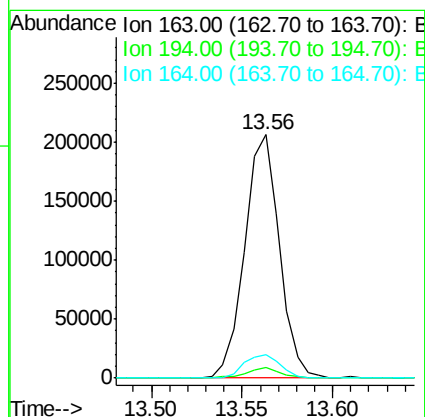



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.84 min Scan# 2373

Delta R.T. -0.01 min

Lab File: BM010850.D

Acq: 18 Jul 2017 00:33

Instrument :

BNA_M

ClientSampleId :

NB-SB01B


Tot Ion:188 Resp: 1268075

Ion Ratio Lower Upper

188 100

94 6.6 8.7 13.1#




80 7.7 9.3 13.9#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

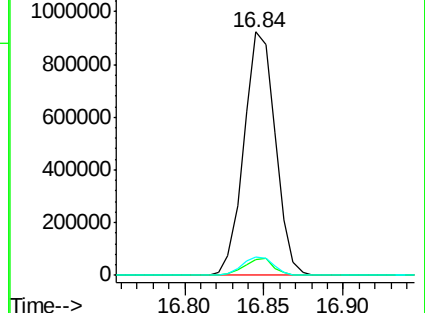

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.06 min Scan# 3090

Delta R.T. -0.01 min

Lab File: BM010850.D

Acq: 18 Jul 2017 00:33


Tgt Ion:240 Resp: 1475386

Ion Ratio Lower Upper

240 100

120 4.6 8.2 12.2#



236 24.9 20.0 30.0




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

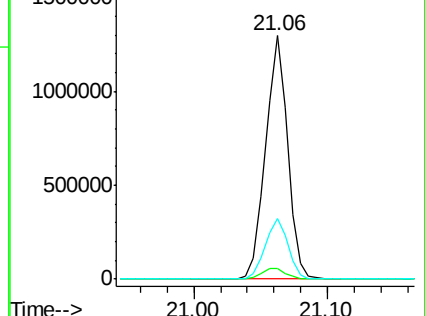



#78

Terphenyl-d14

Concen: 64.049 ng

RT: 19.51 min Scan# 2826

Delta R.T. 0.00 min

Lab File: BM010850.D

Acq: 18 Jul 2017 00:33

Instrument :

BNA_M

ClientSampleId :

NB-SB01B


Tot Ion:244 Resp: 4885861

Ion Ratio Lower Upper

244 100

212 8.9 4.9 7.3#




122 6.6 6.2 9.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

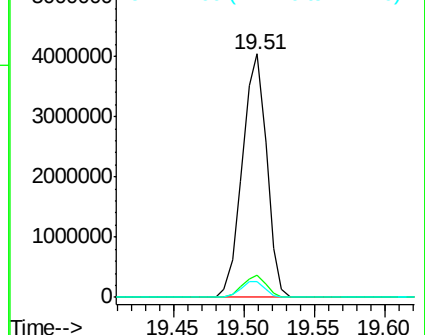

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.19 min Scan# 3452

Delta R.T. -0.01 min

Lab File: BM010850.D

Acq: 18 Jul 2017 00:33


Tgt Ion:264 Resp: 1287919

Ion Ratio Lower Upper

264 100

260 22.8 18.6 27.8

265 22.1 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

