


Data Path : Z:\HPCHEM1\BNA M\Data\BM071717\
 Data File : BM010838.D
 Acq On : 17 Jul 2017 14:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

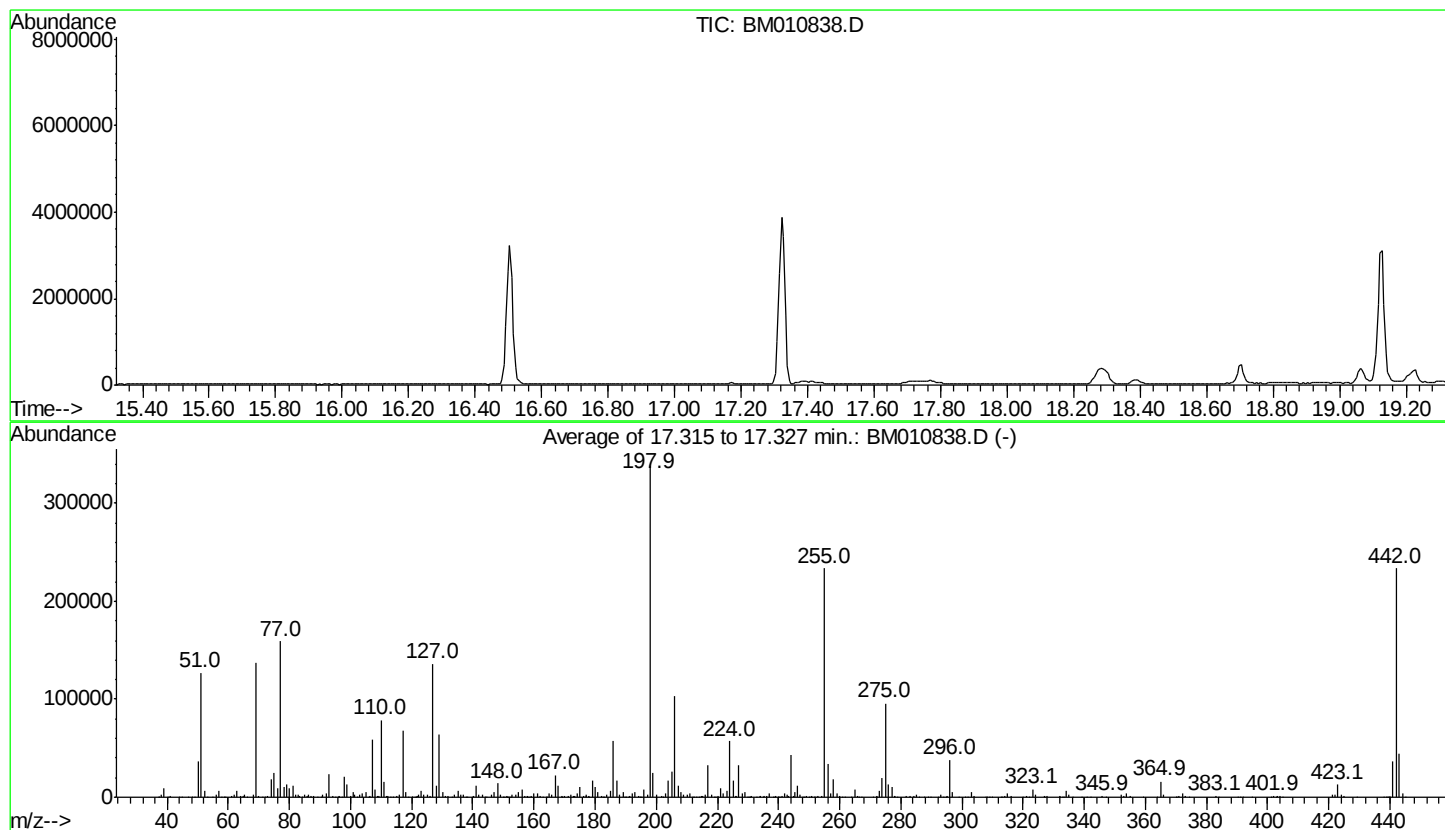

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	126812	PASS
68	69	0.00	2	1.9	2572	PASS
69	198	0.00	100	40.4	136621	PASS
70	69	0.00	2	0.9	1198	PASS
127	198	10	80	40.3	136296	PASS
197	198	0.00	2	0.8	2874	PASS
198	198	100	100	100.0	338346	PASS
199	198	5	9	7.4	25088	PASS
275	198	10	60	28.4	95984	PASS
365	198	1	100	4.7	15751	PASS
441	443	0.01	100	82.9	36421	PASS
442	198	50	100	68.9	233216	PASS
443	442	15	24	18.8	43944	PASS