


Data Path : Z:\HPCHEM1\BNA M\Data\BM071717\
 Data File : BM010842.D
 Acq On : 17 Jul 2017 19:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

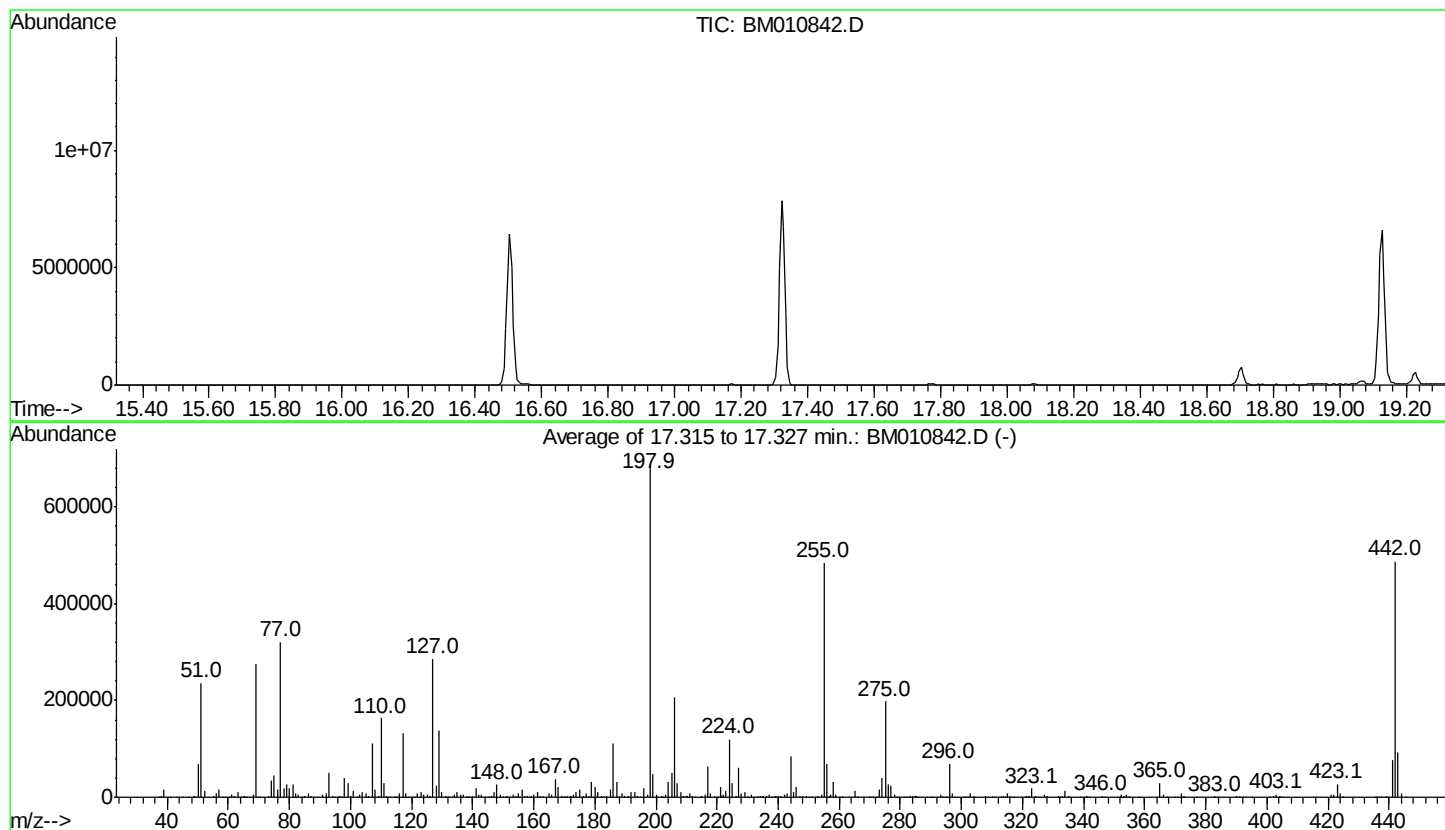

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	236309	PASS
68	69	0.00	2	2.0	5418	PASS
69	198	0.00	100	40.2	275392	PASS
70	69	0.00	2	0.3	691	PASS
127	198	10	80	41.8	286506	PASS
197	198	0.00	2	0.8	5417	PASS
198	198	100	100	100.0	684906	PASS
199	198	5	9	6.9	47349	PASS
275	198	10	60	28.9	198101	PASS
365	198	1	100	4.4	30352	PASS
441	443	0.01	100	82.7	77170	PASS
442	198	50	100	71.2	487381	PASS
443	442	15	24	19.2	93344	PASS