

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071816\
 Data File : BM006517.D
 Acq On : 18 Jul 2016 11:43
 Operator : UM/SJ
 Sample : H3985-19
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJ56

Quant Time: Jul 19 02:05:41 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 02:05:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	139120	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	584188	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	325326	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	749590	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	928795	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	981235	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	6334	1.92	ng/uL	0.00
5) Phenol-d5	6.79	99	255664	22.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	165202	23.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	202762	21.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	207105	22.86	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	94823	21.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	100505	20.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	185585	19.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	258949	26.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	601148	22.58	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	732672	22.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	72657	15.71	ng/ul	0.00
57) Fluorene-d10	15.26	176	529397	22.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	58537	13.50	ng/ul	0.00
70) Anthracene-d10	17.12	188	855440	24.14	ng/ul	0.00
76) Pyrene-d10	19.42	212	1011192	24.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1135039	25.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.73	163	240066	8.89	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071816\
Data File : BM006517.D
Acq On : 18 Jul 2016 11:43
Operator : UM/SJ
Sample : H3985-19
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJ56

Quant Time: Jul 19 02:05:41 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM071416.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 02:05:48 2016
Response via : Initial Calibration

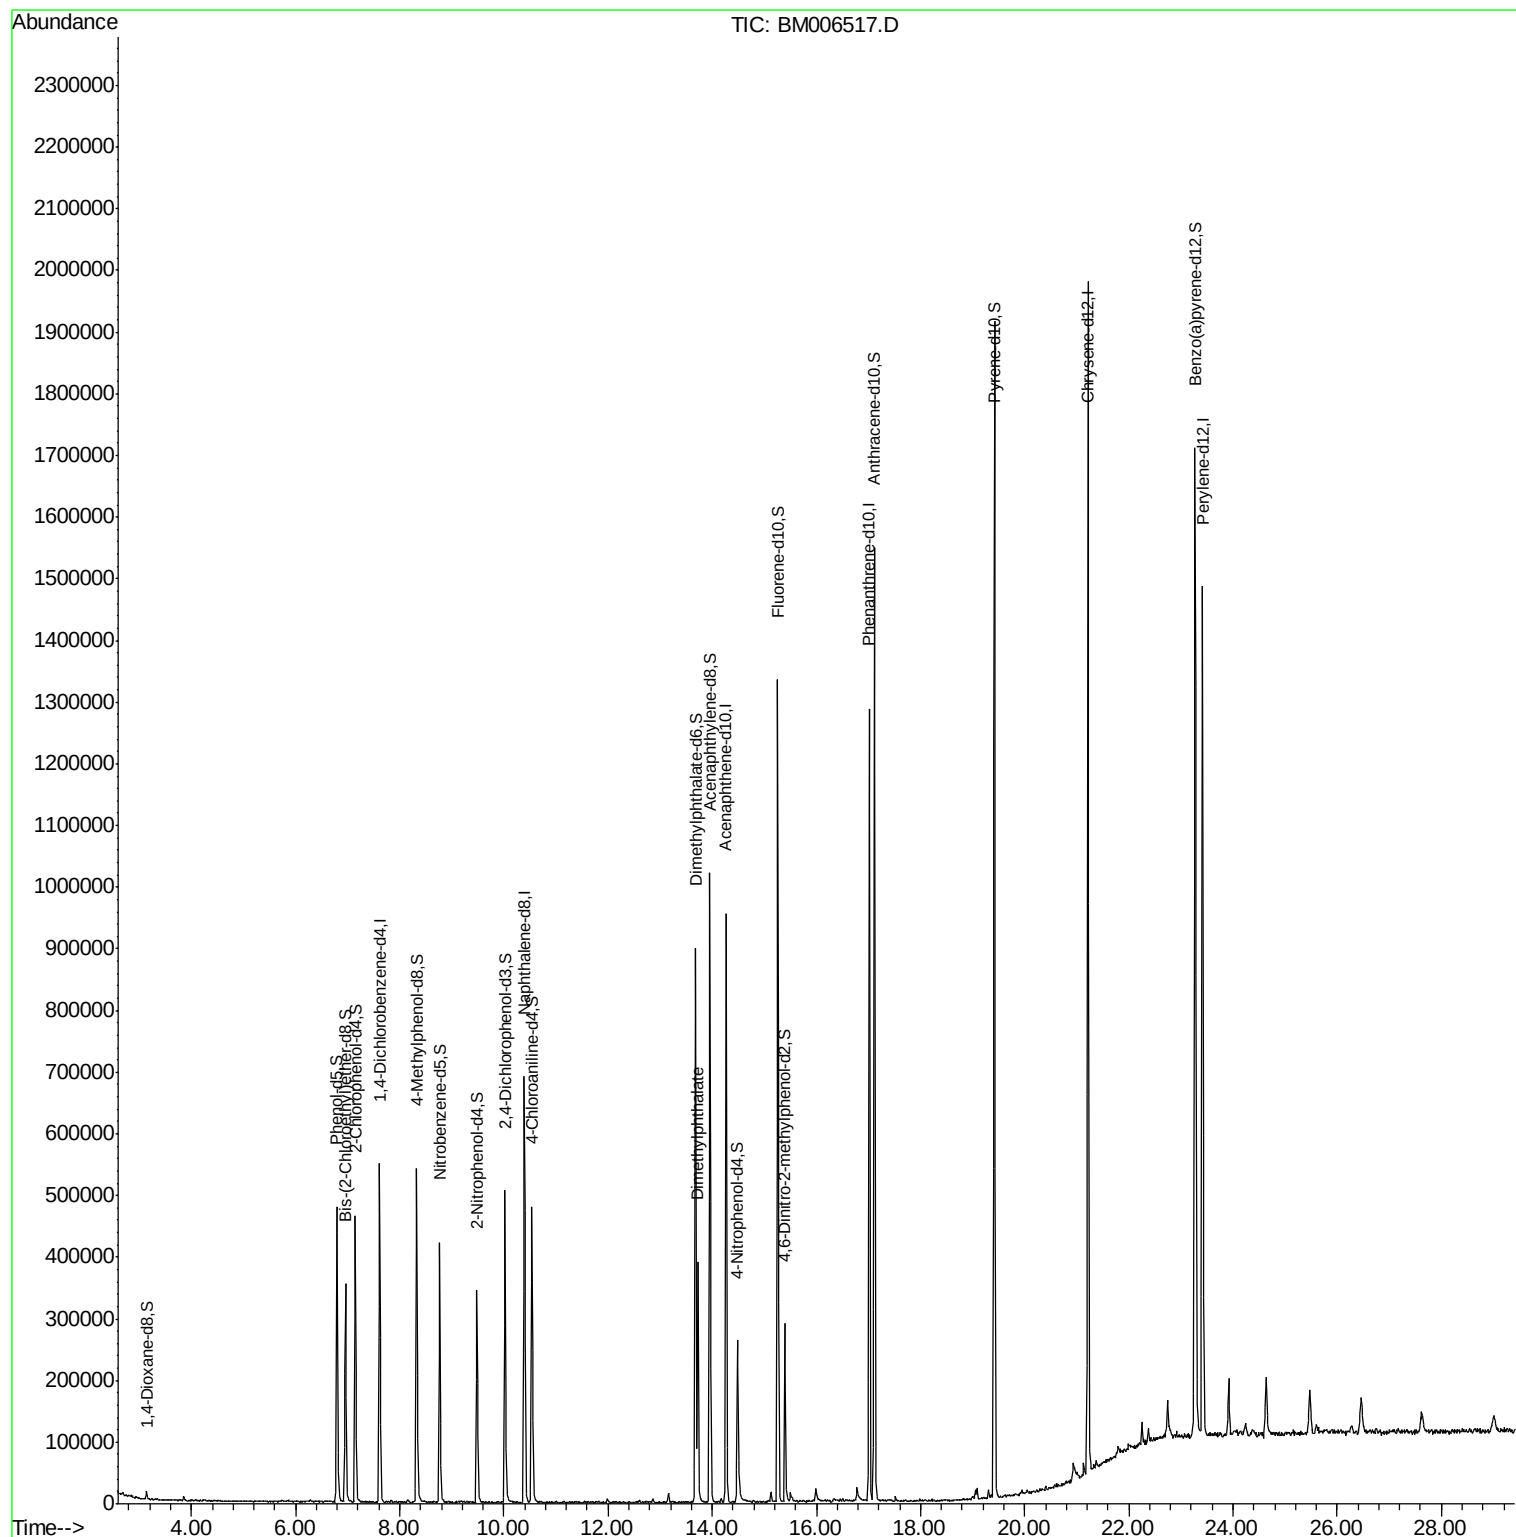

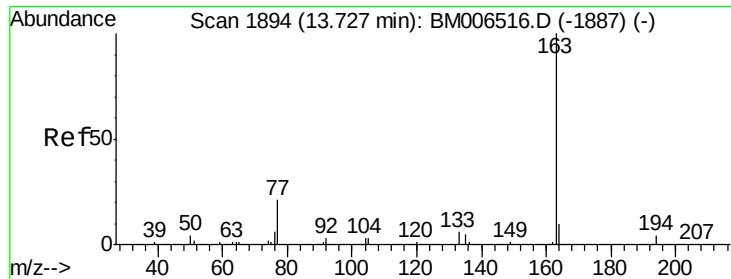

#44

Dimethylphthalate

Concen: 8.89 ng/ul

RT: 13.73 min Scan# 1894

Delta R.T. 0.00 min

Lab File: BM006517.D

Acq: 18 Jul 2016 11:43

Instrument :

BNA_M

ClientSampleId :

BDJ56


Tot Ion:163 Resp: 240066

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 10.1 7.8 11.8

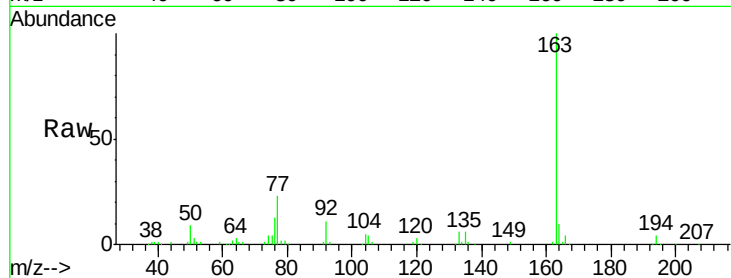

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

